

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
 Data File : FF007896.D
 Signal(s) : FID2B.ch
 Acq On : 18 Nov 2020 15:53
 Operator : DD\AJ
 Sample : L4784-10
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 19 00:17:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.714	2763972	21.638 ug/ml
Target Compounds			
3) N-DODECANE	6.459	226889	1.639 ug/ml
4) N-TETRADECANE	8.258	224304	1.588 ug/ml
5) N-HEXADECANE	9.859	295804	2.035 ug/ml
6) N-OCTADECANE	11.325	288734	1.946 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
Data File : FF007896.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2020 15:53
Operator : DD\AJ
Sample : L4784-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 19 00:17:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

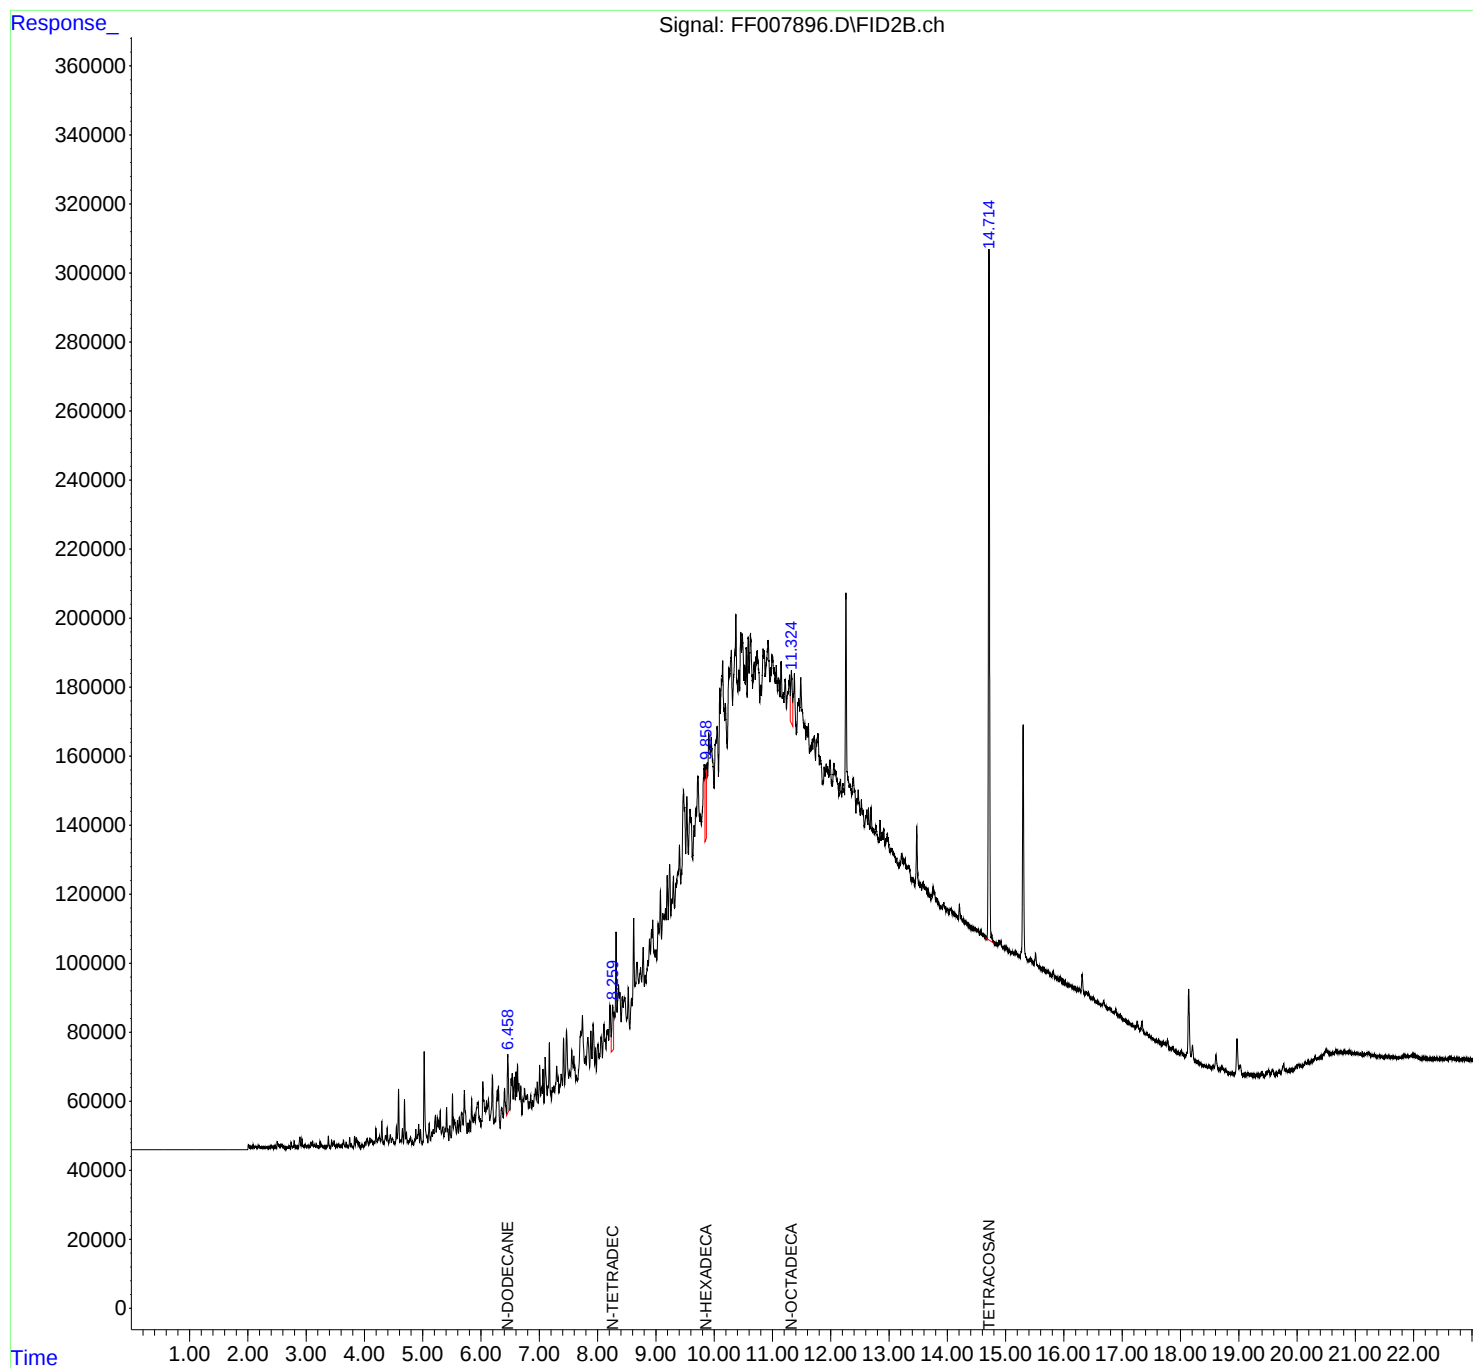


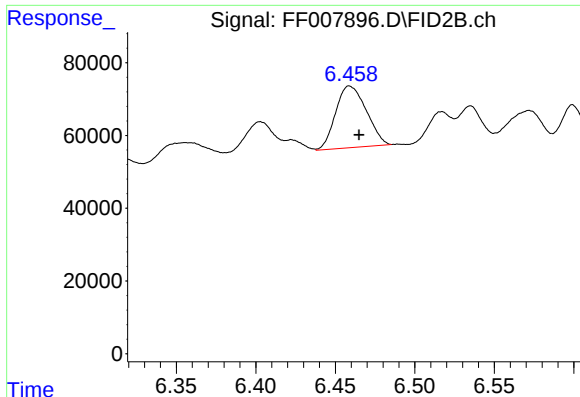

#3 N-DODECANE


R.T.: 6.459 min
Delta R.T.: -0.006 min
Response: 226889
Conc: 1.64 ug/ml

Instrument :
FID_F
ClientSampleId :

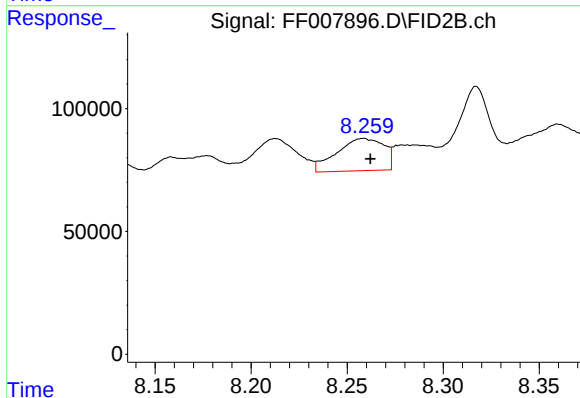


#4 N-TETRADECANE

R.T.: 8.258 min
Delta R.T.: -0.004 min
Response: 224304
Conc: 1.59 ug/ml

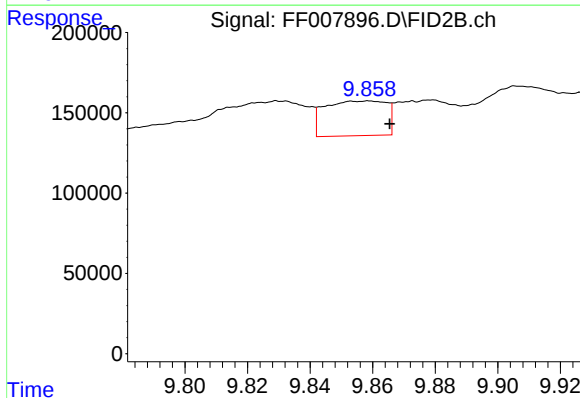


#5 N-HEXADECANE

R.T.: 9.859 min
Delta R.T.: -0.007 min
Response: 295804
Conc: 2.04 ug/ml

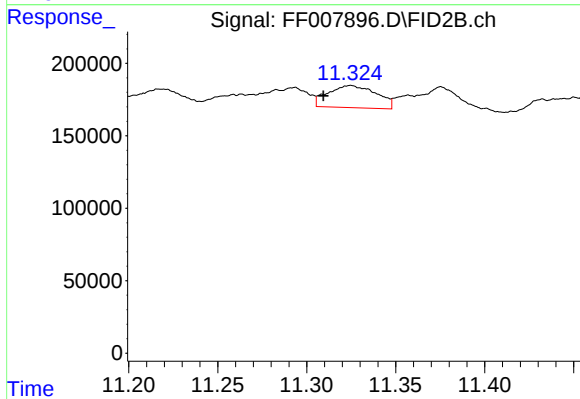

#6 N-OCTADECANE

R.T.: 11.325 min
Delta R.T.: 0.015 min
Response: 288734
Conc: 1.95 ug/ml

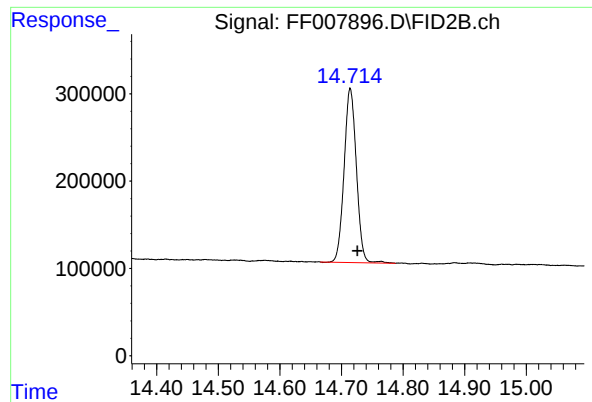

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.714 min
Delta R.T.: -0.011 min
Response: 2763972
Conc: 21.64 ug/ml

Instrument :
FID_F
ClientSampleId :