

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
 Data File : FF007898.D
 Signal(s) : FID2B.ch
 Acq On : 18 Nov 2020 16:55
 Operator : DD\AJ
 Sample : L4784-06 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 19 00:17:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	1111394	8.701 ug/ml
Target Compounds			
3) N-DODECANE	6.449	133964	0.968 ug/ml
4) N-TETRADECANE	8.216	93479	0.662 ug/ml
6) N-OCTADECANE	11.354	167179	1.126 ug/ml
14) N-DOTRIACONTANE	18.613	137611	1.187 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
Data File : FF007898.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2020 16:55
Operator : DD\AJ
Sample : L4784-06 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 19 00:17:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

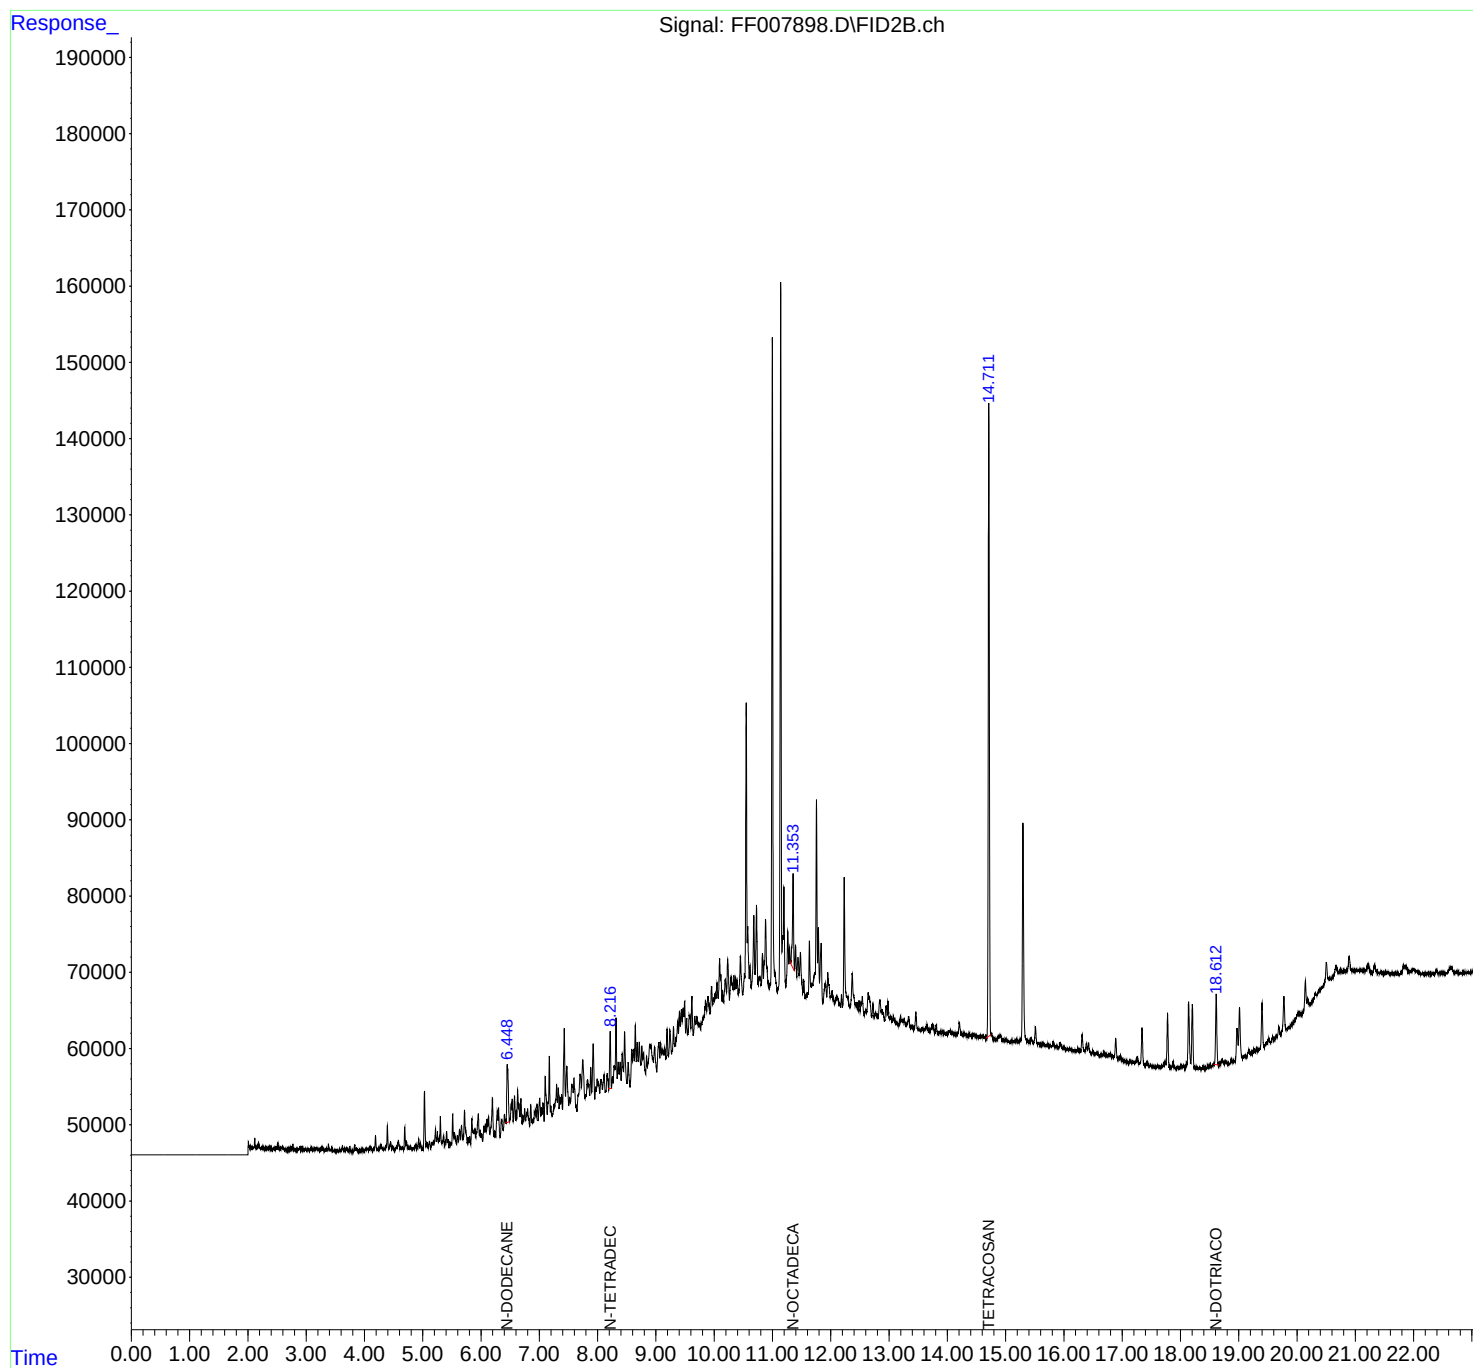


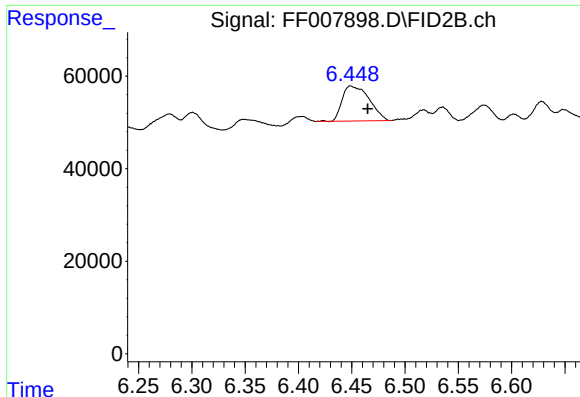

#3 N-DODECANE


R.T.: 6.449 min
Delta R.T.: -0.016 min
Response: 133964
Conc: 0.97 ug/ml

Instrument :
FID_F
ClientSampleId :

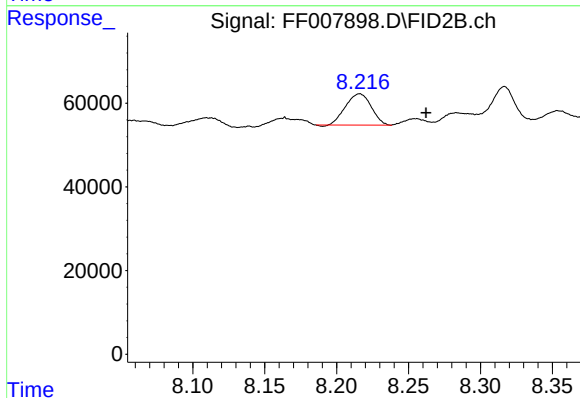


#4 N-TETRADECANE

R.T.: 8.216 min
Delta R.T.: -0.046 min
Response: 93479
Conc: 0.66 ug/ml

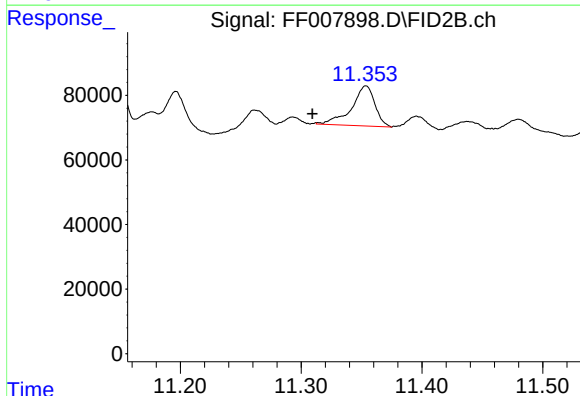


#6 N-OCTADECANE

R.T.: 11.354 min
Delta R.T.: 0.044 min
Response: 167179
Conc: 1.13 ug/ml

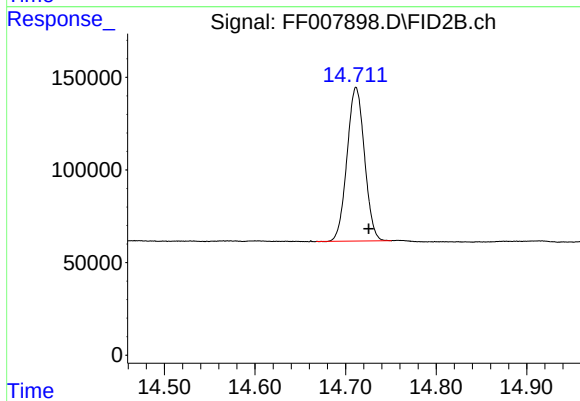

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: -0.014 min
Response: 1111394
Conc: 8.70 ug/ml

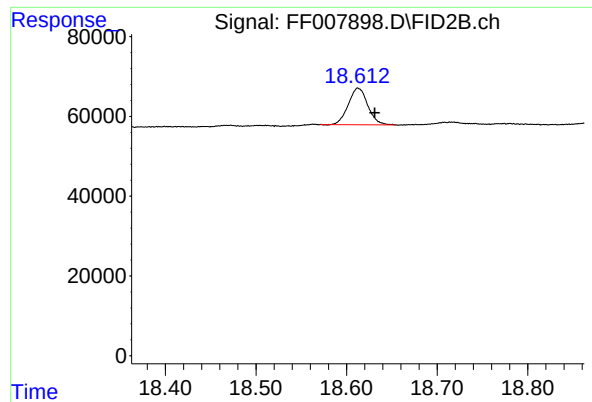

#14 N-DOTRIACONTANE

R.T.: 18.613 min
Delta R.T.: -0.019 min
Response: 137611
Conc: 1.19 ug/ml

Instrument :
FID_F
ClientSampleId :