

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
Data File : FF007894.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2020 14:51
Operator : DD\AJ
Sample : L4784-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSIMW-1-20201117

Integration File: autoint1.e
Quant Time: Nov 19 00:16:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	2481713	19.429 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111820\
Data File : FF007894.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2020 14:51
Operator : DD\AJ
Sample : L4784-08
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CSIMW-1-20201117

Integration File: autoint1.e
Quant Time: Nov 19 00:16:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

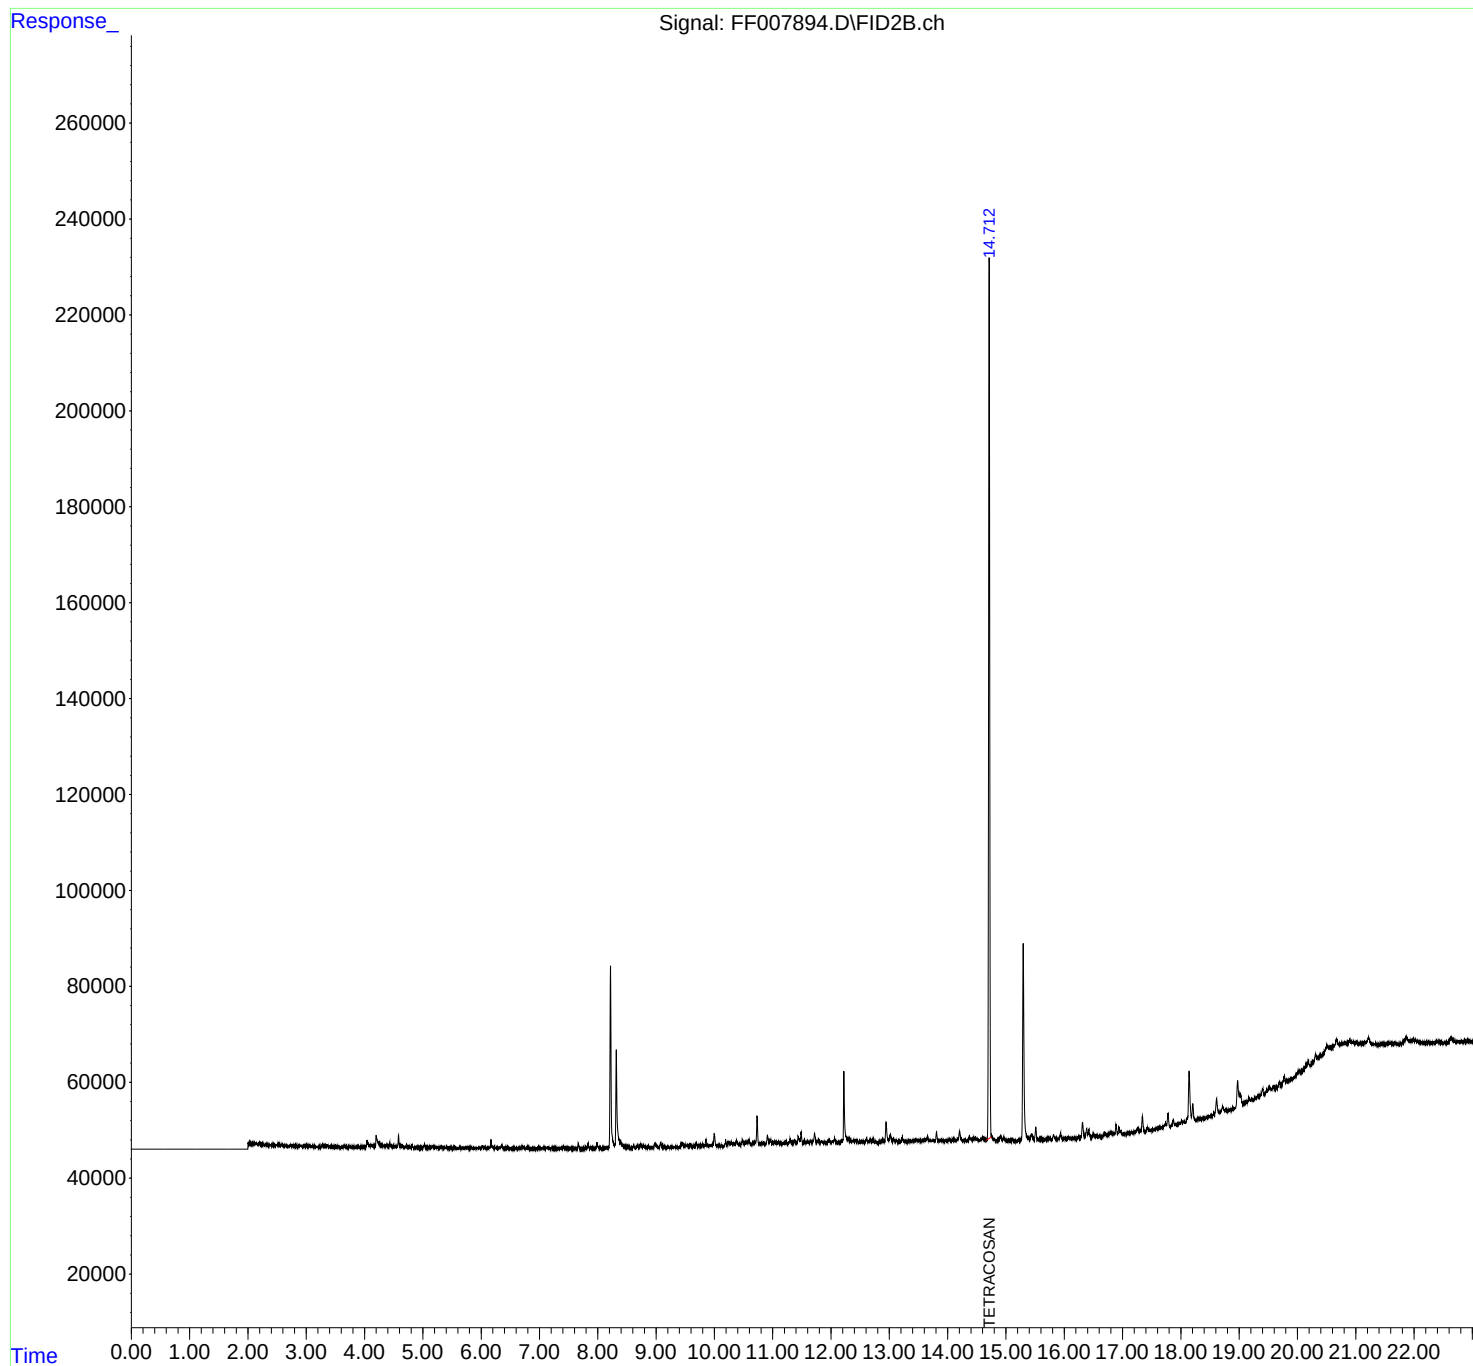

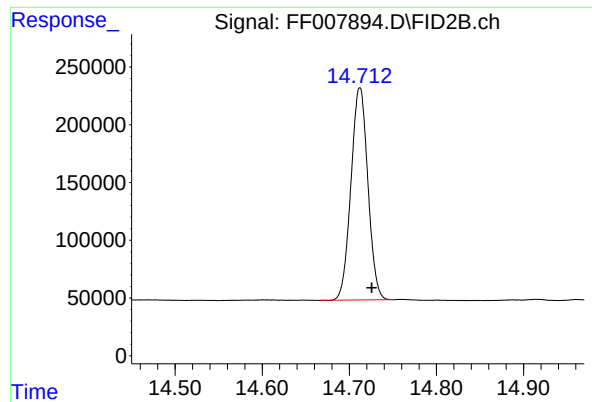

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.712 min
Delta R.T.: -0.013 min
Response: 2481713
Conc: 19.43 ug/ml

Instrument :
FID_F
ClientSampleId :
CSIMW-1-20201117