

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111823\
 Data File : FF013740.D
 Signal(s) : FID2B.ch
 Acq On : 18 Nov 2023 09:20
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 20 02:35:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111023.M
 Quant Title :
 QLast Update : Fri Nov 10 12:42:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.918	38114	0.334 ug/ml
Target Compounds			
10) N-TETRACOSANE	15.131	71223	0.590 ug/ml
14) N-DOTRIACONTANE	18.880	133096	1.229 ug/ml
15) N-TETRATRIACONTANE	19.614	90256	0.968 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111823\
Data File : FF013740.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2023 09:20
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 20 02:35:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111023.M
Quant Title :
QLast Update : Fri Nov 10 12:42:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

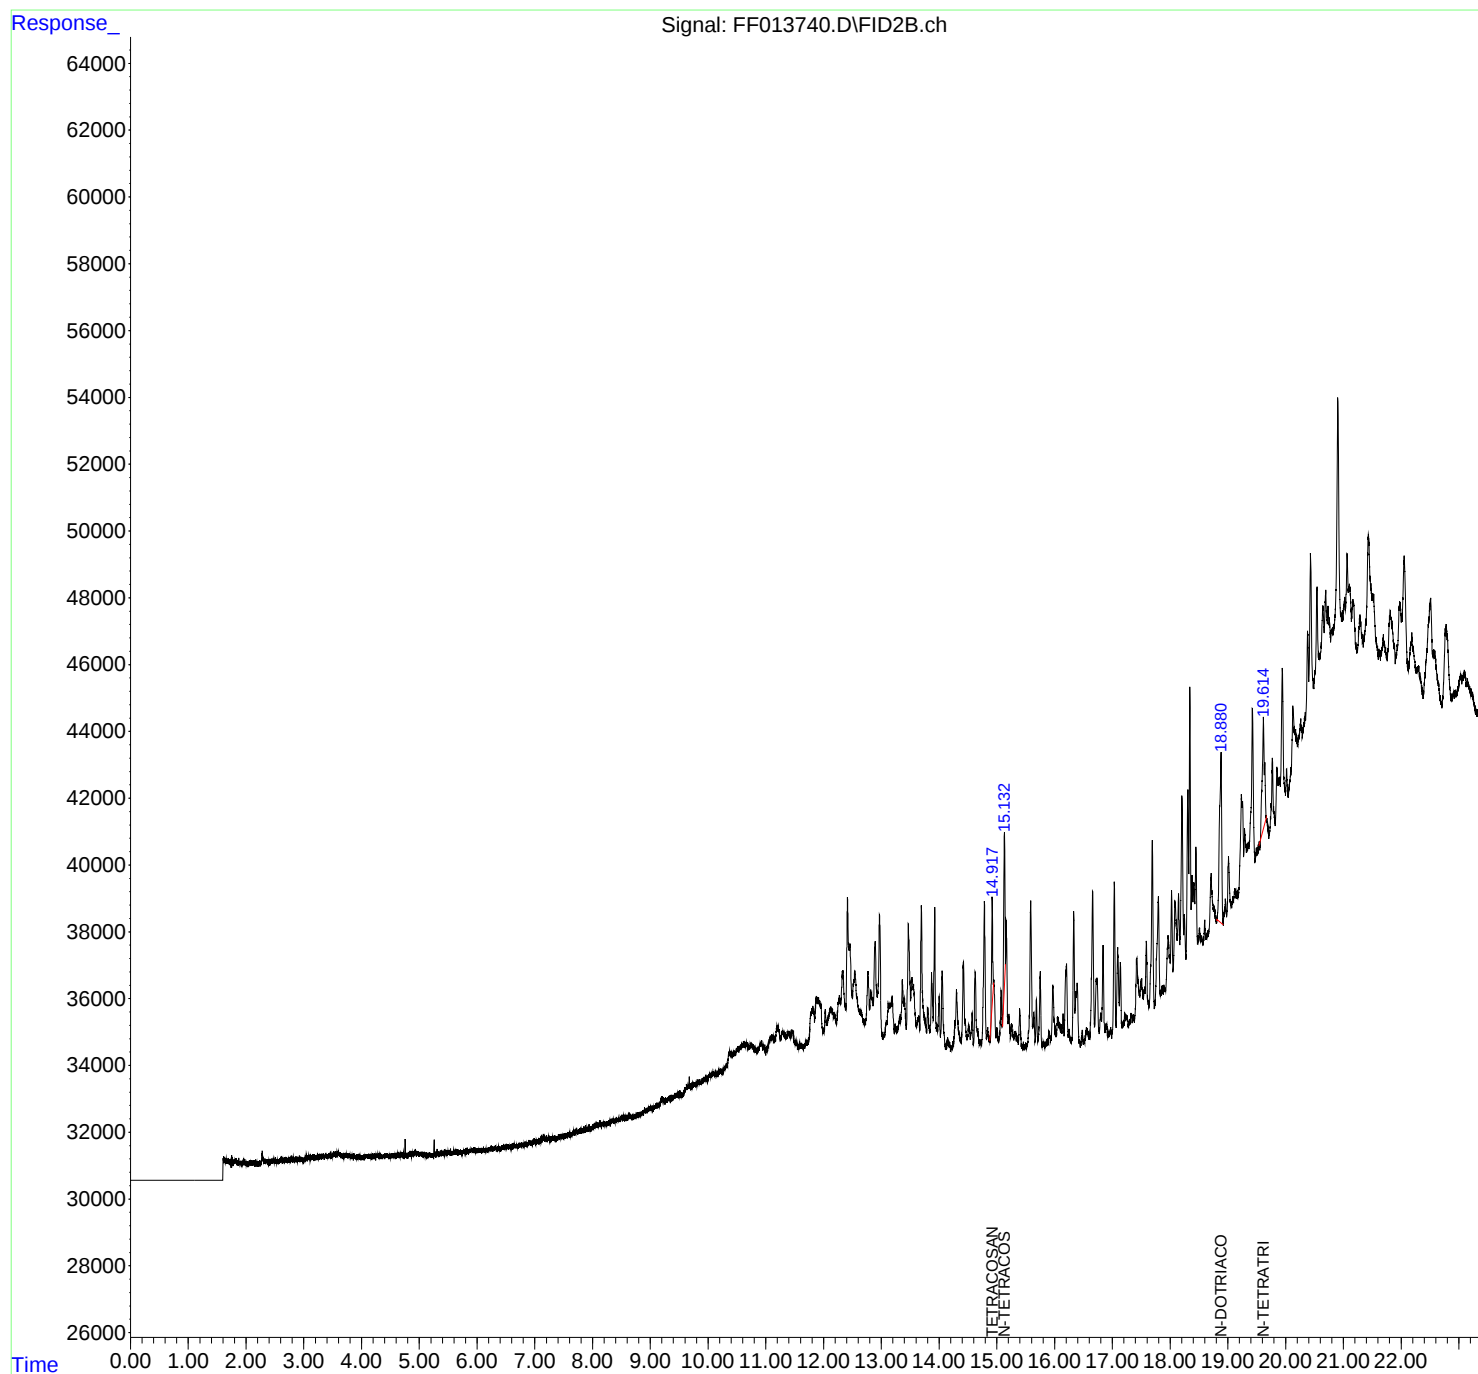

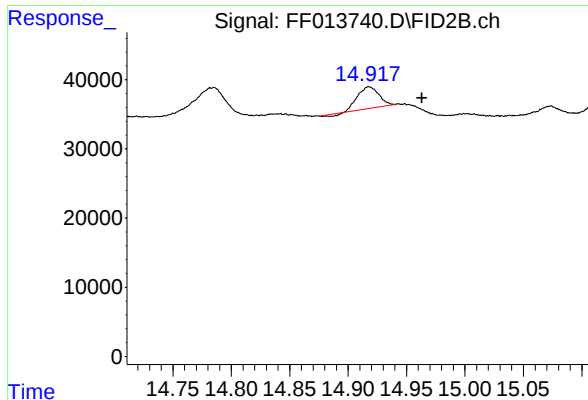


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.918 min
Delta R.T.: -0.046 min
Response: 38114
Conc: 0.33 ug/ml

Instrument :


FID_F

ClientSampleId :

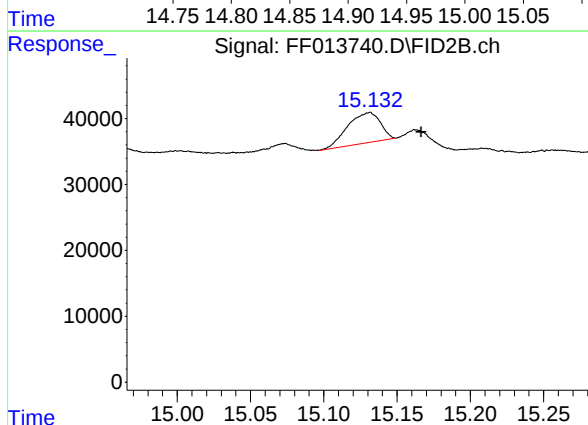


#10 N-TETRACOSANE

R.T.: 15.131 min
Delta R.T.: -0.035 min
Response: 71223
Conc: 0.59 ug/ml

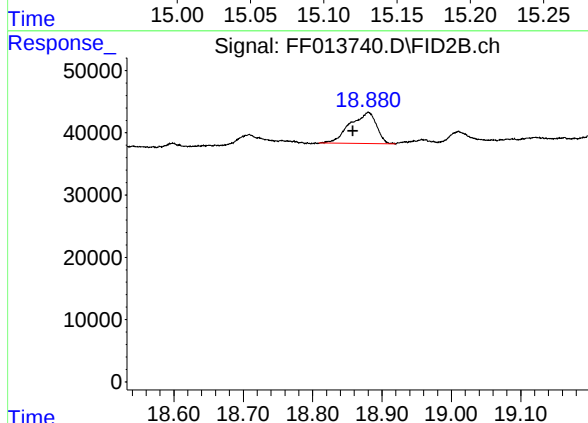

#14 N-DOTRIACONTANE

R.T.: 18.880 min
Delta R.T.: 0.022 min
Response: 133096
Conc: 1.23 ug/ml

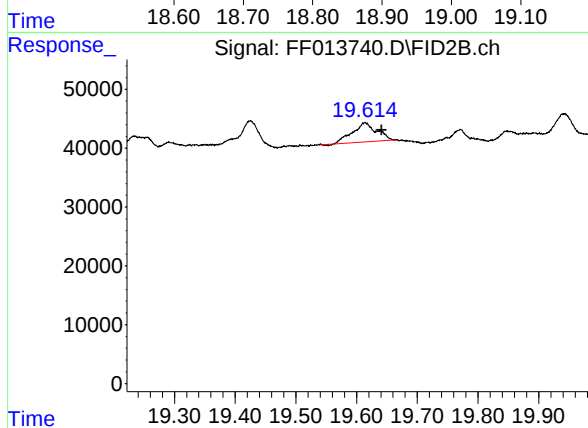

#15 N-TETRATRIACONTANE

R.T.: 19.614 min
Delta R.T.: -0.028 min
Response: 90256
Conc: 0.97 ug/ml