

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111823\
 Data File : FF013743.D
 Signal(s) : FID2B.ch
 Acq On : 18 Nov 2023 10:48
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 20 02:35:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111023.M
 Quant Title :
 QLast Update : Fri Nov 10 12:42:28 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.680	2859506	23.152 ug/ml
12) N-OCTACOSANE	17.140	2736365	23.778 ug/ml
13) N-TRIACONTANE	18.027	69559	0.617 ug/ml
14) N-DOTRIACONTANE	18.859	99423	0.918 ug/ml
15) N-TETRATRIACONTANE	19.643	86052	0.923 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111823\
Data File : FF013743.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2023 10:48
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 20 02:35:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111023.M
Quant Title :
QLast Update : Fri Nov 10 12:42:28 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

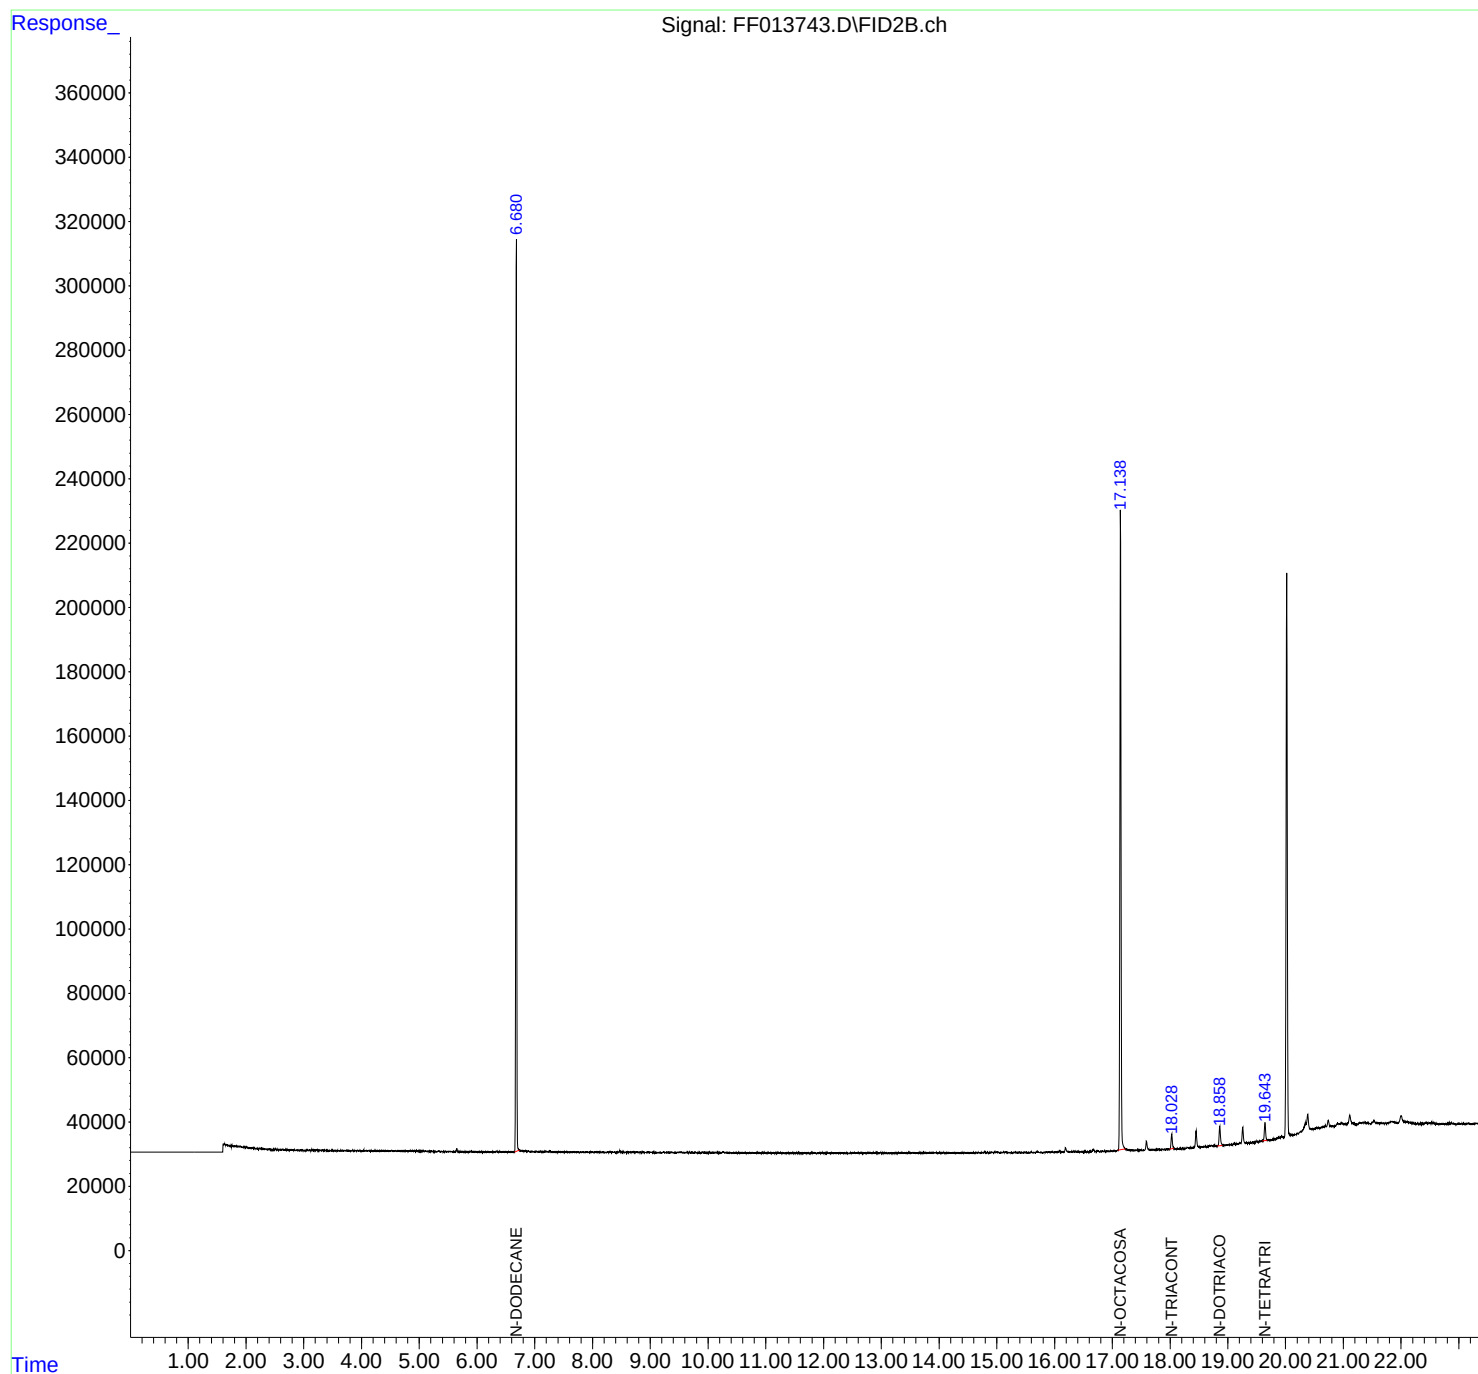


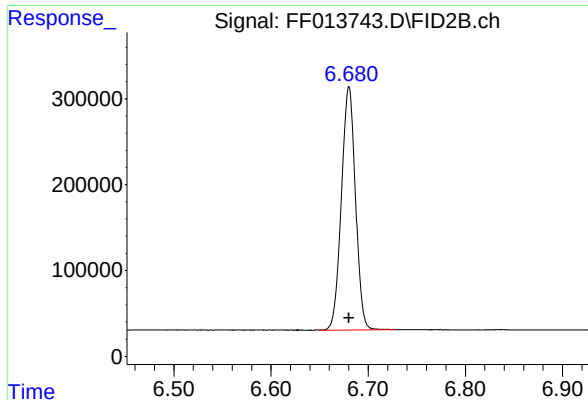

#3 N-DODECANE


R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 2859506
Conc: 23.15 ug/ml

Instrument :
FID_F
ClientSampleId :

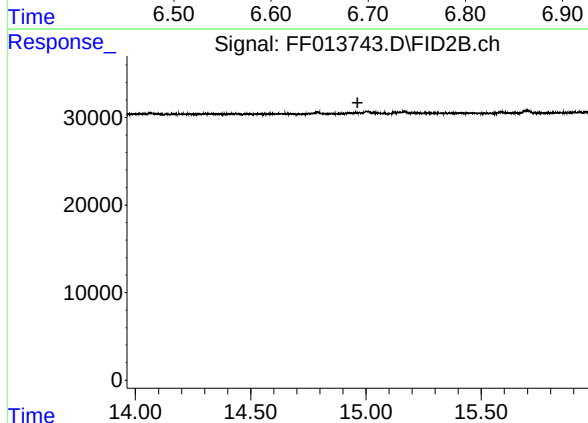


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.963 min
Response: 0
Conc: N.D.

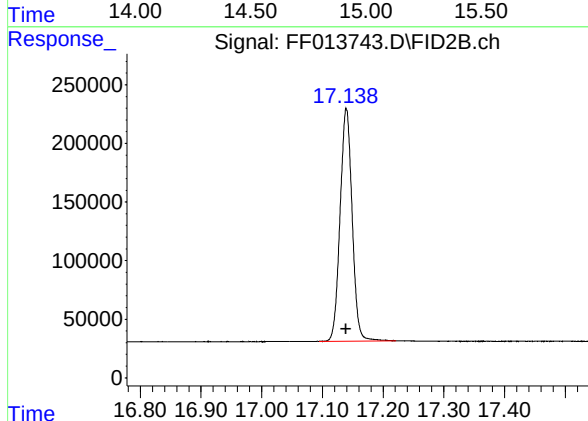


#12 N-OCTACOSANE

R.T.: 17.140 min
Delta R.T.: 0.000 min
Response: 2736365
Conc: 23.78 ug/ml

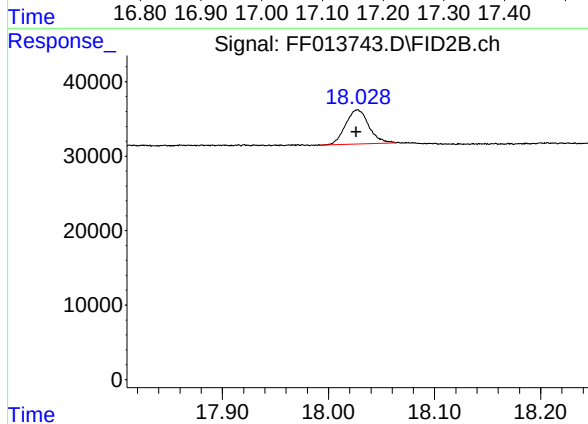

#13 N-TRIACONTANE


R.T.: 18.027 min
Delta R.T.: 0.001 min
Response: 69559
Conc: 0.62 ug/ml

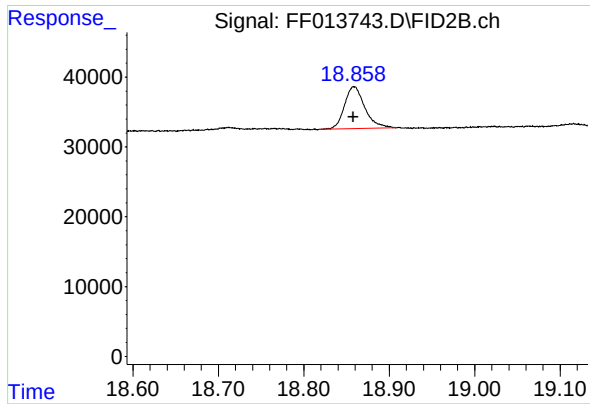

#14 N-DOTRIACONTANE

R.T.: 18.859 min
Delta R.T.: 0.000 min
Response: 99423
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :

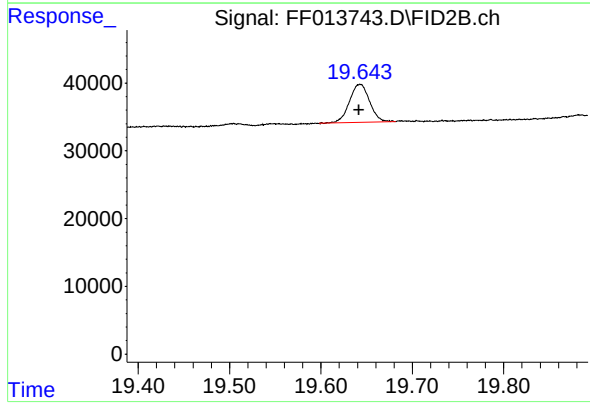

#15 N-TETRATRIACONTANE

R.T.: 19.643 min
Delta R.T.: 0.001 min
Response: 86052
Conc: 0.92 ug/ml