

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111824\
Data File : FF015081.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2024 12:28
Operator : YP\AJ
Sample : P4839-22
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EX-4-TPH-6

Integration File: autoint1.e
Quant Time: Nov 19 00:22:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111324.M
Quant Title :
QLast Update : Wed Nov 13 12:50:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.011	1787297	16.215 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111824\
Data File : FF015081.D
Signal(s) : FID2B.ch
Acq On : 18 Nov 2024 12:28
Operator : YP\AJ
Sample : P4839-22
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EX-4-TPH-6

Integration File: autoint1.e
Quant Time: Nov 19 00:22:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111324.M
Quant Title :
QLast Update : Wed Nov 13 12:50:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

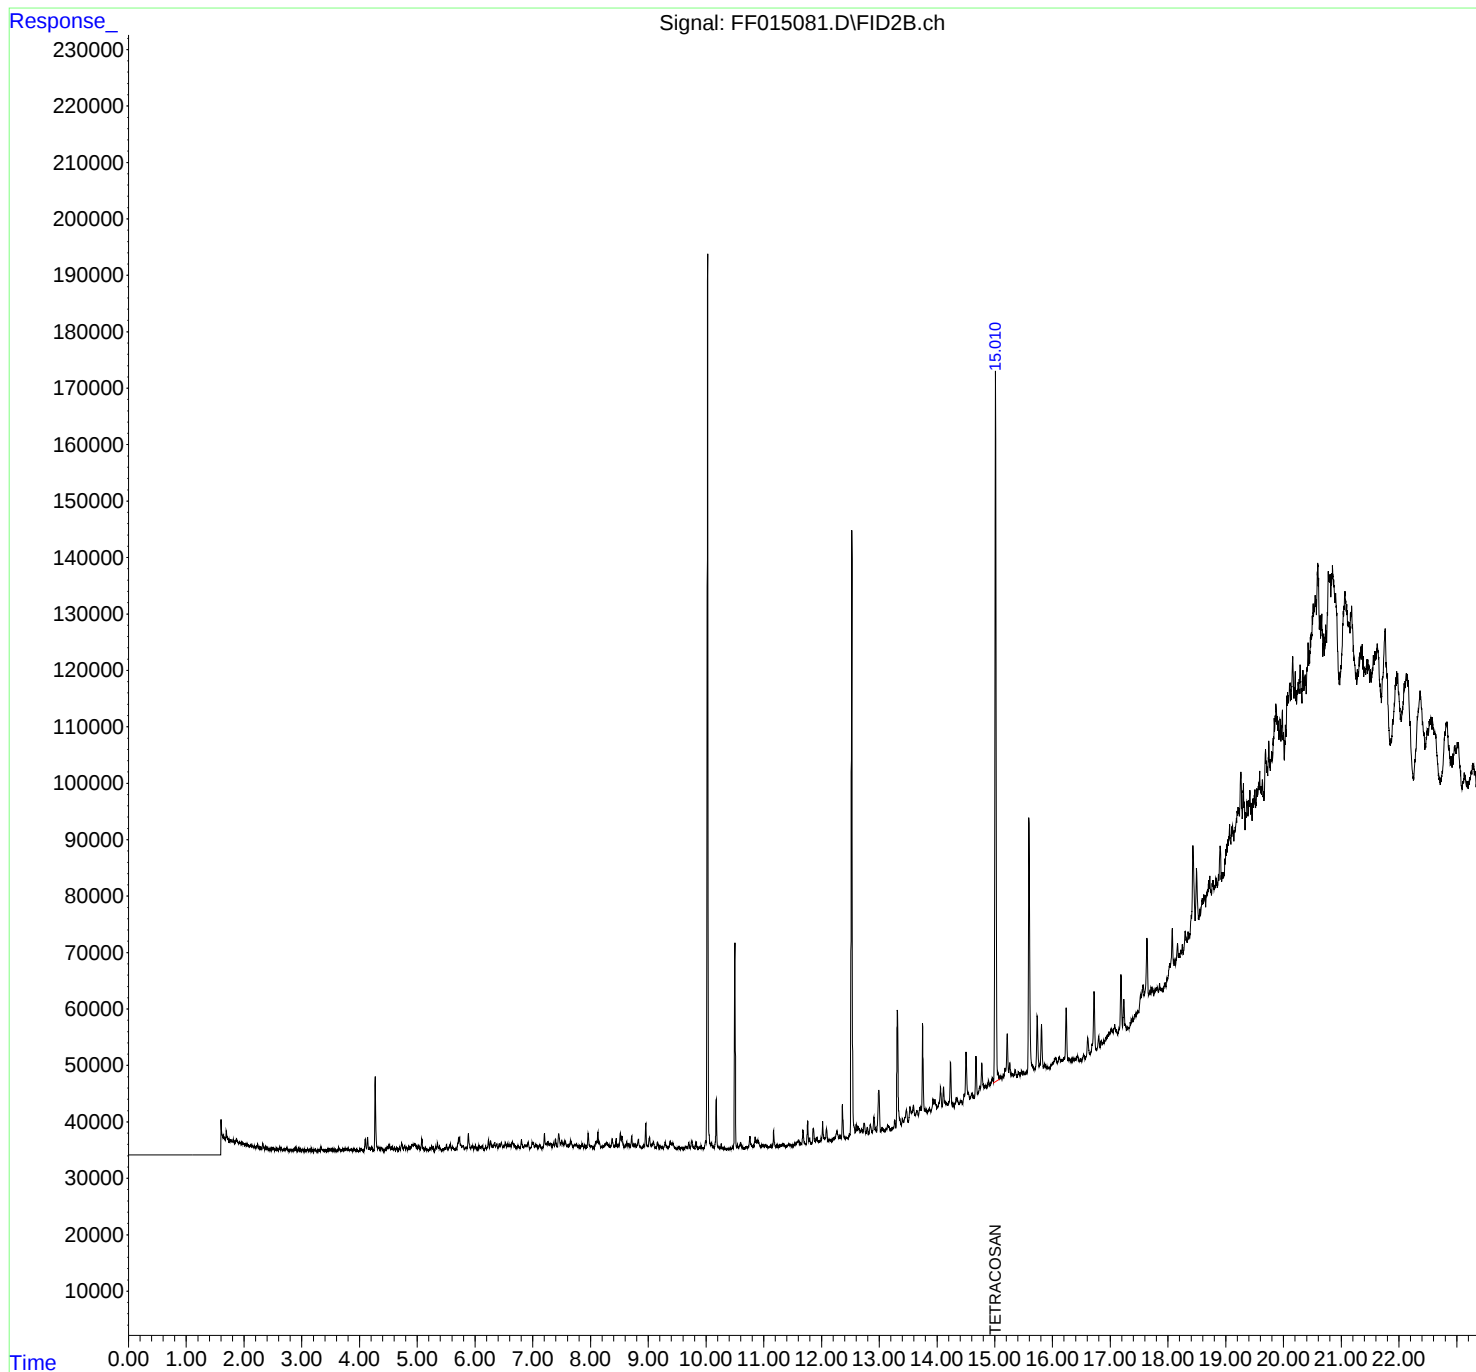

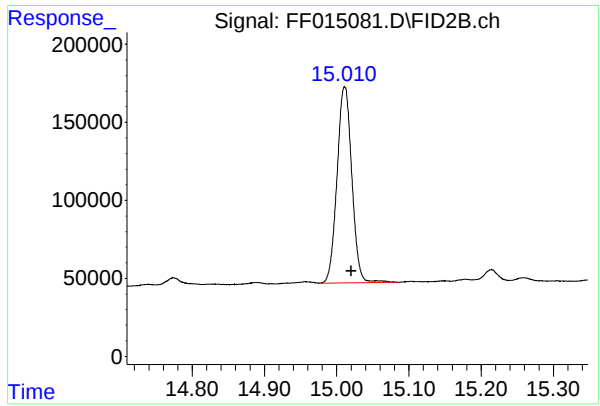

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.011 min
Delta R.T.: -0.009 min
Response: 1787297
Conc: 16.22 ug/ml

Instrument :
FID_F
ClientSampleId :
EX-4-TPH-6