

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111918\
 Data File : FF002739.D
 Signal(s) : FID2B.ch
 Acq On : 19 Nov 2018 18:41
 Operator : AJ\SJ
 Sample : J5964-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 20 00:27:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.644	1583121	20.266 ug/ml
Target Compounds			
4) N-TETRADECANE	8.242f	528247	4.573 ug/ml
5) N-HEXADECANE	9.787	121768	1.114 ug/ml
6) N-OCTADECANE	11.229	114433	1.102 ug/ml
7) N-EICOSANE	12.590	160415	1.657 ug/ml
12) N-OCTACOSANE	16.819	96917	1.016 ug/ml
13) N-TRIACONTANE	17.711	120178	1.212 ug/ml
14) N-DOTRIACONTANE	18.542	133329	1.347 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111918\
Data File : FF002739.D
Signal(s) : FID2B.ch
Acq On : 19 Nov 2018 18:41
Operator : AJ\SJ
Sample : J5964-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 20 00:27:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

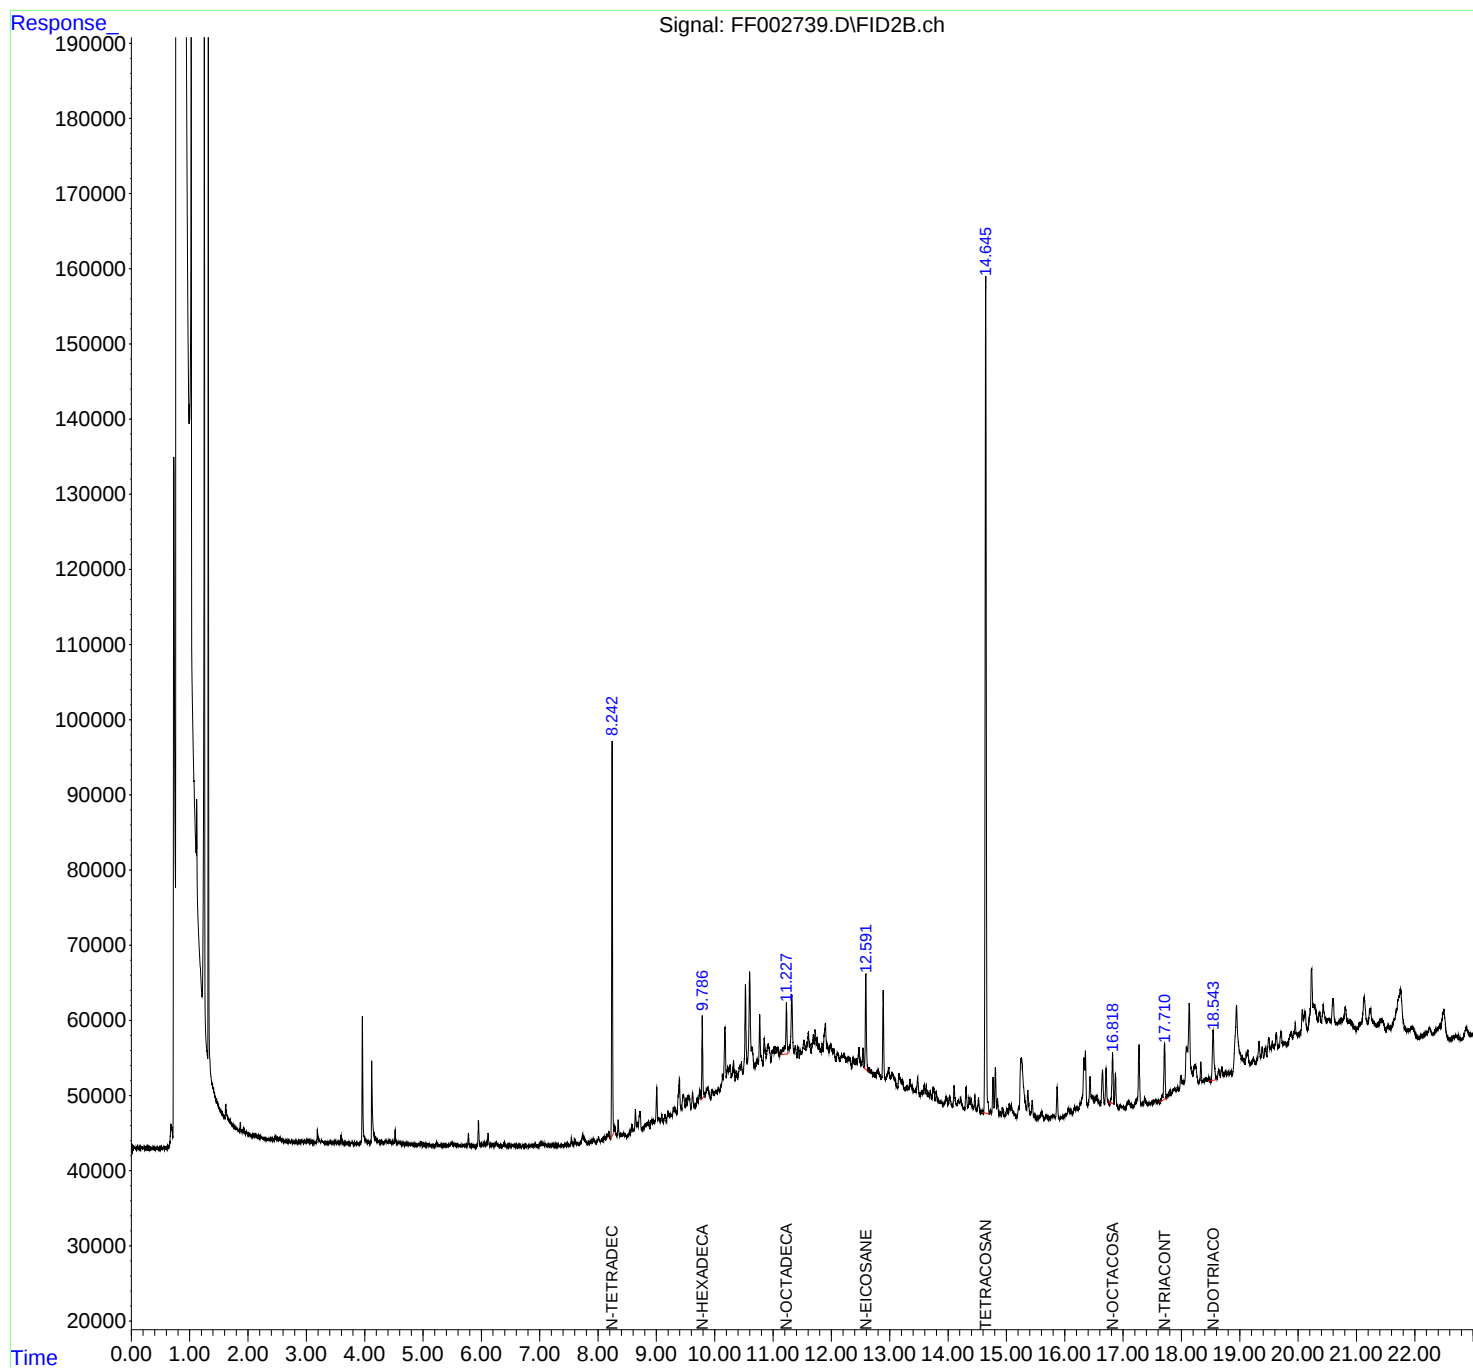

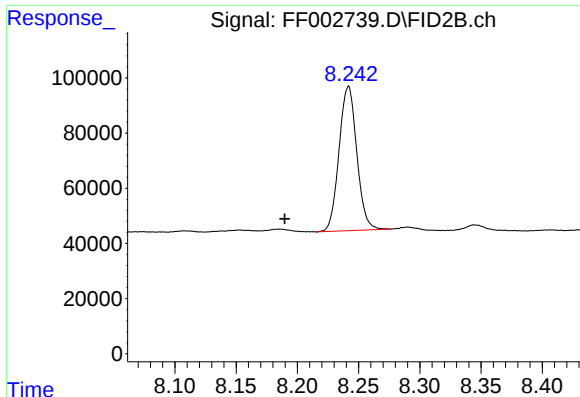


#4 N-TETRADECANE

R.T.: 8.242 min
Delta R.T.: 0.052 min
Response: 528247
Conc: 4.57 ug/ml

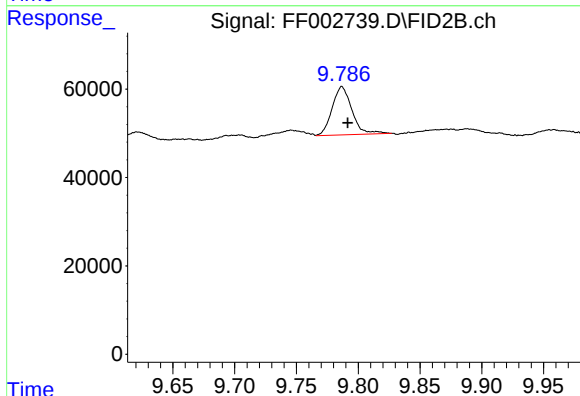


#5 N-HEXADECANE

R.T.: 9.787 min
Delta R.T.: -0.005 min
Response: 121768
Conc: 1.11 ug/ml

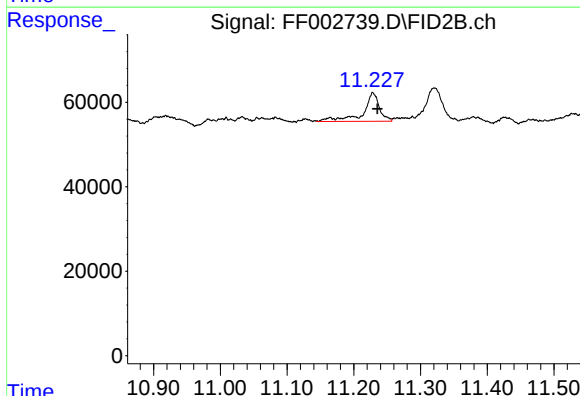


#6 N-OCTADECANE

R.T.: 11.229 min
Delta R.T.: -0.007 min
Response: 114433
Conc: 1.10 ug/ml

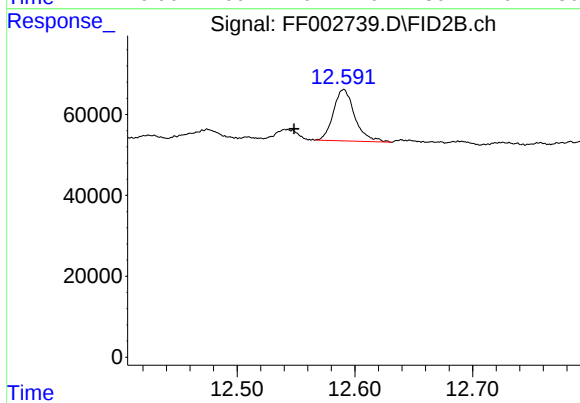


#7 N-EICOSANE

R.T.: 12.590 min
Delta R.T.: 0.042 min
Response: 160415
Conc: 1.66 ug/ml

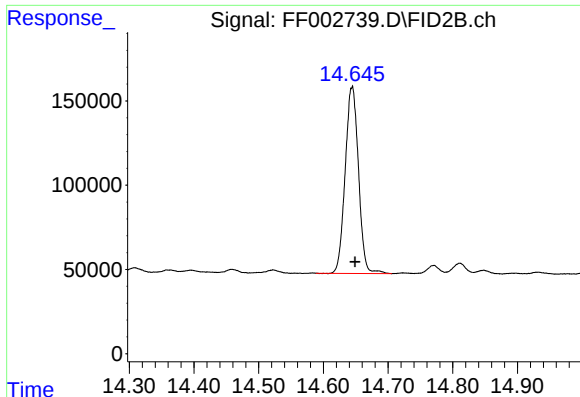


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.644 min
Delta R.T.: -0.004 min
Response: 1583121
Conc: 20.27 ug/ml

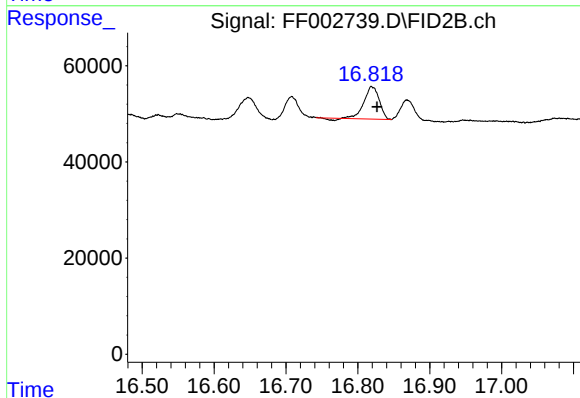


#12 N-OCTACOSANE

R.T.: 16.819 min
Delta R.T.: -0.008 min
Response: 96917
Conc: 1.02 ug/ml

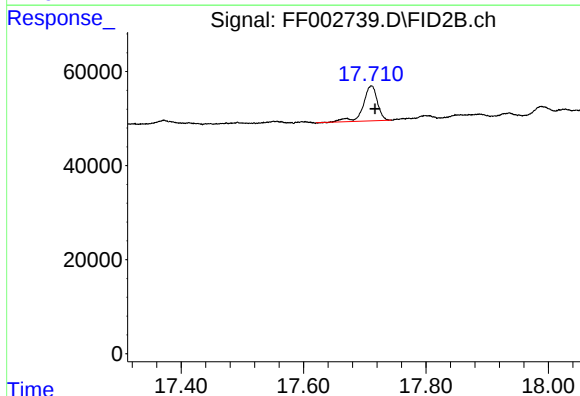

#13 N-TRIACONTANE

R.T.: 17.711 min
Delta R.T.: -0.006 min
Response: 120178
Conc: 1.21 ug/ml

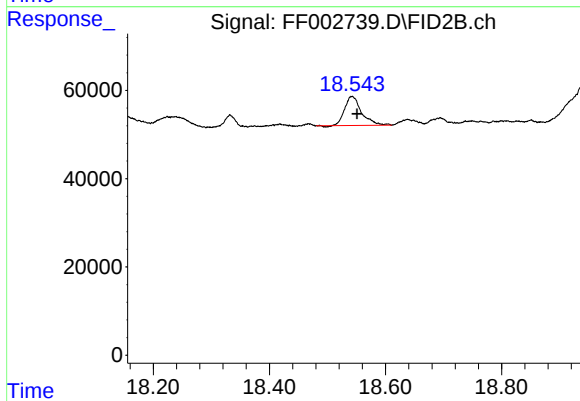

#14 N-DOTRIACONTANE

R.T.: 18.542 min
Delta R.T.: -0.008 min
Response: 133329
Conc: 1.35 ug/ml