

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111918\
 Data File : FF002742.D
 Signal(s) : FID2B.ch
 Acq On : 19 Nov 2018 20:11
 Operator : AJ\SJ
 Sample : J5762-05 2X
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 20 00:28:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.645	905007	11.585 ug/ml
Target Compounds			
4) N-TETRADECANE	8.242f	213557	1.849 ug/ml
5) N-HEXADECANE	9.788	114667	1.049 ug/ml
6) N-OCTADECANE	11.231	80798	0.778 ug/ml
7) N-EICOSANE	12.595	219245	2.264 ug/ml
10) N-TETRACOSANE	14.836	542282	6.087 ug/ml
11) N-HEXACOSANE	15.873	163055	1.797 ug/ml
12) N-OCTACOSANE	16.822	280755	2.944 ug/ml
13) N-TRIACONTANE	17.711	515938	5.204 ug/ml
14) N-DOTRIACONTANE	18.544	520921	5.262 ug/ml
15) N-TETRATRIACONTANE	19.333	165039	1.672 ug/ml
16) N-HEXATRIACONTANE	20.078	98522	1.034 ug/ml
17) N-OCTATRIACONTANE	20.819	121470	1.382 ug/ml
18) N-TETRACONTANE	21.729	74701	0.853 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111918\
Data File : FF002742.D
Signal(s) : FID2B.ch
Acq On : 19 Nov 2018 20:11
Operator : AJ\SJ
Sample : J5762-05 2X
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 20 00:28:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

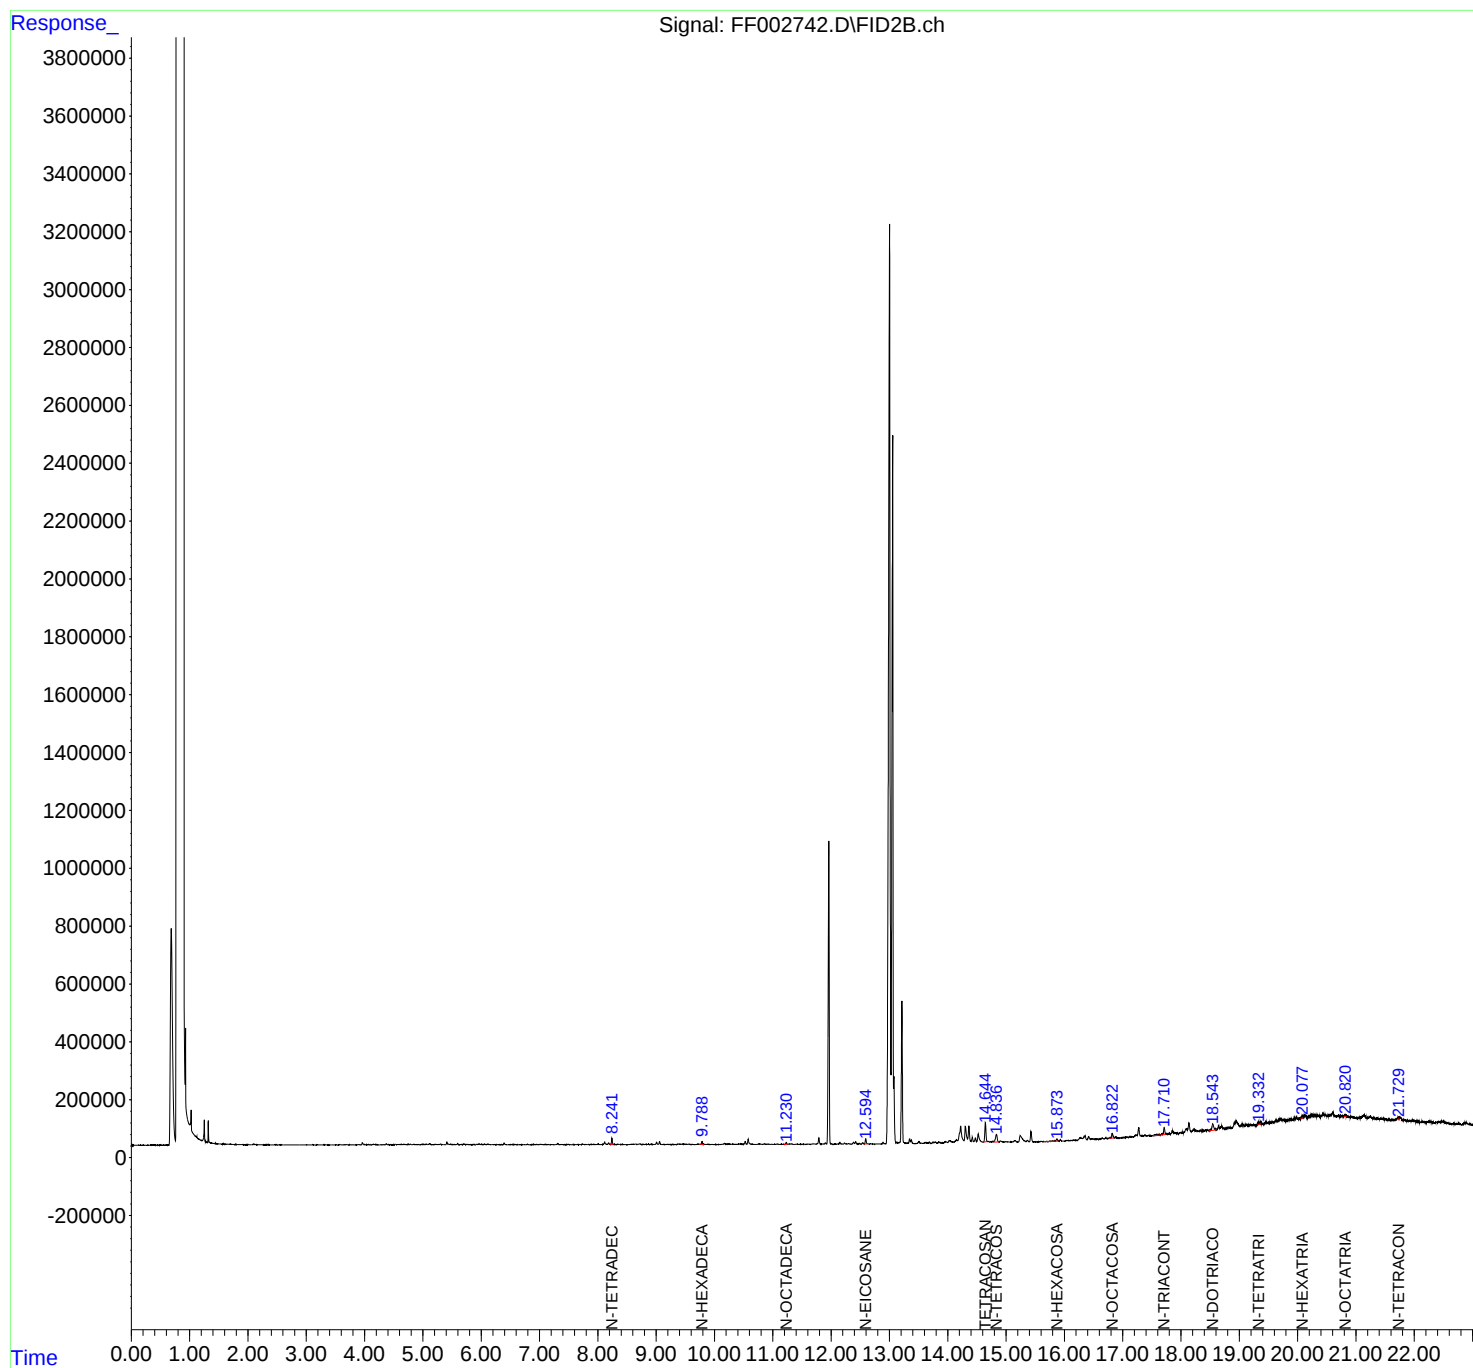

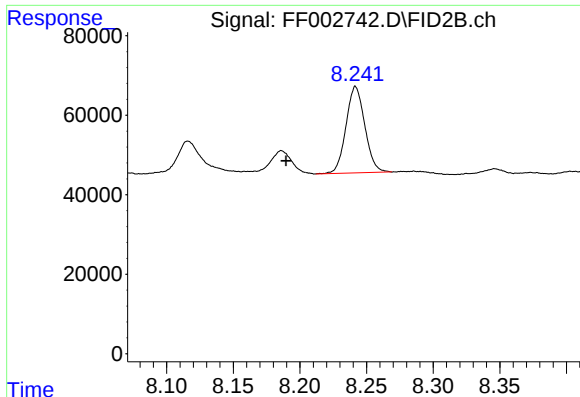


#4 N-TETRADECANE

R.T.: 8.242 min
Delta R.T.: 0.052 min
Response: 213557
Conc: 1.85 ug/ml

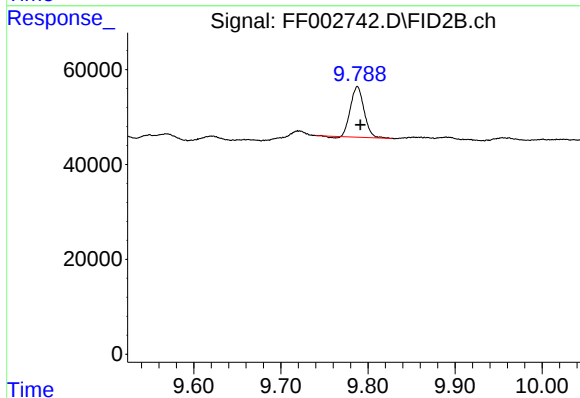


#5 N-HEXADECANE

R.T.: 9.788 min
Delta R.T.: -0.003 min
Response: 114667
Conc: 1.05 ug/ml

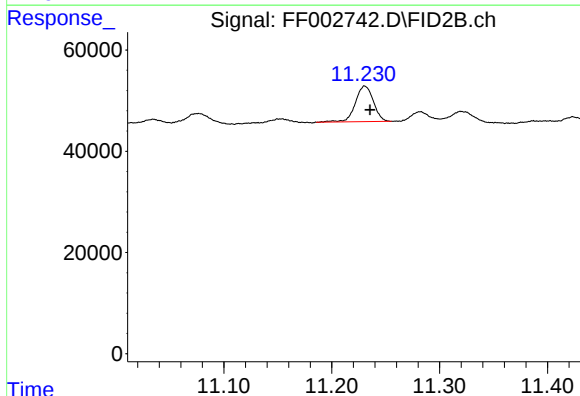


#6 N-OCTADECANE

R.T.: 11.231 min
Delta R.T.: -0.005 min
Response: 80798
Conc: 0.78 ug/ml

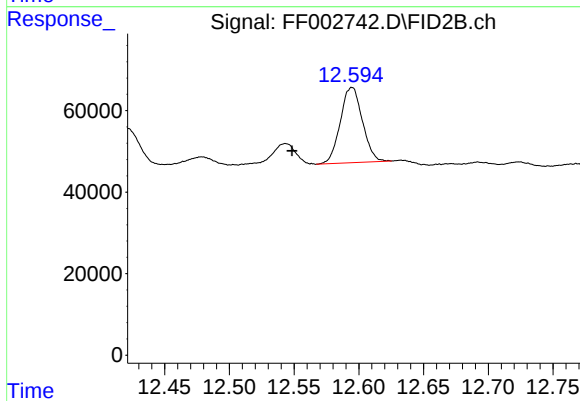


#7 N-EICOSANE

R.T.: 12.595 min
Delta R.T.: 0.046 min
Response: 219245
Conc: 2.26 ug/ml

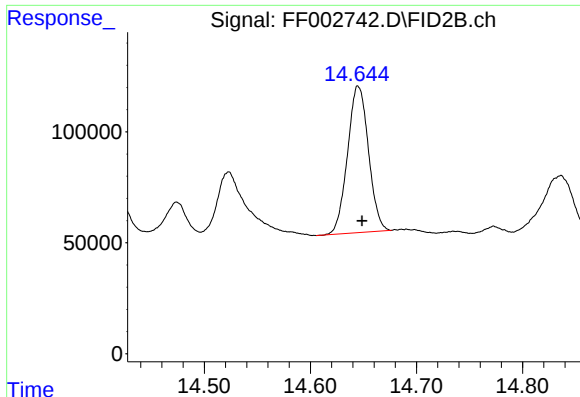


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.645 min
Delta R.T.: -0.004 min
Response: 905007
Conc: 11.59 ug/ml

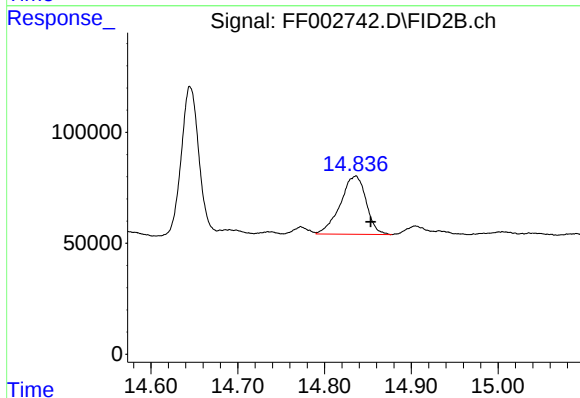


#10 N-TETRACOSANE

R.T.: 14.836 min
Delta R.T.: -0.017 min
Response: 542282
Conc: 6.09 ug/ml

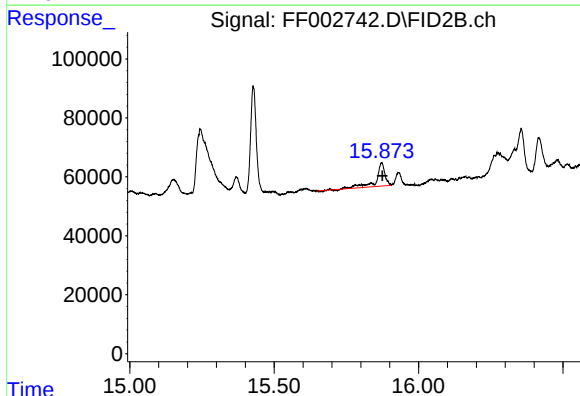


#11 N-HEXACOSANE

R.T.: 15.873 min
Delta R.T.: -0.002 min
Response: 163055
Conc: 1.80 ug/ml

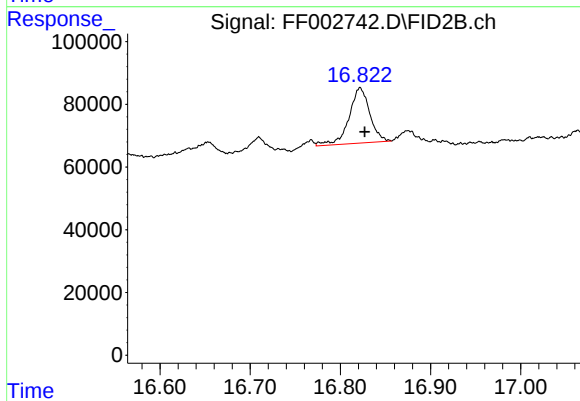


#12 N-OCTACOSANE

R.T.: 16.822 min
Delta R.T.: -0.005 min
Response: 280755
Conc: 2.94 ug/ml

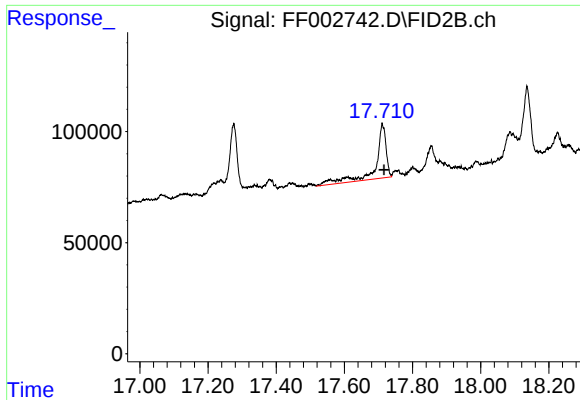


#13 N-TRIACONTANE

R.T.: 17.711 min
Delta R.T.: -0.006 min
Response: 515938
Conc: 5.20 ug/ml

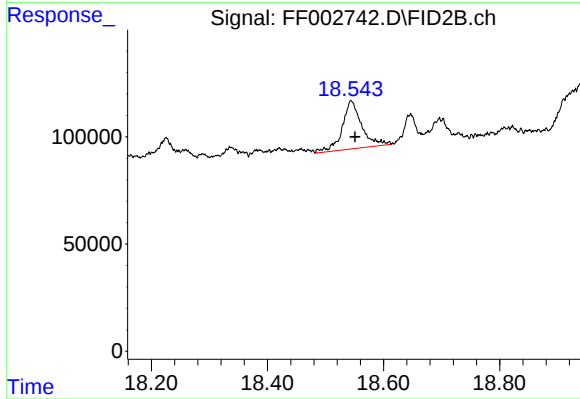


#14 N-DOTRIACONTANE

R.T.: 18.544 min
Delta R.T.: -0.007 min
Response: 520921
Conc: 5.26 ug/ml

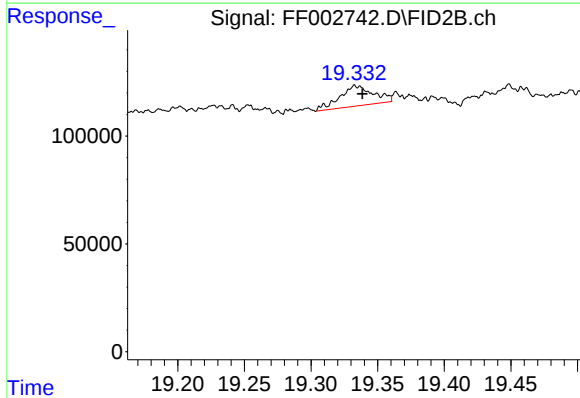


#15 N-TETRATRIACONTANE

R.T.: 19.333 min
Delta R.T.: -0.005 min
Response: 165039
Conc: 1.67 ug/ml

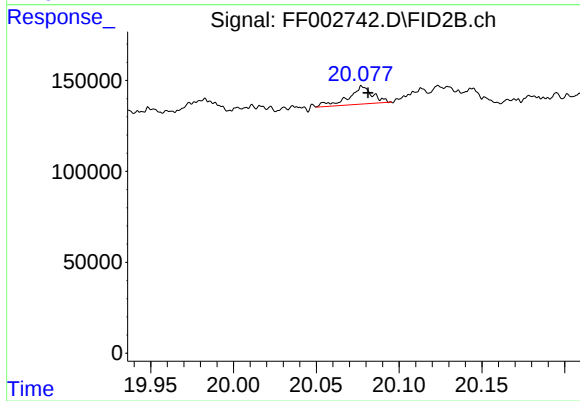


#16 N-HEXATRIACONTANE

R.T.: 20.078 min
Delta R.T.: -0.003 min
Response: 98522
Conc: 1.03 ug/ml

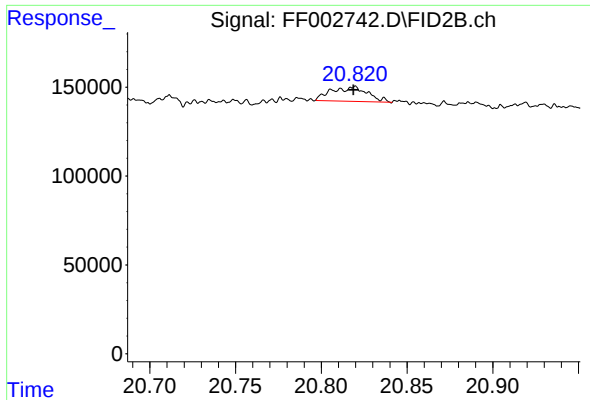

#17 N-OCTATRIACONTANE

R.T.: 20.819 min
Delta R.T.: 0.000 min
Response: 121470
Conc: 1.38 ug/ml

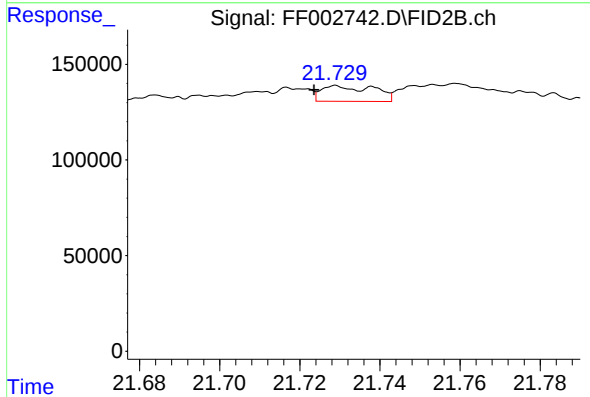

#18 N-TETRACONTANE

R.T.: 21.729 min
Delta R.T.: 0.005 min
Response: 74701
Conc: 0.85 ug/ml