

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111918\
 Data File : FF002737.D
 Signal(s) : FID2B.ch
 Acq On : 19 Nov 2018 17:40
 Operator : AJ\SJ
 Sample : J5989-01MS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 20 00:27:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	1993479	25.519 ug/mlm
Target Compounds			
2) N-DECANE	4.373	2229305	17.849 ug/ml
3) N-DODECANE	6.393	2451895	20.229 ug/ml
4) N-TETRADECANE	8.187	2431457	21.049 ug/ml
5) N-HEXADECANE	9.788	2420204	22.135 ug/ml
6) N-OCTADECANE	11.231	2357572	22.711 ug/ml
7) N-EICOSANE	12.543	2402459	24.813 ug/ml
8) N-DOCOSANE	13.744	2453552	26.798 ug/ml
10) N-TETRACOSANE	14.849	2301678	25.836 ug/ml
11) N-HEXACOSANE	15.873	2312383	25.480 ug/ml
12) N-OCTACOSANE	16.825	2558739	26.827 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111918\
Data File : FF002737.D
Signal(s) : FID2B.ch
Acq On : 19 Nov 2018 17:40
Operator : AJ\SJ
Sample : J5989-01MS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 20 00:27:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

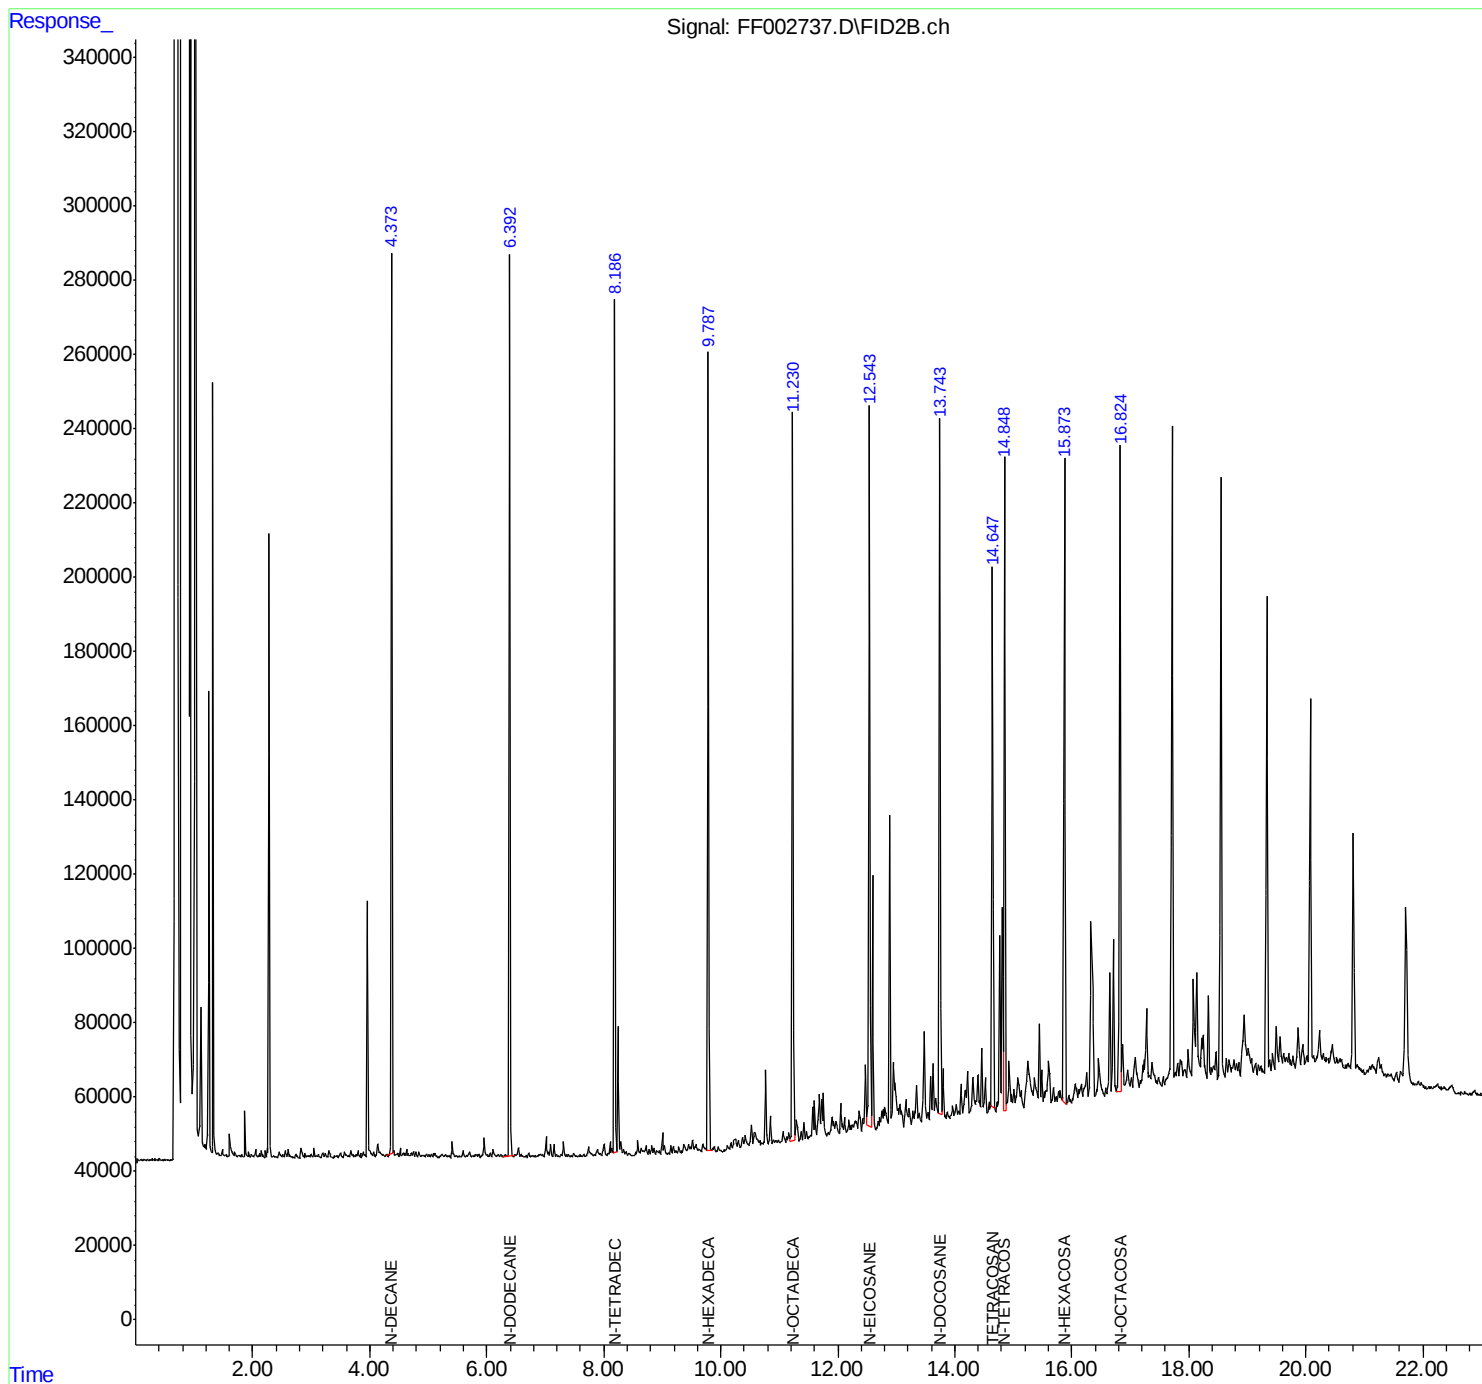

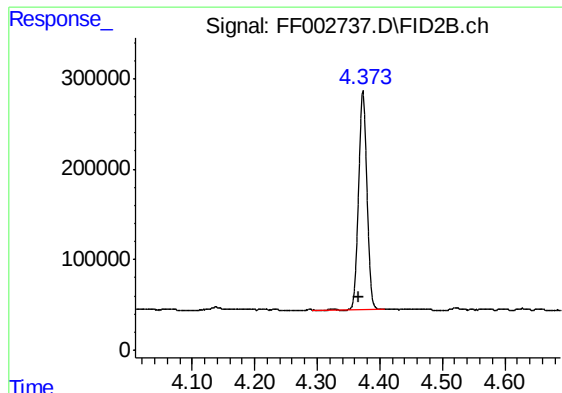


#2 N-DECANE

R.T.: 4.373 min
Delta R.T.: 0.007 min
Response: 2229305
Conc: 17.85 ug/ml

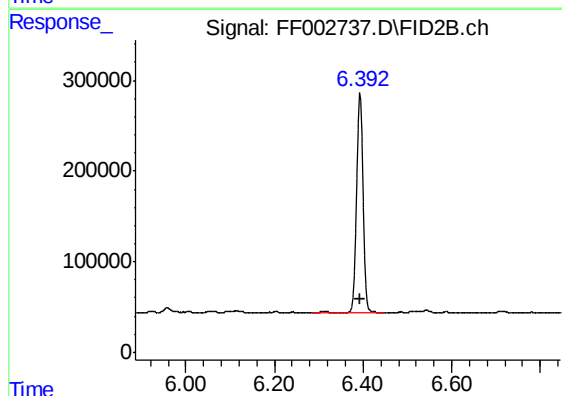


#3 N-DODECANE

R.T.: 6.393 min
Delta R.T.: 0.000 min
Response: 2451895
Conc: 20.23 ug/ml

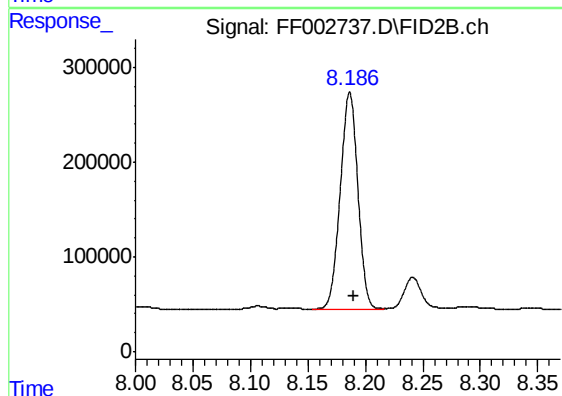


#4 N-TETRADECANE

R.T.: 8.187 min
Delta R.T.: -0.003 min
Response: 2431457
Conc: 21.05 ug/ml

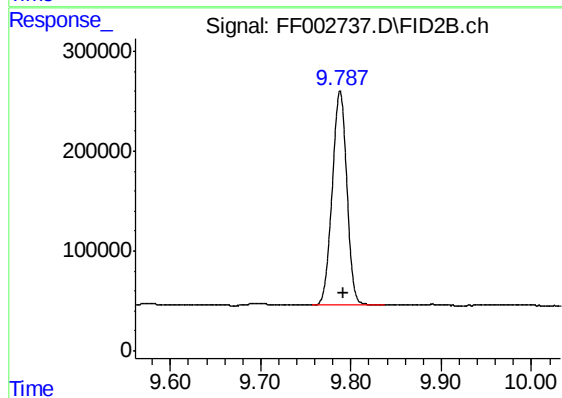


#5 N-HEXADECANE

R.T.: 9.788 min
Delta R.T.: -0.003 min
Response: 2420204
Conc: 22.13 ug/ml

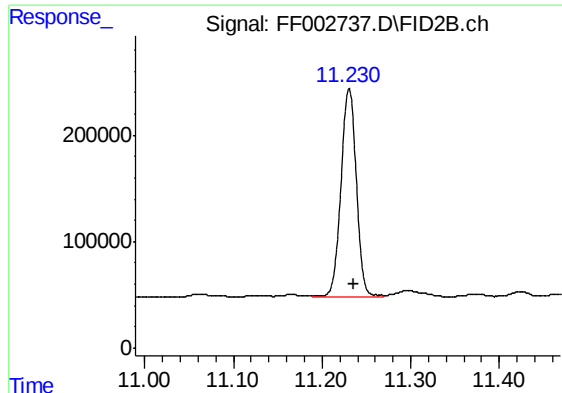


#6 N-OCTADECANE

R.T.: 11.231 min
Delta R.T.: -0.005 min
Response: 2357572
Conc: 22.71 ug/ml

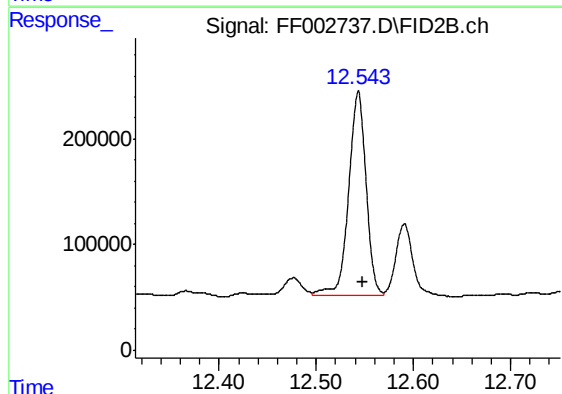


#7 N-EICOSANE

R.T.: 12.543 min
Delta R.T.: -0.005 min
Response: 2402459
Conc: 24.81 ug/ml

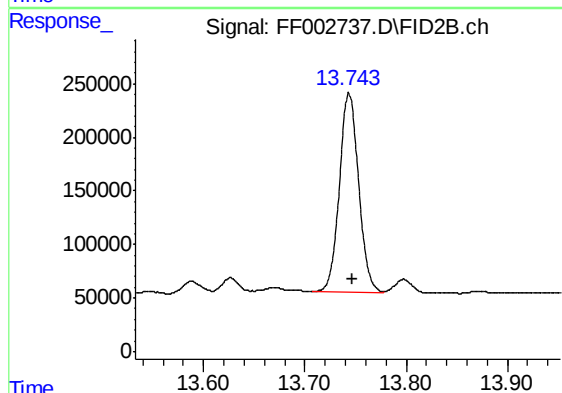


#8 N-DOCOSANE

R.T.: 13.744 min
Delta R.T.: -0.004 min
Response: 2453552
Conc: 26.80 ug/ml

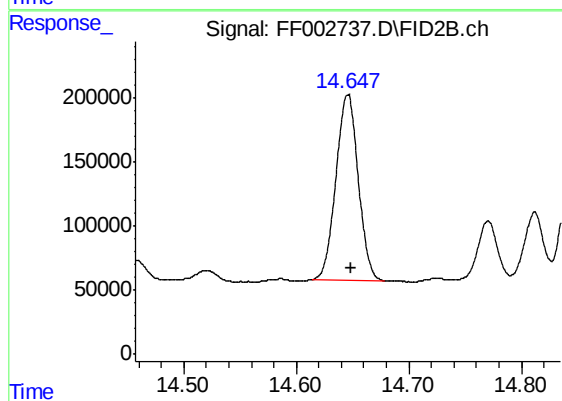


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.002 min
Response: 1993479
Conc: 25.52 ug/ml m

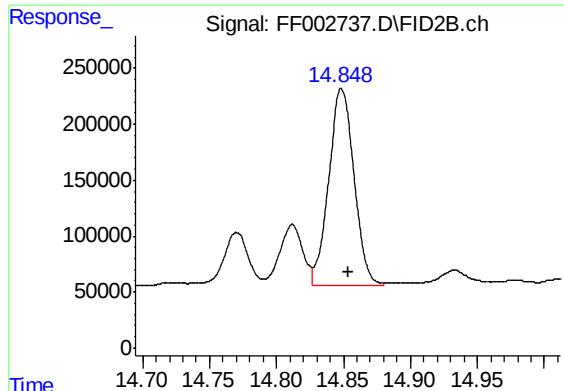


#10 N-TETRACOSANE

R.T.: 14.849 min
Delta R.T.: -0.005 min
Response: 2301678
Conc: 25.84 ug/ml

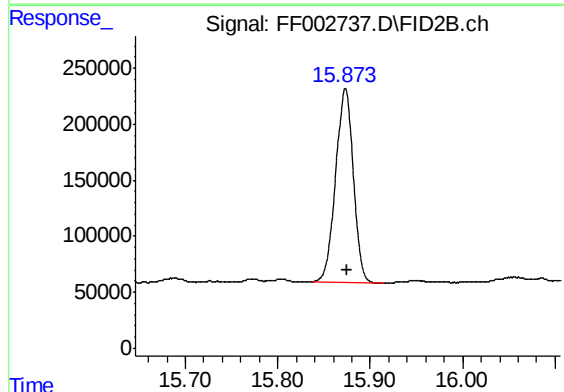

#11 N-HEXACOSANE

R.T.: 15.873 min
Delta R.T.: -0.002 min
Response: 2312383
Conc: 25.48 ug/ml

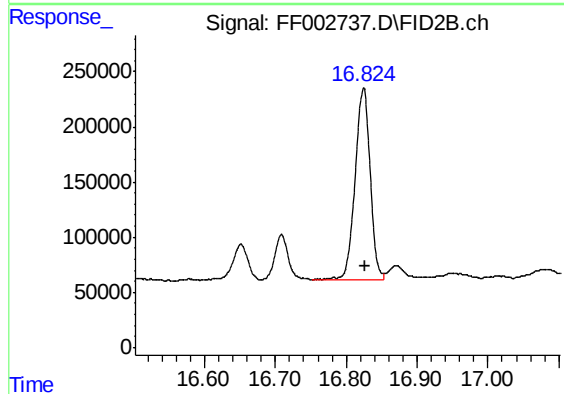

#12 N-OCTACOSANE

R.T.: 16.825 min
Delta R.T.: -0.002 min
Response: 2558739
Conc: 26.83 ug/ml