

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
 Data File : FF007906.D
 Signal(s) : FID2B.ch
 Acq On : 25 Nov 2020 10:27
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 25 16:31:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	5704893	44.662 ug/ml
Target Compounds			
1) N-OCTANE	2.324	6761665	50.378 ug/ml
2) N-DECANE	4.432	7156758	52.602 ug/ml
3) N-DODECANE	6.457	7203345	52.040 ug/ml
4) N-TETRADECANE	8.253	7160892	50.709 ug/ml
5) N-HEXADECANE	9.856	7123418	49.014 ug/ml
6) N-OCTADECANE	11.299	7074758	47.671 ug/ml
7) N-EICOSANE	12.610	6871708	46.360 ug/ml
8) N-DOCOSANE	13.811	6590924	45.239 ug/ml
10) N-TETRACOSANE	14.917	6415331	44.362 ug/ml
11) N-HEXACOSANE	15.939	6157074	43.869 ug/ml
12) N-OCTACOSANE	16.890	5975190	44.053 ug/ml
13) N-TRIACONTANE	17.780	5831546	45.069 ug/ml
14) N-DOTRIACONTANE	18.614	5417303	46.730 ug/ml
15) N-TETRATRIACONTANE	19.399	4593436	48.904 ug/ml
16) N-HEXATRIACONTANE	20.142	3731284	49.122 ug/ml
17) N-OCTATRIACONTANE	20.891	3135257	50.459 ug/ml
18) N-TETRACONTANE	21.824	2918536	47.837 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
Data File : FF007906.D
Signal(s) : FID2B.ch
Acq On : 25 Nov 2020 10:27
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 25 16:31:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

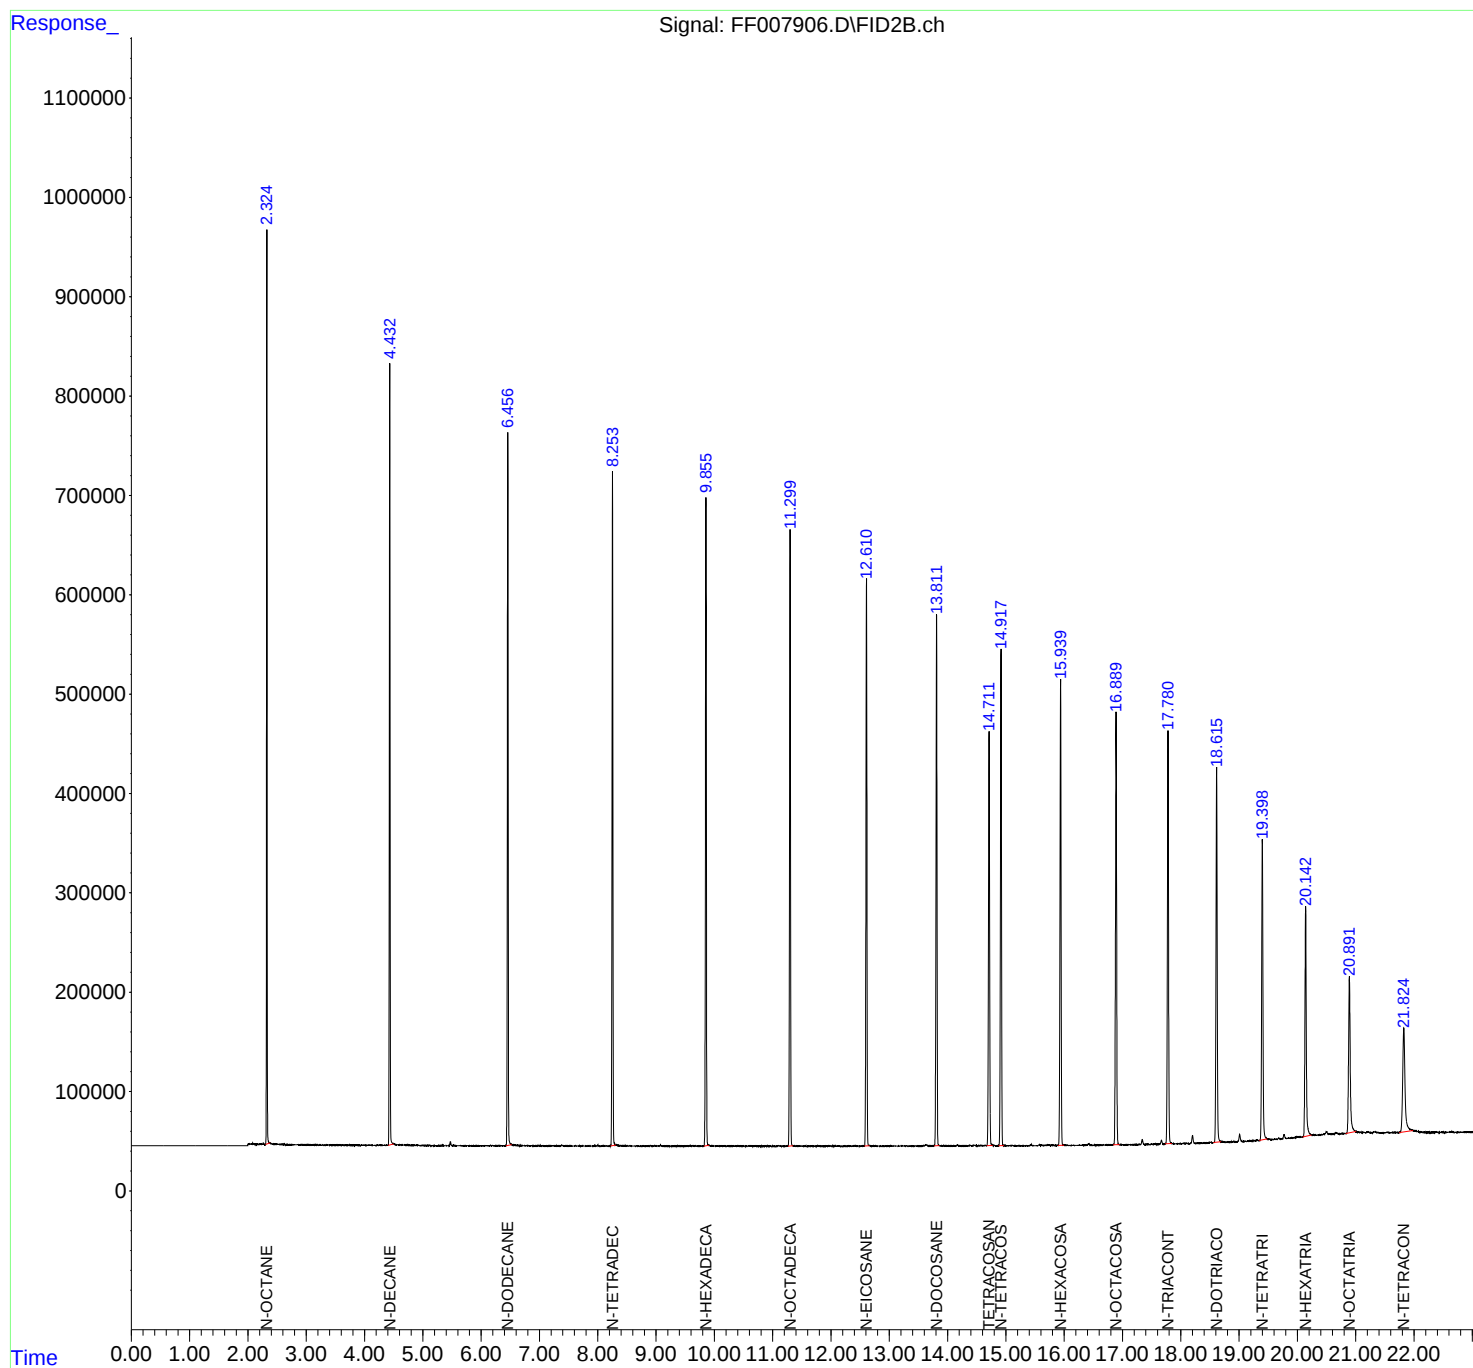


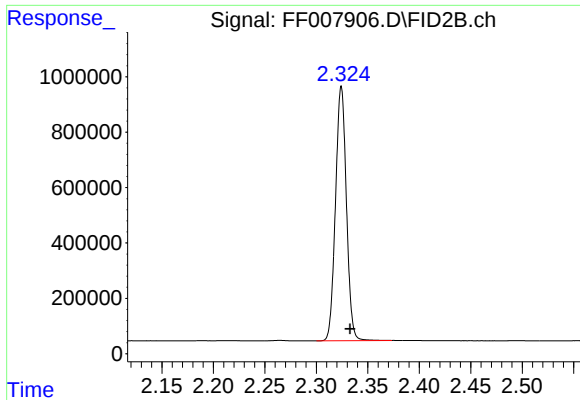

#1 N-OCTANE


R.T.: 2.324 min
Delta R.T.: -0.009 min
Response: 6761665
Conc: 50.38 ug/ml

Instrument :
FID_F
ClientSampleId :

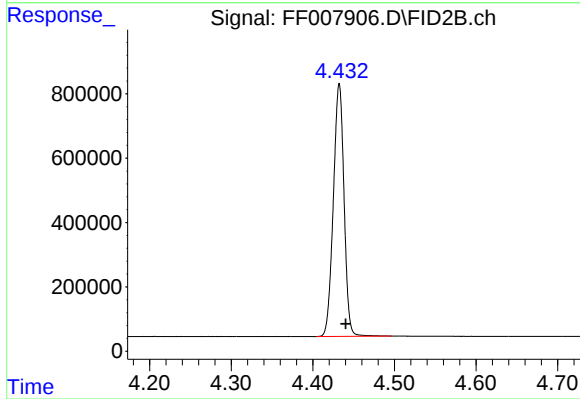


#2 N-DECANE

R.T.: 4.432 min
Delta R.T.: -0.008 min
Response: 7156758
Conc: 52.60 ug/ml

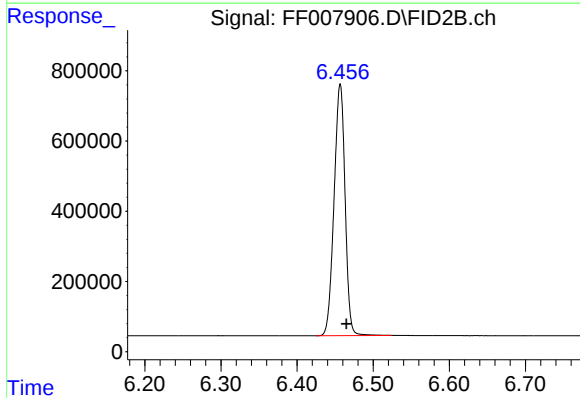


#3 N-DODECANE

R.T.: 6.457 min
Delta R.T.: -0.008 min
Response: 7203345
Conc: 52.04 ug/ml

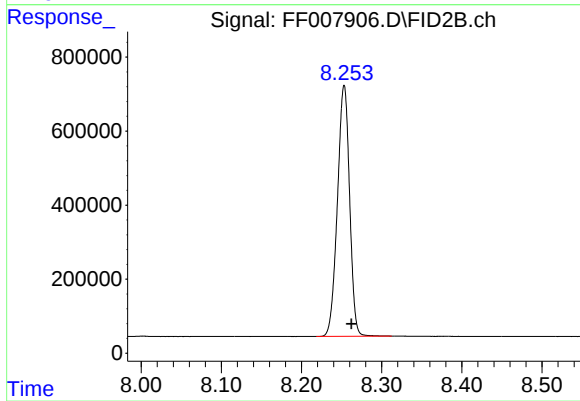

#4 N-TETRADECANE


R.T.: 8.253 min
Delta R.T.: -0.009 min
Response: 7160892
Conc: 50.71 ug/ml

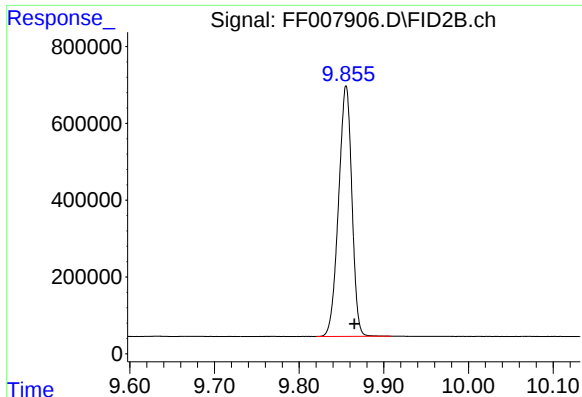

#5 N-HEXADECANE


R.T.: 9.856 min
Delta R.T.: -0.010 min
Response: 7123418
Conc: 49.01 ug/ml

Instrument :
FID_F
ClientSampleId :

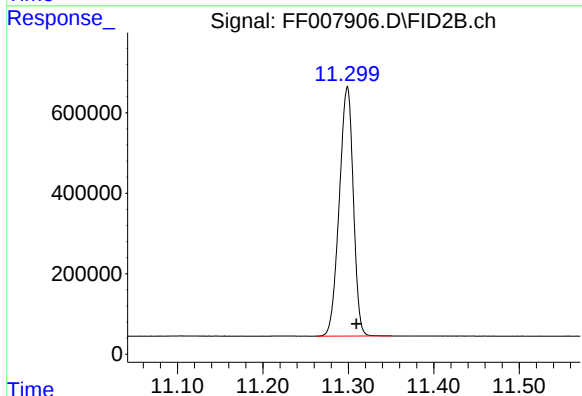


#6 N-OCTADECANE

R.T.: 11.299 min
Delta R.T.: -0.010 min
Response: 7074758
Conc: 47.67 ug/ml

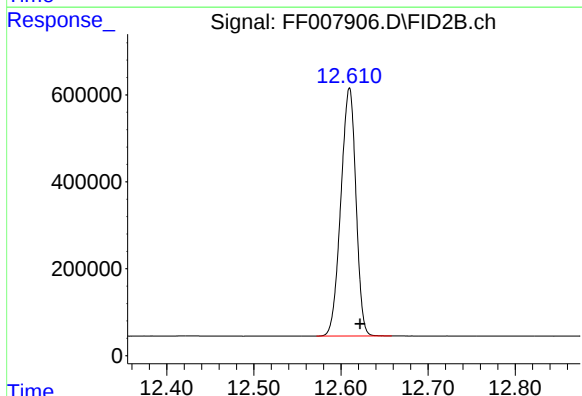


#7 N-EICOSANE

R.T.: 12.610 min
Delta R.T.: -0.012 min
Response: 6871708
Conc: 46.36 ug/ml

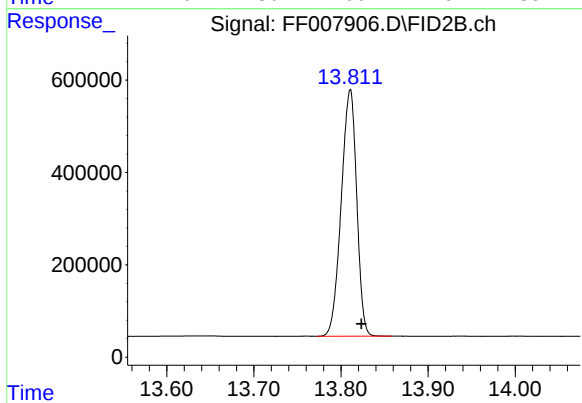

#8 N-DOCOSANE


R.T.: 13.811 min
Delta R.T.: -0.012 min
Response: 6590924
Conc: 45.24 ug/ml

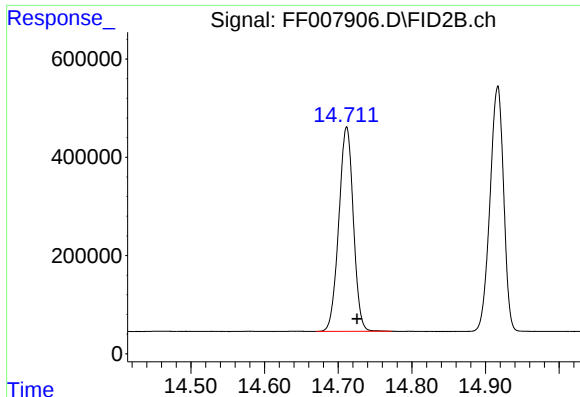

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.712 min
Delta R.T.: -0.014 min
Response: 5704893
Conc: 44.66 ug/ml

Instrument :
FID_F
ClientSampleId :

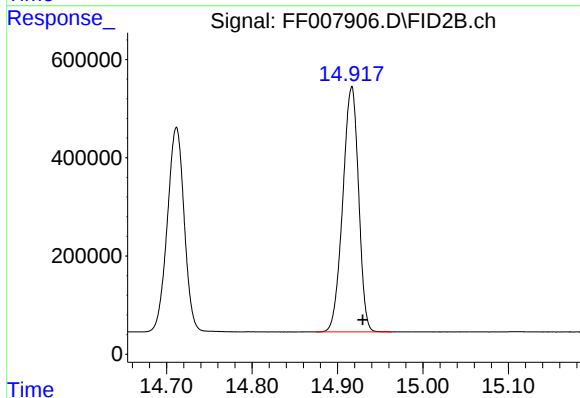


#10 N-TETRACOSANE

R.T.: 14.917 min
Delta R.T.: -0.013 min
Response: 6415331
Conc: 44.36 ug/ml

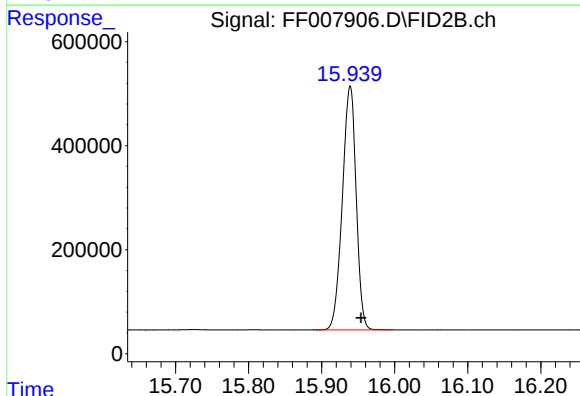


#11 N-HEXACOSANE

R.T.: 15.939 min
Delta R.T.: -0.015 min
Response: 6157074
Conc: 43.87 ug/ml

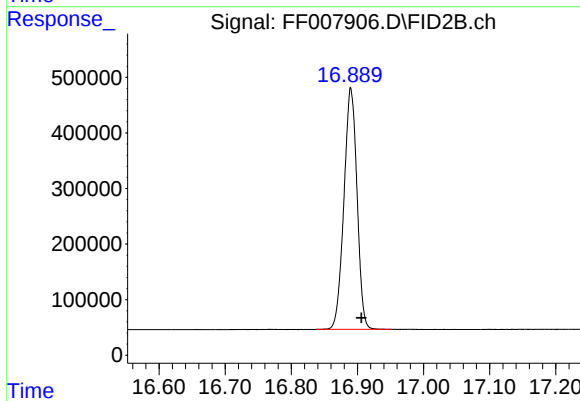

#12 N-OCTACOSANE


R.T.: 16.890 min
Delta R.T.: -0.016 min
Response: 5975190
Conc: 44.05 ug/ml

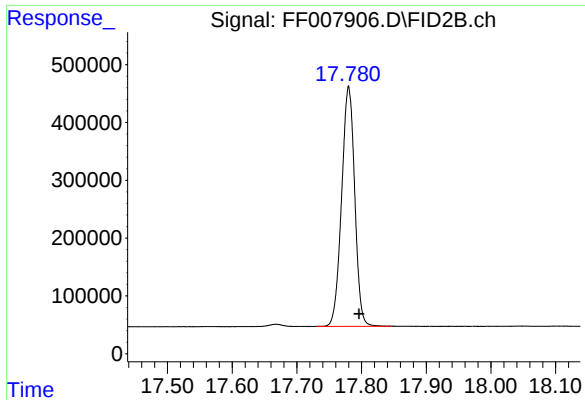

#13 N-TRIACONTANE


R.T.: 17.780 min
Delta R.T.: -0.016 min
Response: 5831546
Conc: 45.07 ug/ml

Instrument :
FID_F
ClientSampleId :

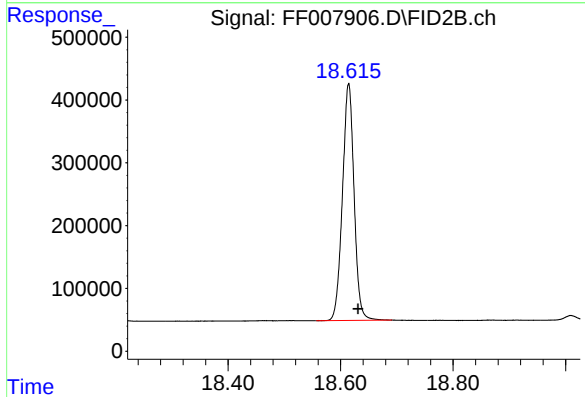


#14 N-DOTRIACONTANE

R.T.: 18.614 min
Delta R.T.: -0.017 min
Response: 5417303
Conc: 46.73 ug/ml

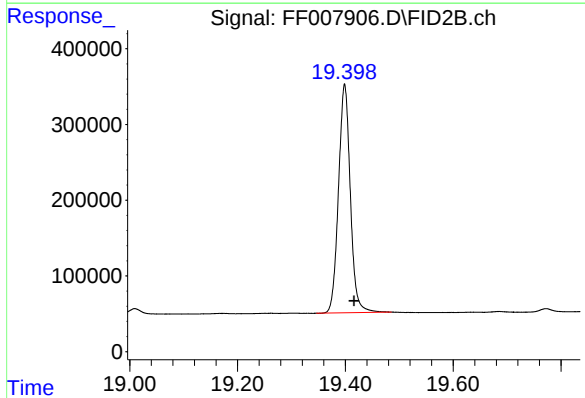


#15 N-TETRATRIACONTANE

R.T.: 19.399 min
Delta R.T.: -0.017 min
Response: 4593436
Conc: 48.90 ug/ml

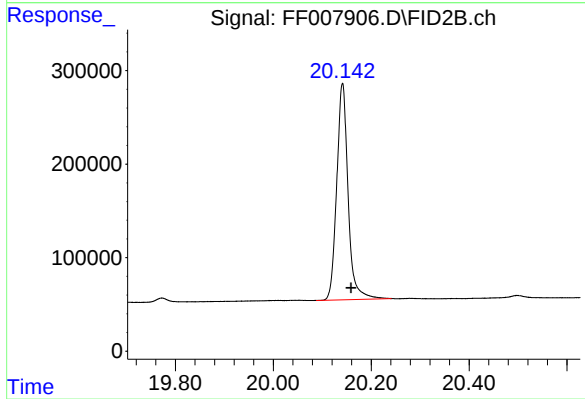

#16 N-HEXATRIACONTANE


R.T.: 20.142 min
Delta R.T.: -0.017 min
Response: 3731284
Conc: 49.12 ug/ml

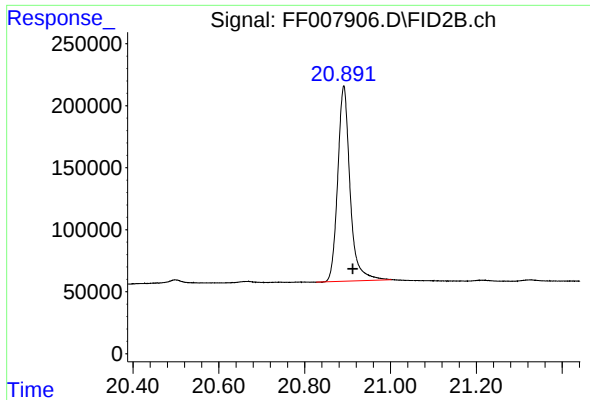

#17 N-OCTATRIACONTANE

R.T.: 20.891 min
Delta R.T.: -0.020 min
Response: 3135257
Conc: 50.46 ug/ml

Instrument :
FID_F
ClientSampleId :

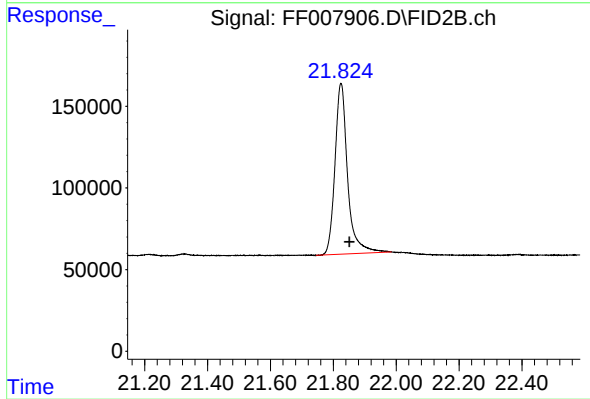

#18 N-TETRACONTANE

R.T.: 21.824 min
Delta R.T.: -0.027 min
Response: 2918536
Conc: 47.84 ug/ml