

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
 Data File : FF007909.D
 Signal(s) : FID2B.ch
 Acq On : 25 Nov 2020 12:54
 Operator : DD\AJ
 Sample : L4597-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 25 16:31:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.710	3551511	27.804 ug/ml
Target Compounds			
4) N-TETRADECANE	8.213	98569	0.698 ug/ml
7) N-EICOSANE	12.601	127598	0.861 ug/ml
10) N-TETRACOSANE	14.904	260603	1.802 ug/ml
11) N-HEXACOSANE	15.936	55399	0.395 ug/ml
12) N-OCTACOSANE	16.920	304113	2.242 ug/ml
13) N-TRIACONTANE	17.781	442332	3.419 ug/ml
14) N-DOTRIACONTANE	18.609	731240	6.308 ug/ml
15) N-TETRATRIACONTANE	19.404	774359	8.244 ug/ml
16) N-HEXATRIACONTANE	20.145	1048700	13.806 ug/ml
17) N-OCTATRIACONTANE	20.902	402293	6.475 ug/ml
18) N-TETRACONTANE	21.836	595518	9.761 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
Data File : FF007909.D
Signal(s) : FID2B.ch
Acq On : 25 Nov 2020 12:54
Operator : DD\AJ
Sample : L4597-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 25 16:31:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

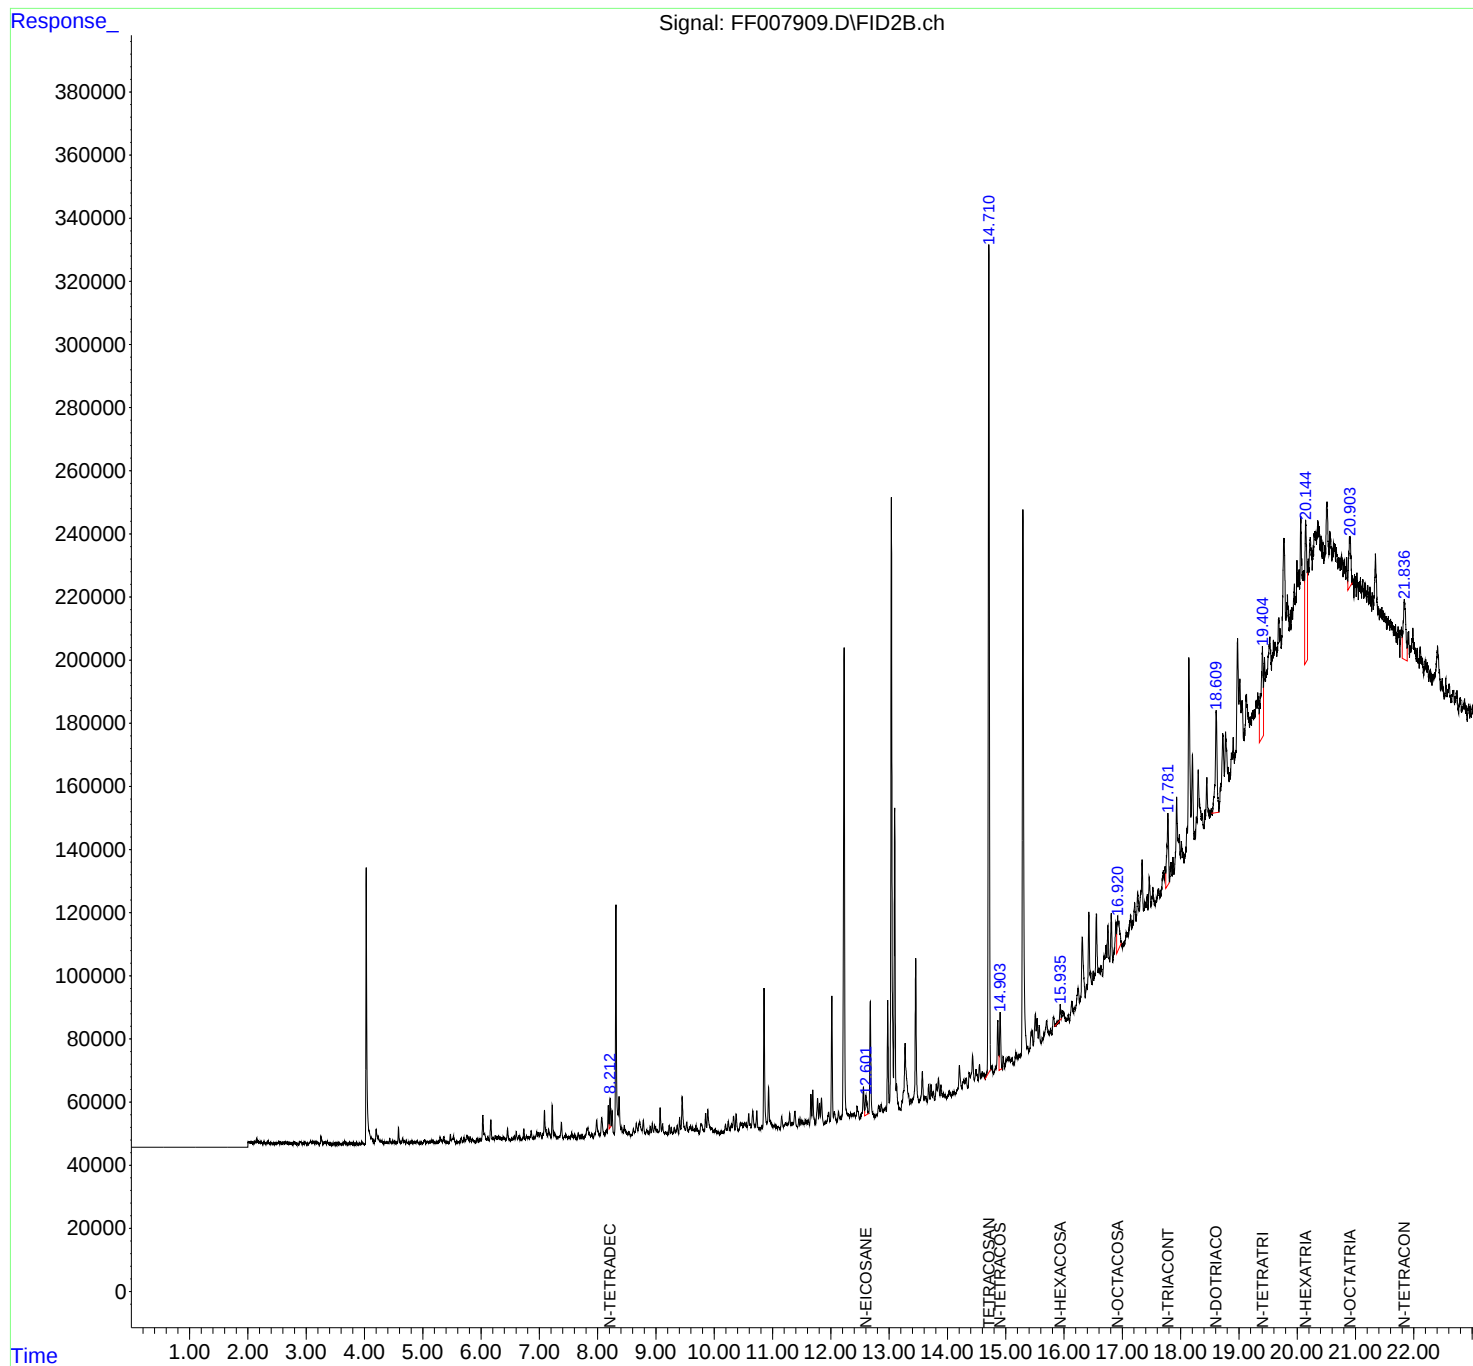


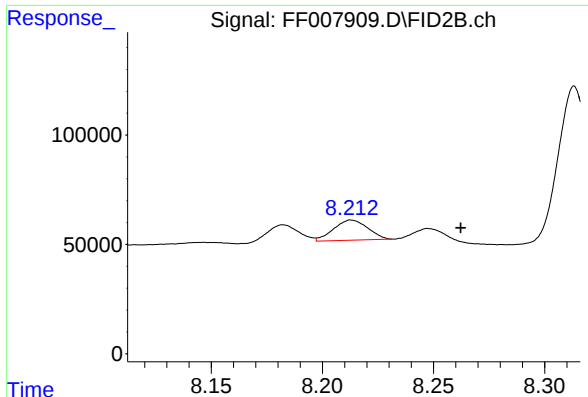

#4 N-TETRADECANE


R.T.: 8.213 min
Delta R.T.: -0.049 min
Response: 98569
Conc: 0.70 ug/ml

Instrument :
FID_F
ClientSampleId :

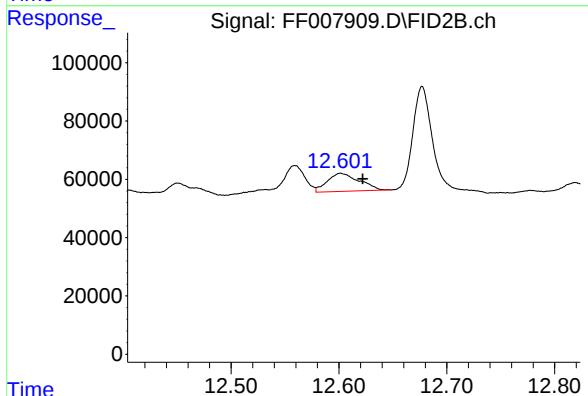


#7 N-EICOSANE

R.T.: 12.601 min
Delta R.T.: -0.020 min
Response: 127598
Conc: 0.86 ug/ml

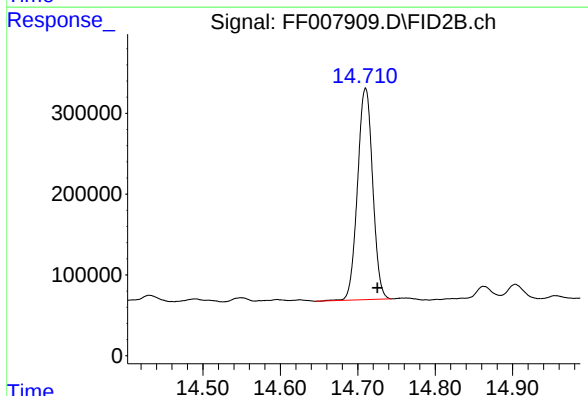


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.710 min
Delta R.T.: -0.015 min
Response: 3551511
Conc: 27.80 ug/ml

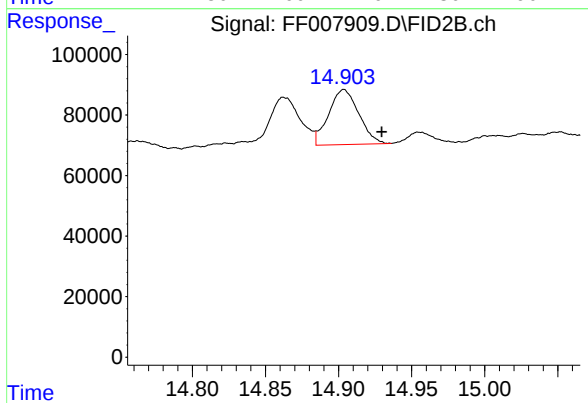

#10 N-TETRACOSANE


R.T.: 14.904 min
Delta R.T.: -0.026 min
Response: 260603
Conc: 1.80 ug/ml

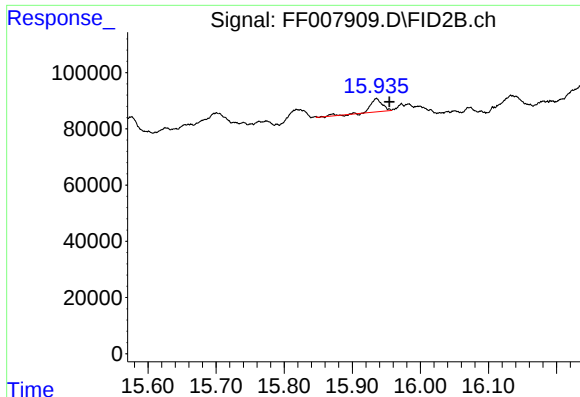

#11 N-HEXACOSANE


R.T.: 15.936 min
Delta R.T.: -0.019 min
Response: 55399
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :

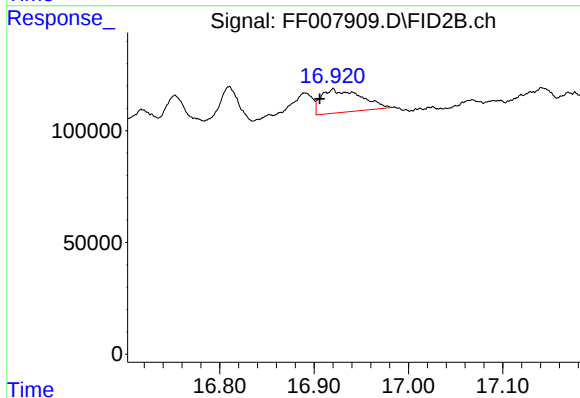


#12 N-OCTACOSANE

R.T.: 16.920 min
Delta R.T.: 0.014 min
Response: 304113
Conc: 2.24 ug/ml

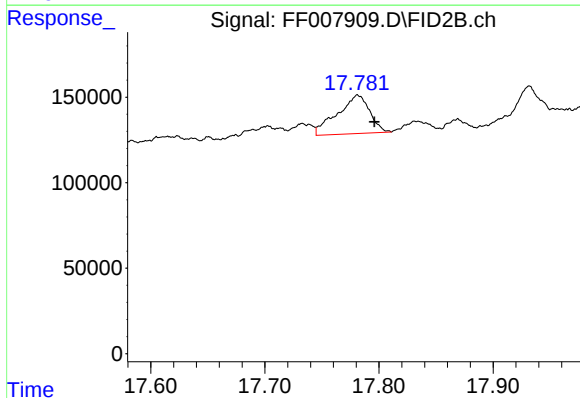


#13 N-TRIACONTANE

R.T.: 17.781 min
Delta R.T.: -0.015 min
Response: 442332
Conc: 3.42 ug/ml

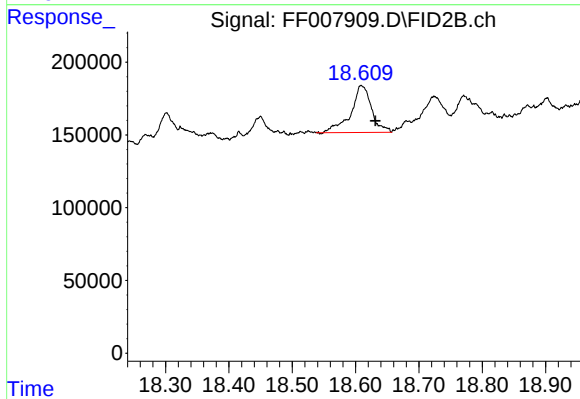

#14 N-DOTRIACONTANE

R.T.: 18.609 min
Delta R.T.: -0.022 min
Response: 731240
Conc: 6.31 ug/ml

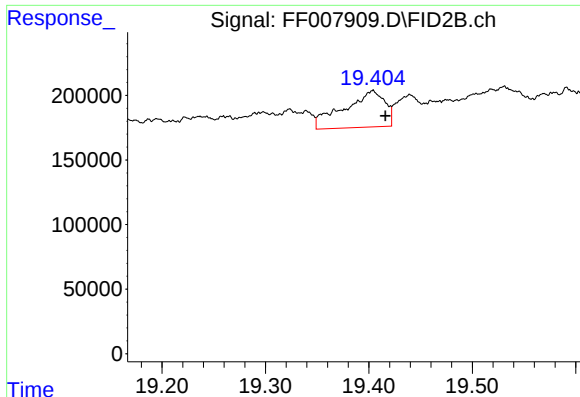

#15 N-TETRATRIACONTANE


R.T.: 19.404 min

Delta R.T.: -0.012 min

Response: 774359

Conc: 8.24 ug/ml

Instrument :
FID_F
ClientSampleId :

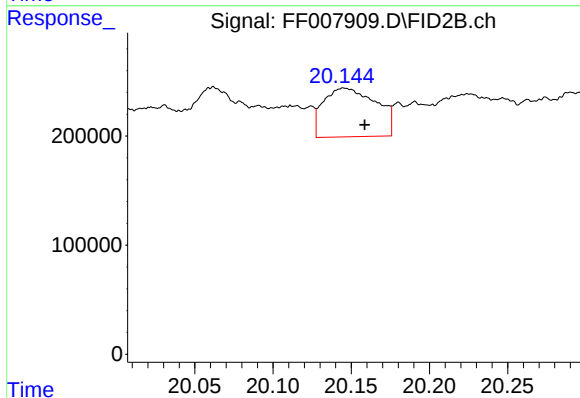


#16 N-HEXATRIACONTANE

R.T.: 20.145 min

Delta R.T.: -0.013 min

Response: 1048700

Conc: 13.81 ug/ml

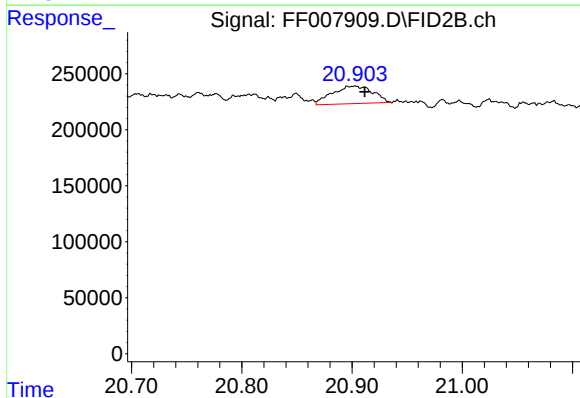


#17 N-OCTATRIACONTANE

R.T.: 20.902 min

Delta R.T.: -0.009 min

Response: 402293

Conc: 6.47 ug/ml

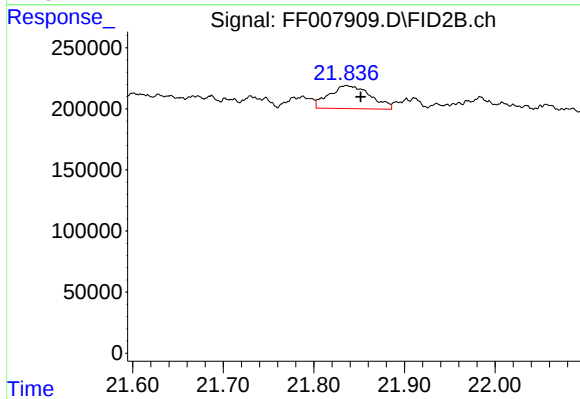

#18 N-TETRACONTANE

R.T.: 21.836 min

Delta R.T.: -0.016 min

Response: 595518

Conc: 9.76 ug/ml