

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
 Data File : FF007910.D
 Signal(s) : FID2B.ch
 Acq On : 25 Nov 2020 13:25
 Operator : DD\AJ
 Sample : L4891-05
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 25 16:31:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	1557684	12.195 ug/ml
Target Compounds			
4) N-TETRADECANE	8.316f	796621	5.641 ug/ml
7) N-EICOSANE	12.682f	97118	0.655 ug/ml
14) N-DOTRIACONTANE	18.606	207018	1.786 ug/ml
15) N-TETRATRIACONTANE	19.402	72470	0.772 ug/ml
16) N-HEXATRIACONTANE	20.127	232142	3.056 ug/ml
17) N-OCTATRIACONTANE	20.847f	87823	1.413 ug/ml
18) N-TETRACONTANE	21.836	923855	15.143 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
Data File : FF007910.D
Signal(s) : FID2B.ch
Acq On : 25 Nov 2020 13:25
Operator : DD\AJ
Sample : L4891-05
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 25 16:31:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

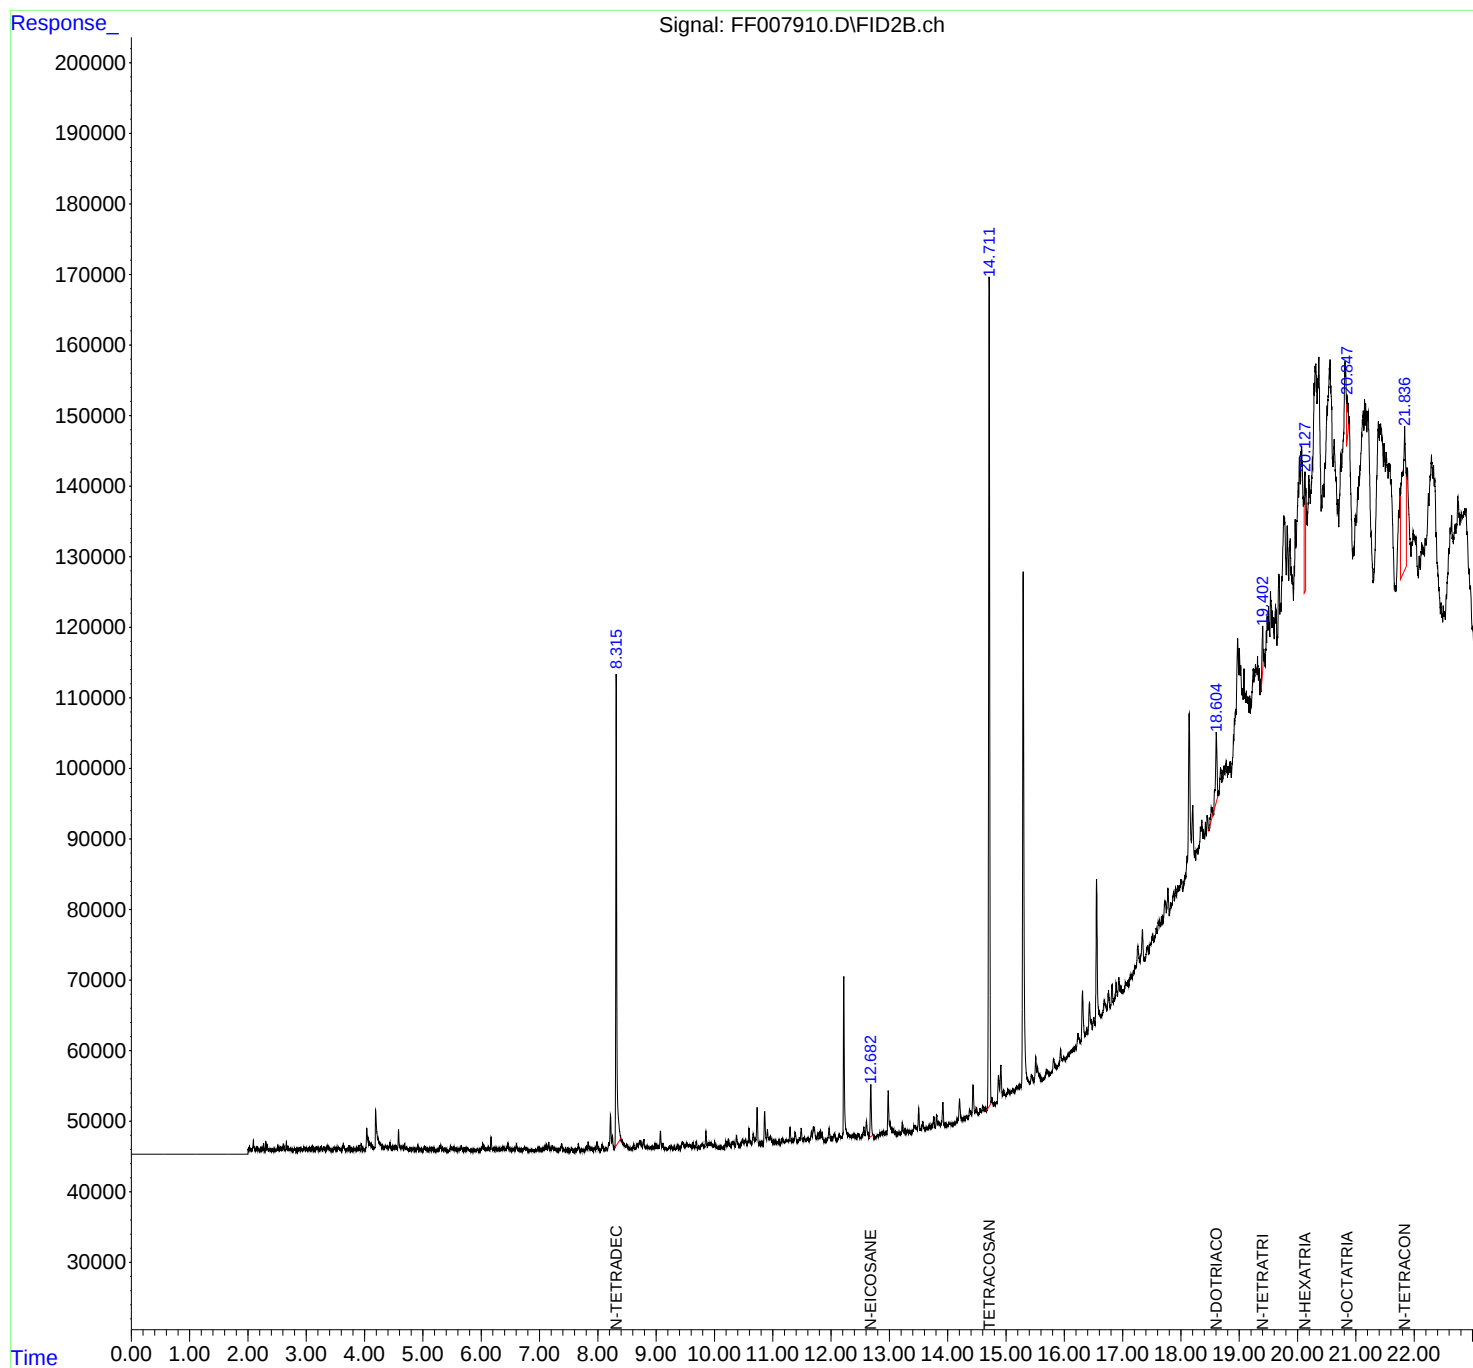


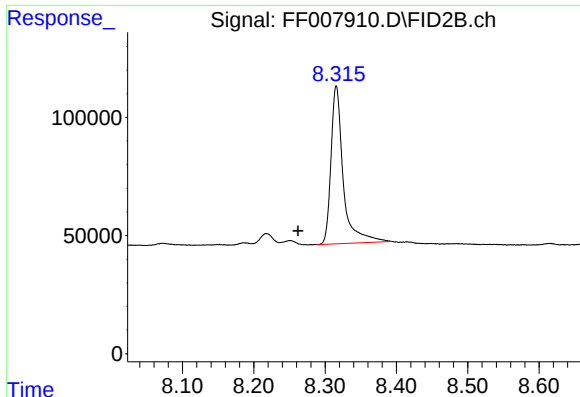

#4 N-TETRADECANE


R.T.: 8.316 min
Delta R.T.: 0.053 min
Response: 796621
Conc: 5.64 ug/ml

Instrument :
FID_F
ClientSampleId :

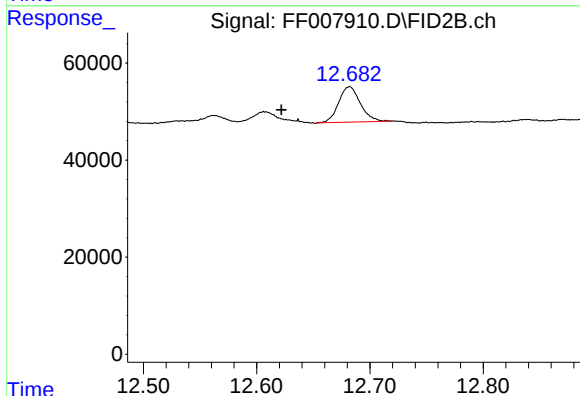


#7 N-EICOSANE

R.T.: 12.682 min
Delta R.T.: 0.060 min
Response: 97118
Conc: 0.66 ug/ml

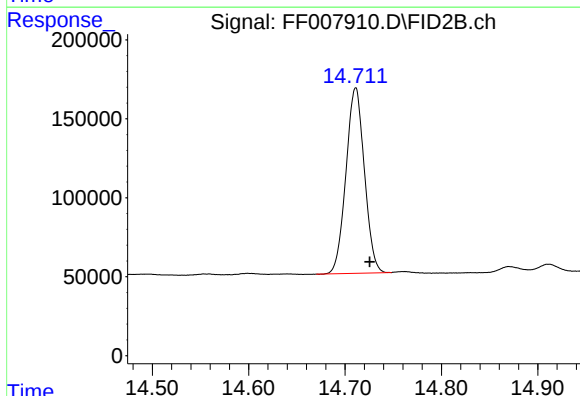


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.711 min
Delta R.T.: -0.014 min
Response: 1557684
Conc: 12.19 ug/ml

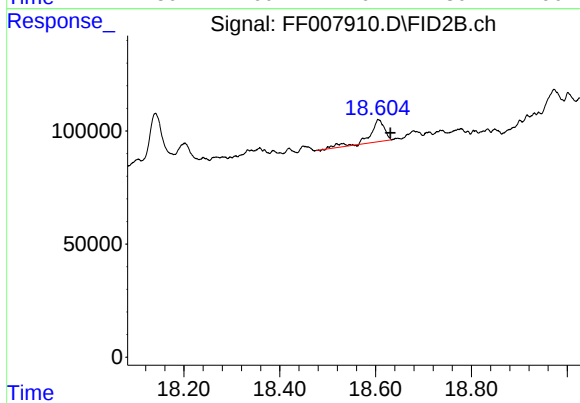

#14 N-DOTRIACONTANE


R.T.: 18.606 min
Delta R.T.: -0.025 min
Response: 207018
Conc: 1.79 ug/ml

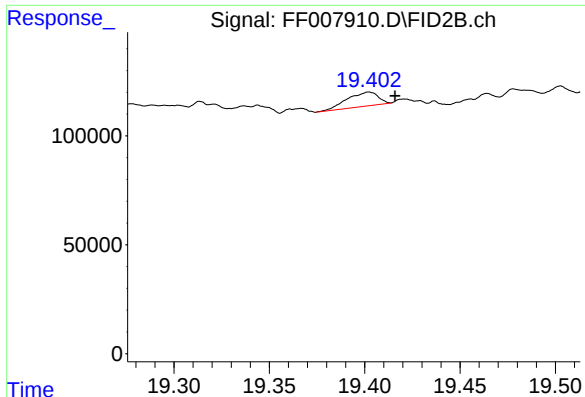

#15 N-TETRATRIACONTANE


R.T.: 19.402 min
Delta R.T.: -0.014 min
Response: 72470
Conc: 0.77 ug/ml

Instrument :
FID_F
ClientSampleId :

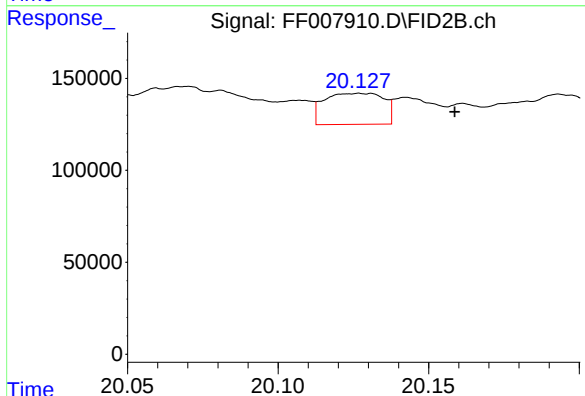


#16 N-HEXATRIACONTANE

R.T.: 20.127 min
Delta R.T.: -0.032 min
Response: 232142
Conc: 3.06 ug/ml

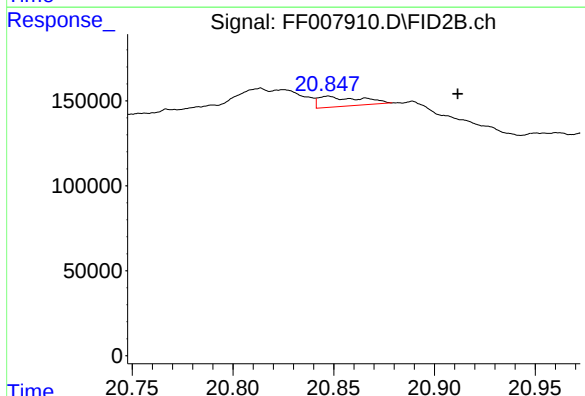

#17 N-OCTATRIACONTANE

R.T.: 20.847 min
Delta R.T.: -0.064 min
Response: 87823
Conc: 1.41 ug/ml

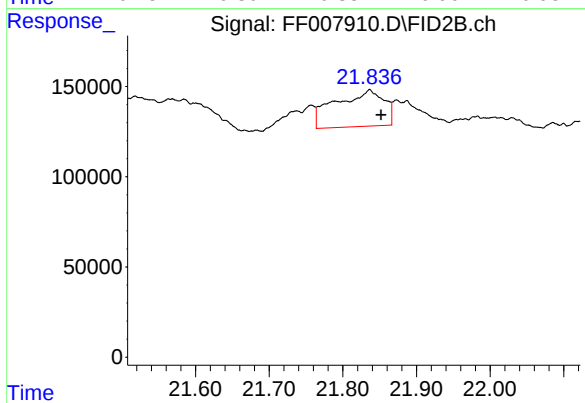

#18 N-TETRACONTANE

R.T.: 21.836 min
Delta R.T.: -0.015 min
Response: 923855
Conc: 15.14 ug/ml