

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
 Data File : FF007912.D
 Signal(s) : FID2B.ch
 Acq On : 25 Nov 2020 14:26
 Operator : DD\AJ
 Sample : L4880-08
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 25 16:32:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	2097438	16.420 ug/ml
Target Compounds			
4) N-TETRADECANE	8.316f	1125910	7.973 ug/ml
12) N-OCTACOSANE	16.939	214307	1.580 ug/ml
14) N-DOTRIACONTANE	18.608	131636	1.136 ug/ml
16) N-HEXATRIACONTANE	20.143	233949	3.080 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
Data File : FF007912.D
Signal(s) : FID2B.ch
Acq On : 25 Nov 2020 14:26
Operator : DD\AJ
Sample : L4880-08
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 25 16:32:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

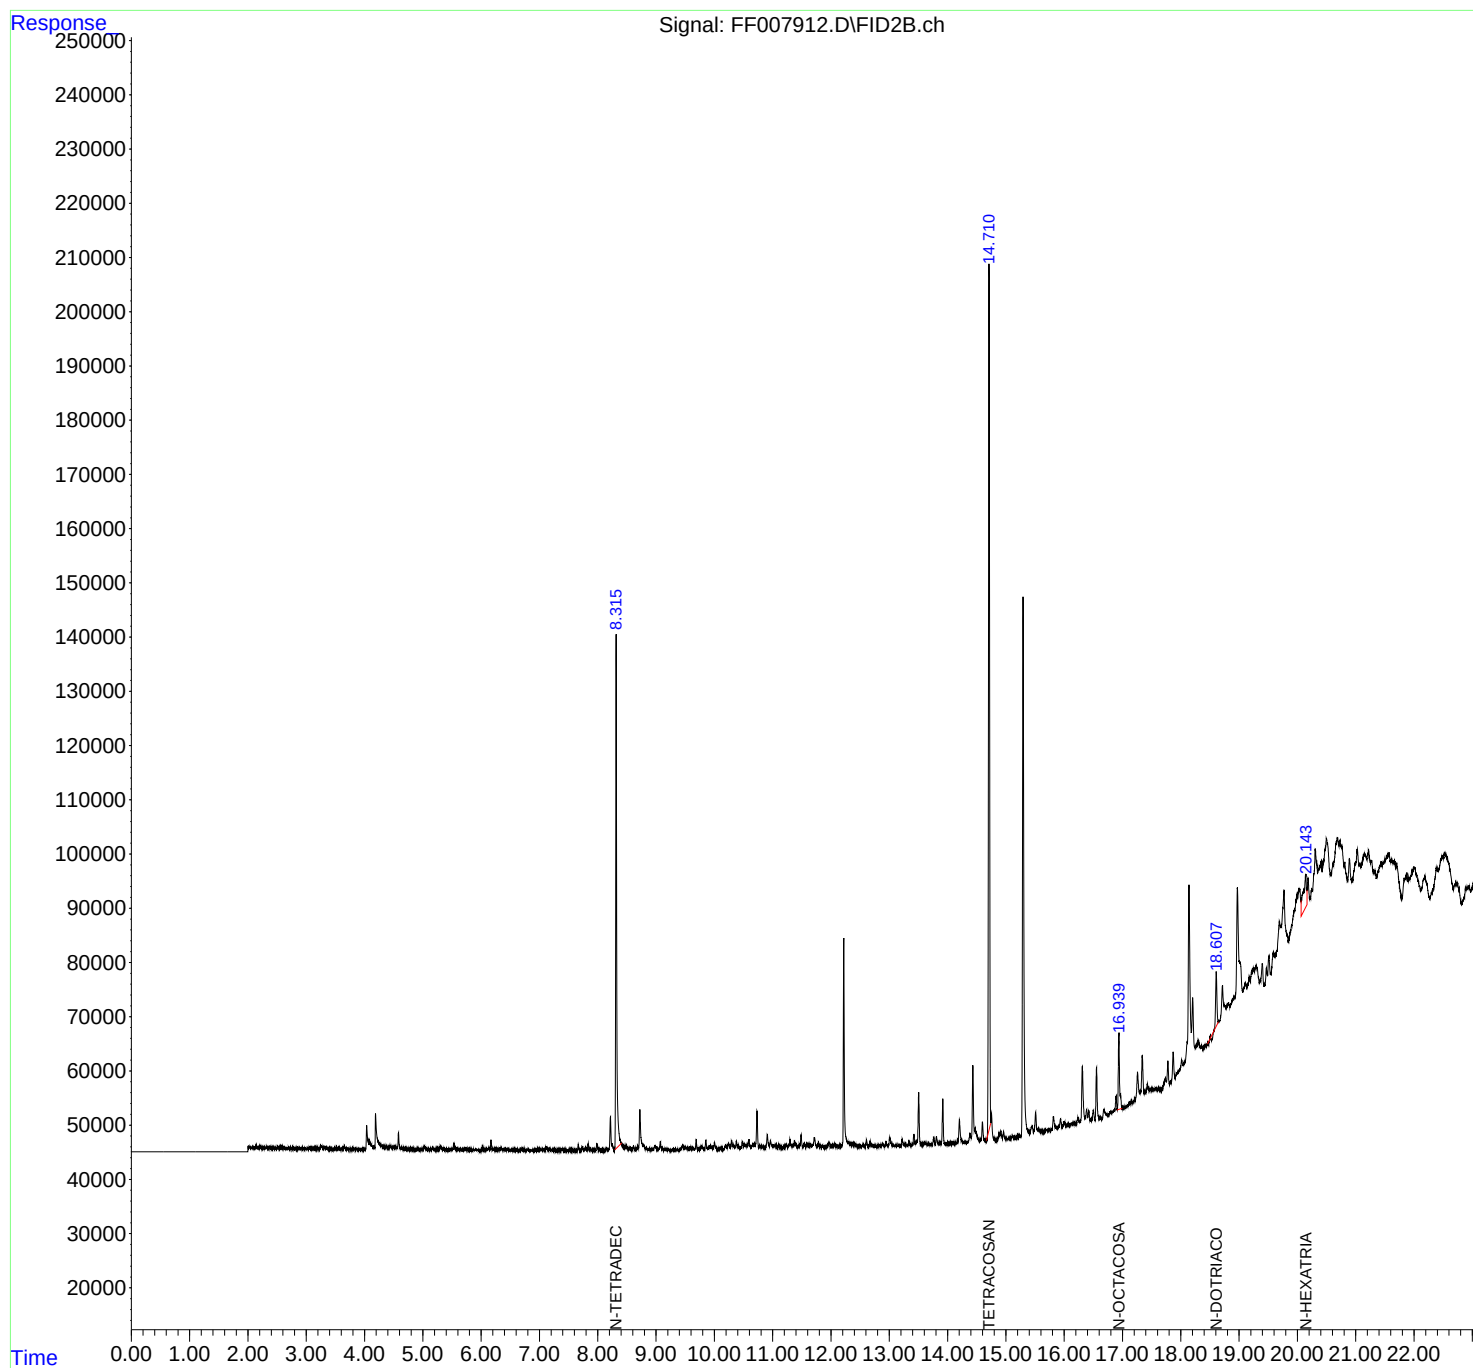


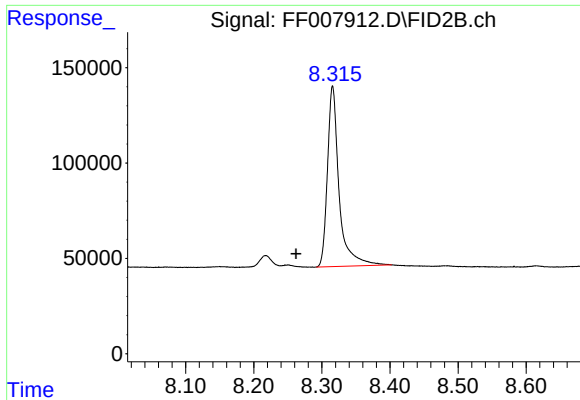

#4 N-TETRADECANE


R.T.: 8.316 min
Delta R.T.: 0.054 min
Response: 1125910
Conc: 7.97 ug/ml

Instrument :
FID_F
ClientSampleId :

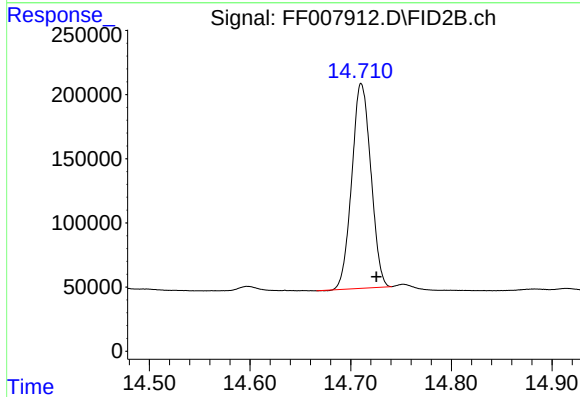


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.711 min
Delta R.T.: -0.015 min
Response: 2097438
Conc: 16.42 ug/ml

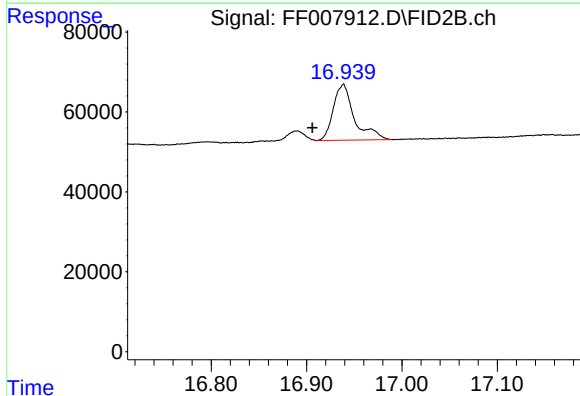


#12 N-OCTACOSANE

R.T.: 16.939 min
Delta R.T.: 0.033 min
Response: 214307
Conc: 1.58 ug/ml

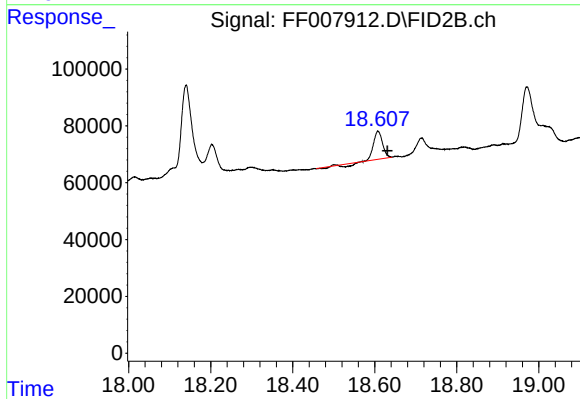

#14 N-DOTRIACONTANE

R.T.: 18.608 min
Delta R.T.: -0.023 min
Response: 131636
Conc: 1.14 ug/ml

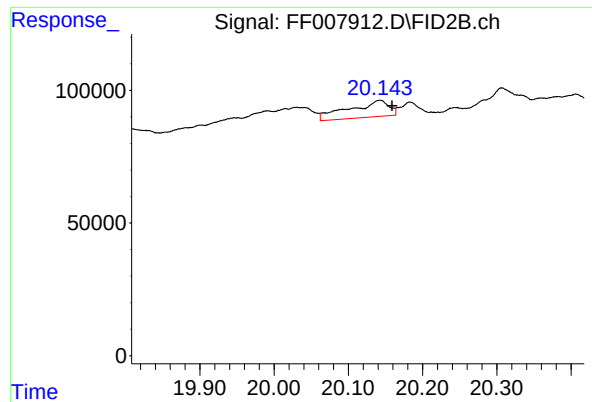

#16 N-HEXATRIACONTANE

R.T.: 20.143 min
Delta R.T.: -0.016 min
Response: 233949
Conc: 3.08 ug/ml

Instrument :
FID_F
ClientSampleId :