

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
 Data File : FF007916.D
 Signal(s) : FID2B.ch
 Acq On : 25 Nov 2020 16:34
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 25 16:49:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	2198457	17.211 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.780	105213	0.813 ug/ml
14) N-DOTRIACONTANE	18.613	177787	1.534 ug/ml
15) N-TETRATRIACONTANE	19.401	338587	3.605 ug/ml
17) N-OCTATRIACONTANE	20.892	228111	3.671 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
Data File : FF007916.D
Signal(s) : FID2B.ch
Acq On : 25 Nov 2020 16:34
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 25 16:49:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

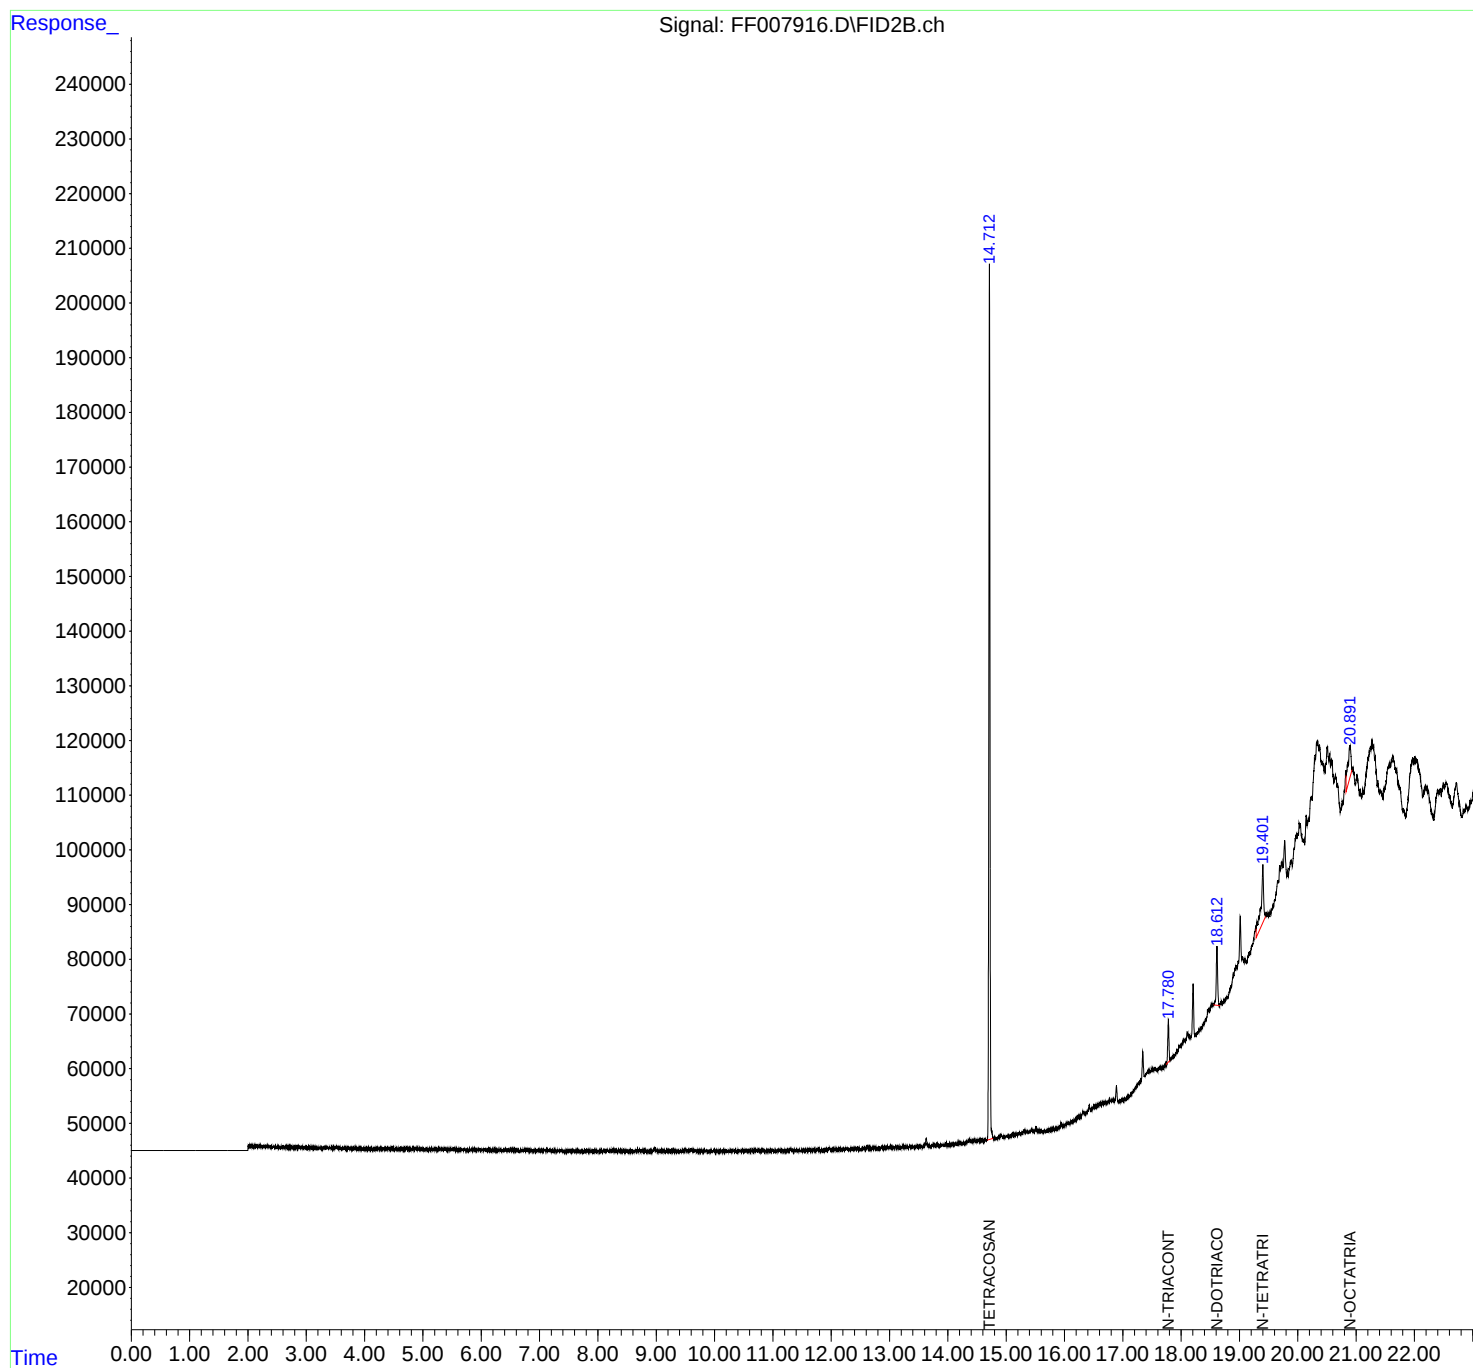


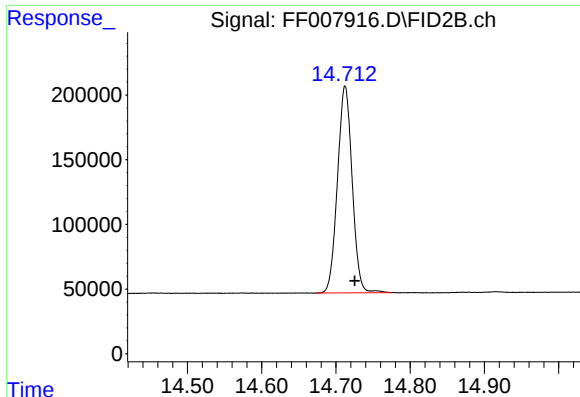

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.712 min
Delta R.T.: -0.013 min
Response: 2198457
Conc: 17.21 ug/ml

Instrument :
FID_F
ClientSampleId :

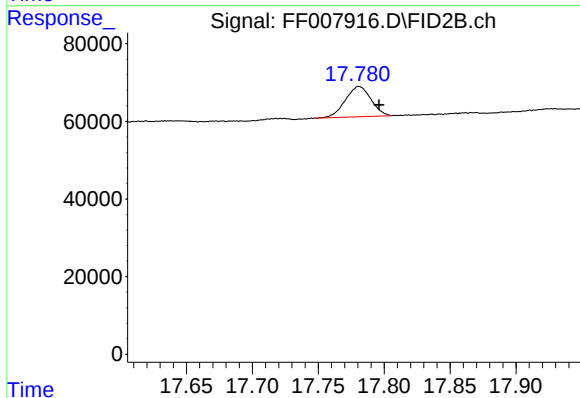


#13 N-TRIACONTANE

R.T.: 17.780 min
Delta R.T.: -0.016 min
Response: 105213
Conc: 0.81 ug/ml

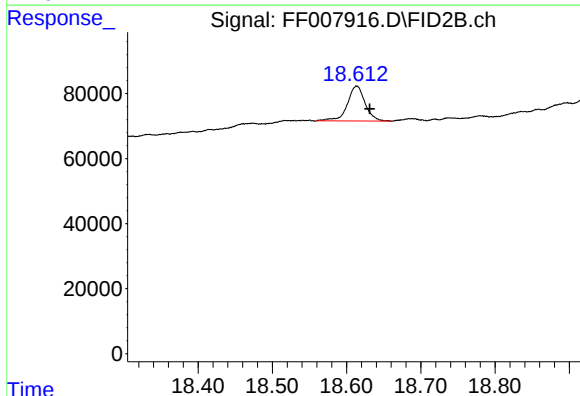


#14 N-DOTRIACONTANE

R.T.: 18.613 min
Delta R.T.: -0.018 min
Response: 177787
Conc: 1.53 ug/ml

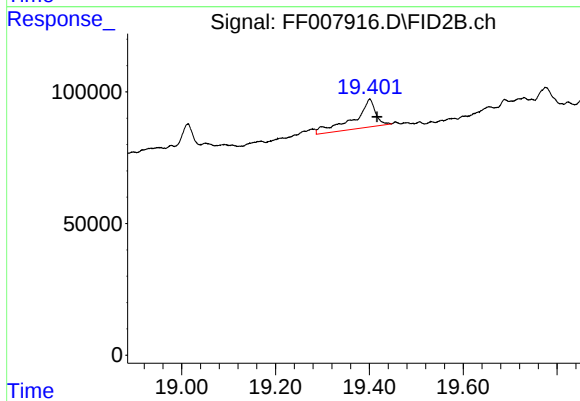

#15 N-TETRATRIACONTANE

R.T.: 19.401 min
Delta R.T.: -0.015 min
Response: 338587
Conc: 3.60 ug/ml

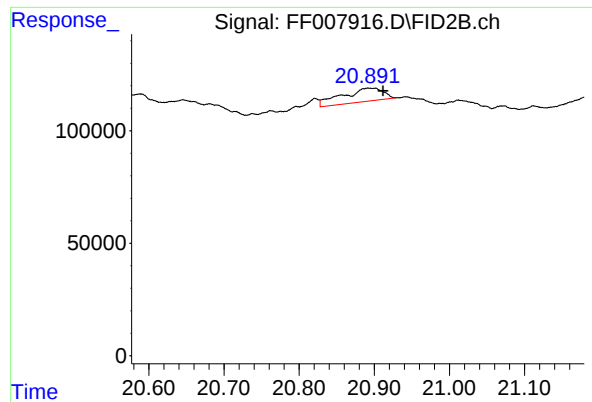

#17 N-OCTATRIACONTANE

R.T.: 20.892 min
Delta R.T.: -0.020 min
Response: 228111
Conc: 3.67 ug/ml

Instrument :
FID_F
ClientSampleId :