

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
 Data File : FF007919.D
 Signal(s) : FID2B.ch
 Acq On : 25 Nov 2020 18:07
 Operator : DD\AJ
 Sample : L4880-06MSD
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 KENS-B4-112320-0-2MSD

Integration File: autoint1.e
 Quant Time: Nov 26 00:33:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
 Quant Title :
 QLast Update : Tue Nov 03 01:29:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.711	1930542	15.114 ug/ml
Target Compounds			
2) N-DECANE	4.433	3032485	22.288 ug/ml
3) N-DODECANE	6.456	3083100	22.274 ug/ml
4) N-TETRADECANE	8.253	3107677	22.007 ug/ml
5) N-HEXADECANE	9.854	3054143	21.014 ug/ml
6) N-OCTADECANE	11.298	3049942	20.551 ug/ml
7) N-EICOSANE	12.611	3018325	20.363 ug/ml
8) N-DOCOSANE	13.812	2928129	20.098 ug/ml
10) N-TETRACOSANE	14.916	2818113	19.487 ug/ml
11) N-HEXACOSANE	15.939	2702811	19.257 ug/ml
12) N-OCTACOSANE	16.892	2689271	19.827 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112520\
Data File : FF007919.D
Signal(s) : FID2B.ch
Acq On : 25 Nov 2020 18:07
Operator : DD\AJ
Sample : L4880-06MSD
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
KENS-B4-112320-0-2MSD

Integration File: autoint1.e
Quant Time: Nov 26 00:33:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110220.M
Quant Title :
QLast Update : Tue Nov 03 01:29:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

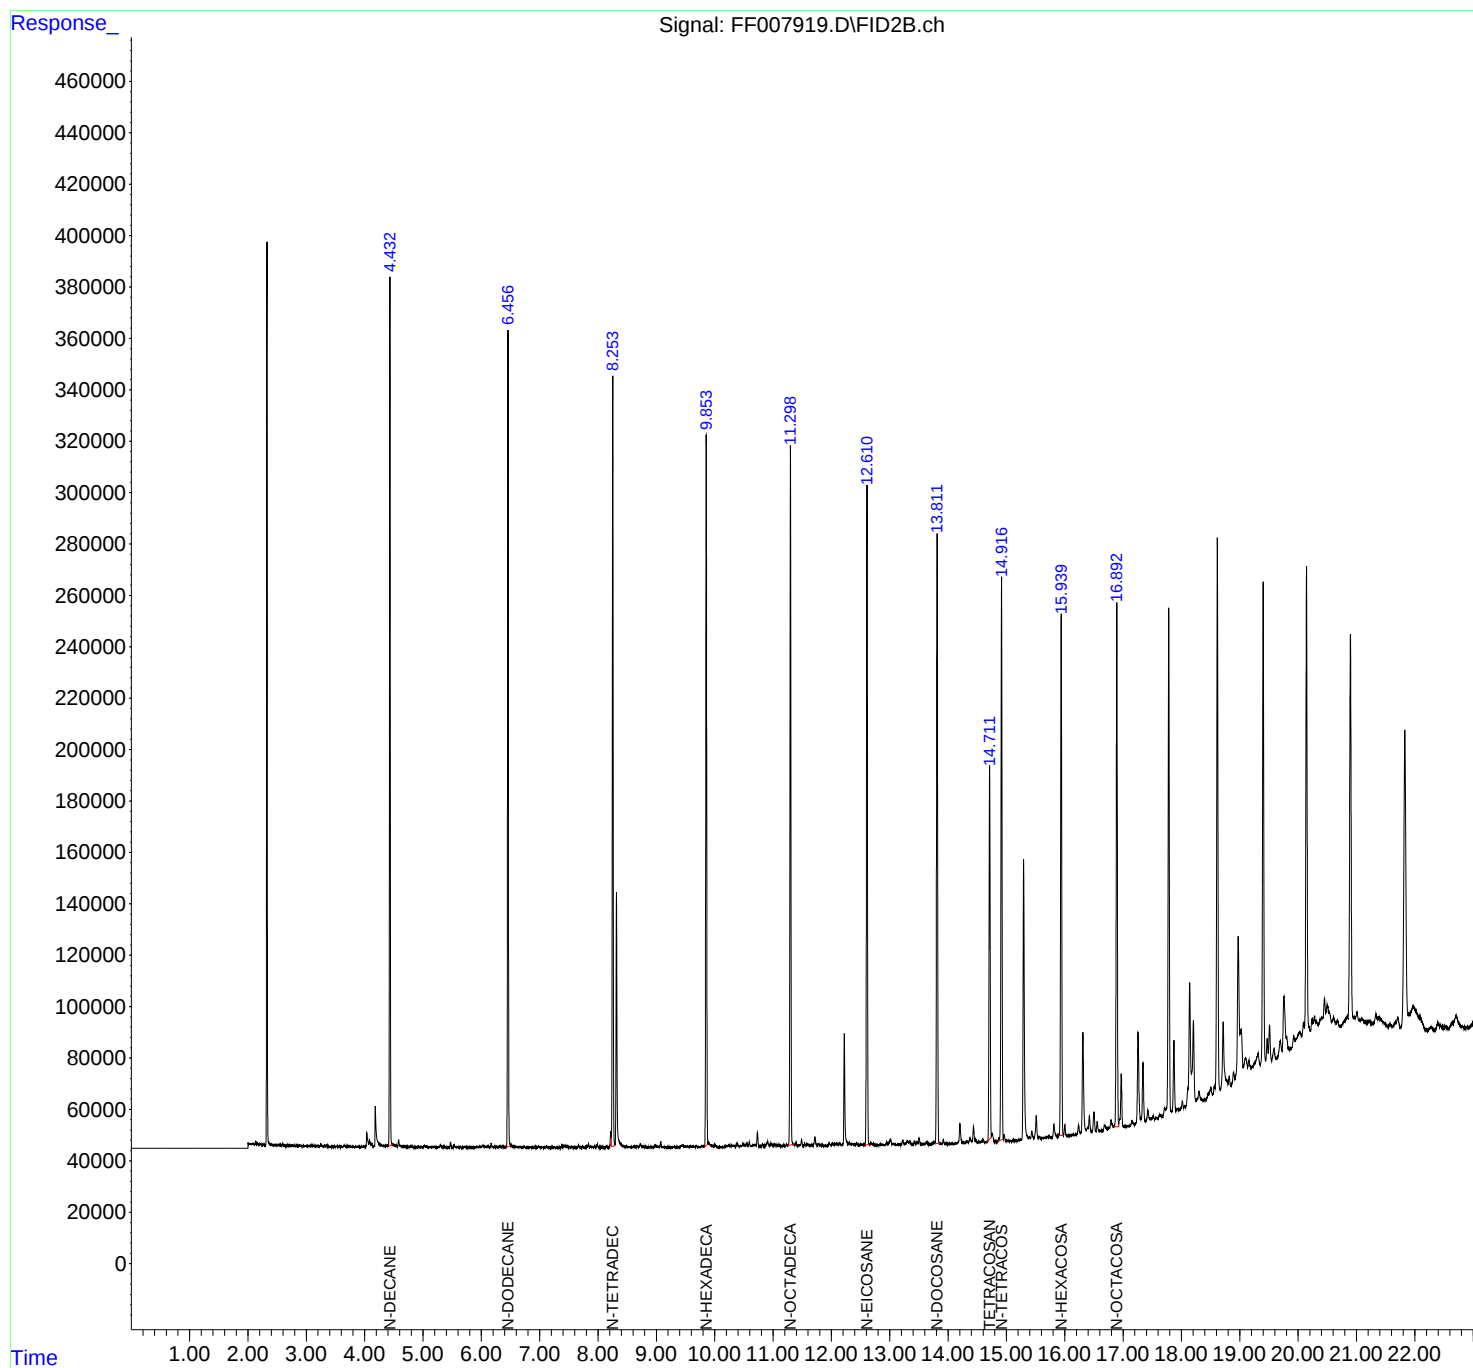


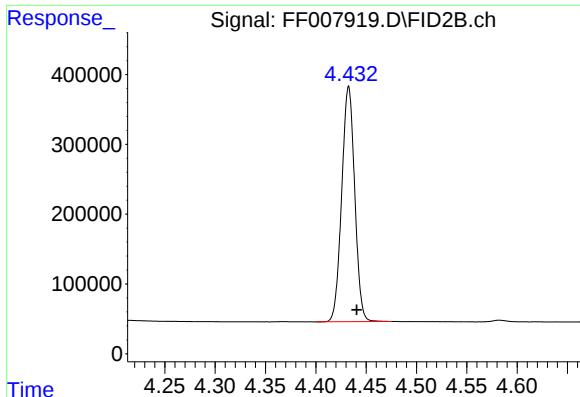

#2 N-DECANE


R.T.: 4.433 min
Delta R.T.: -0.008 min
Response: 3032485
Conc: 22.29 ug/ml

Instrument :
FID_F
ClientSampleId :
KENS-B4-112320-0-2MSD

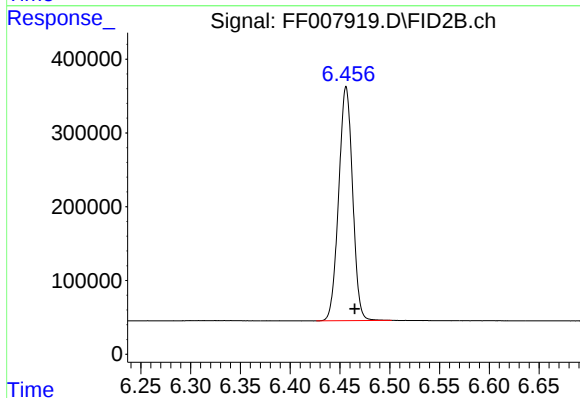


#3 N-DODECANE

R.T.: 6.456 min
Delta R.T.: -0.009 min
Response: 3083100
Conc: 22.27 ug/ml

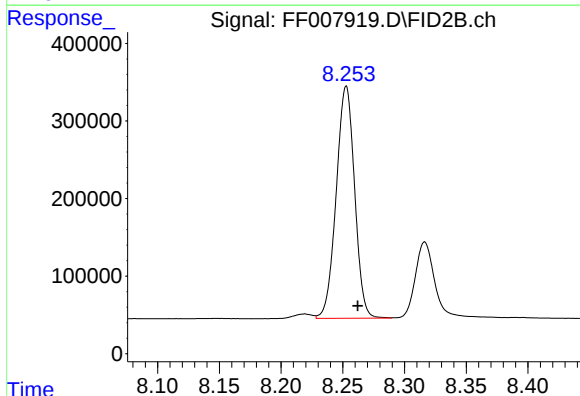


#4 N-TETRADECANE

R.T.: 8.253 min
Delta R.T.: -0.009 min
Response: 3107677
Conc: 22.01 ug/ml

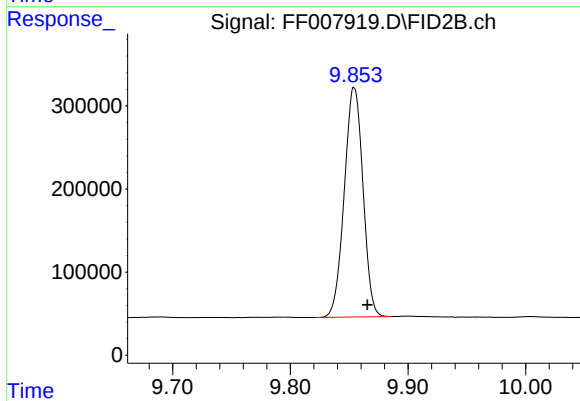

#5 N-HEXADECANE


R.T.: 9.854 min
Delta R.T.: -0.011 min
Response: 3054143
Conc: 21.01 ug/ml

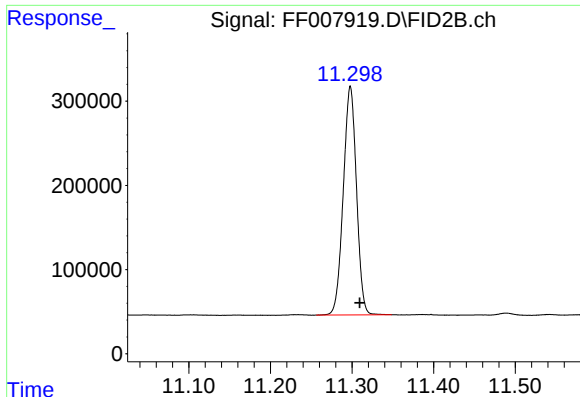

#6 N-OCTADECANE


R.T.: 11.298 min
Delta R.T.: -0.011 min
Response: 3049942
Conc: 20.55 ug/ml

Instrument :
FID_F
ClientSampleId :
KENS-B4-112320-0-2MSD

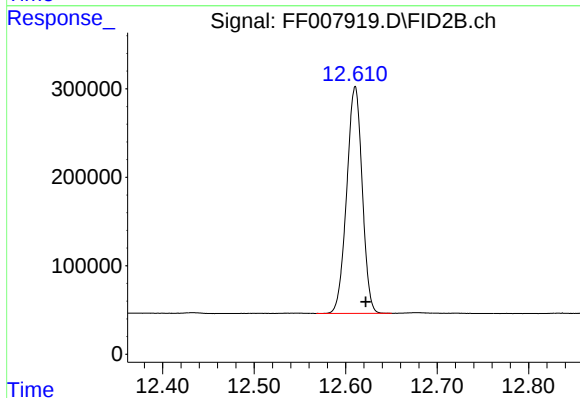


#7 N-EICOSANE

R.T.: 12.611 min
Delta R.T.: -0.011 min
Response: 3018325
Conc: 20.36 ug/ml

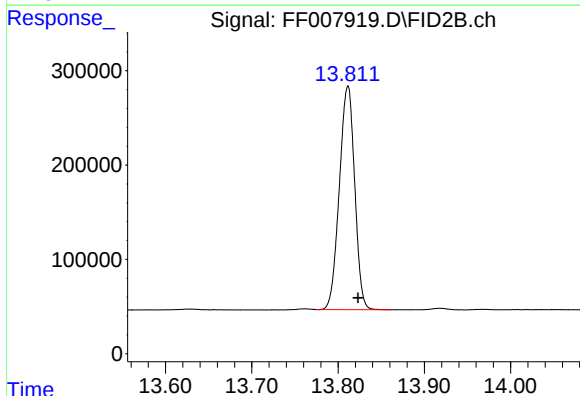


#8 N-DOCOSANE

R.T.: 13.812 min
Delta R.T.: -0.012 min
Response: 2928129
Conc: 20.10 ug/ml

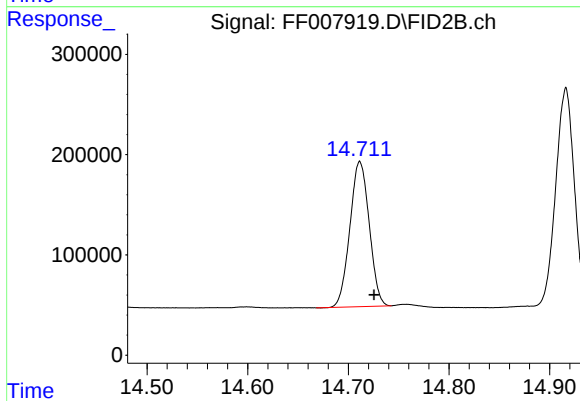

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.711 min
Delta R.T.: -0.014 min
Response: 1930542
Conc: 15.11 ug/ml

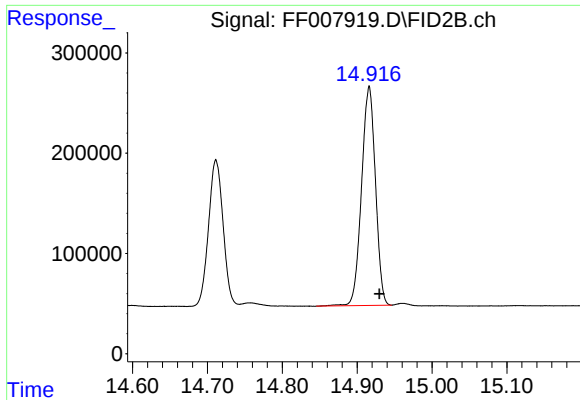

#10 N-TETRACOSANE


R.T.: 14.916 min
Delta R.T.: -0.013 min
Response: 2818113
Conc: 19.49 ug/ml

Instrument :
FID_F
ClientSampleId :
KENS-B4-112320-0-2MSD

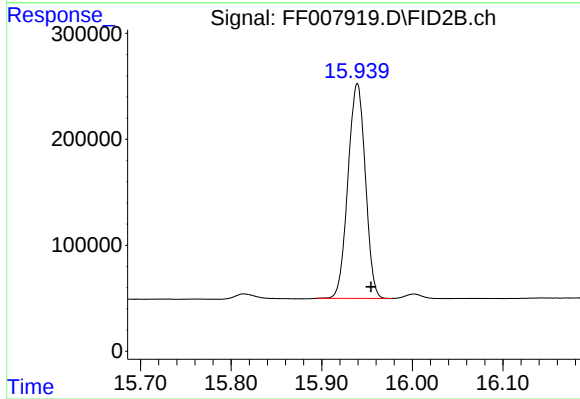

#11 N-HEXACOSANE

R.T.: 15.939 min
Delta R.T.: -0.015 min
Response: 2702811
Conc: 19.26 ug/ml

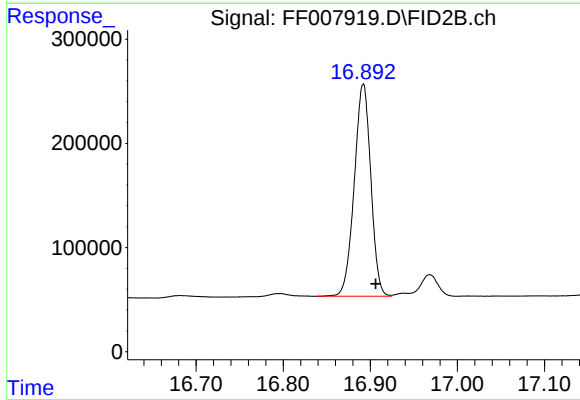

#12 N-OCTACOSANE

R.T.: 16.892 min
Delta R.T.: -0.014 min
Response: 2689271
Conc: 19.83 ug/ml