

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112618\
 Data File : FF002782.D
 Signal(s) : FID2B.ch
 Acq On : 26 Nov 2018 15:52
 Operator : AJ\SJ
 Sample : J5770-05RE 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 27 01:23:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	421409	5.395 ug/ml
Target Compounds			
4) N-TETRADECANE	8.242f	140382	1.215 ug/ml
5) N-HEXADECANE	9.793	120589	1.103 ug/ml
7) N-EICOSANE	12.599f	2983892	30.818 ug/ml
8) N-DOCOSANE	13.763	284946	3.112 ug/ml
10) N-TETRACOSANE	14.821	1236157	13.876 ug/ml
11) N-HEXACOSANE	15.879	141137	1.555 ug/ml
12) N-OCTACOSANE	16.823	433853	4.549 ug/ml
13) N-TRIACONTANE	17.724	202652	2.044 ug/ml
14) N-DOTRIACONTANE	18.556	185714	1.876 ug/ml
15) N-TETRATRIACONTANE	19.346	138262	1.401 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112618\
Data File : FF002782.D
Signal(s) : FID2B.ch
Acq On : 26 Nov 2018 15:52
Operator : AJ\SJ
Sample : J5770-05RE 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 27 01:23:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

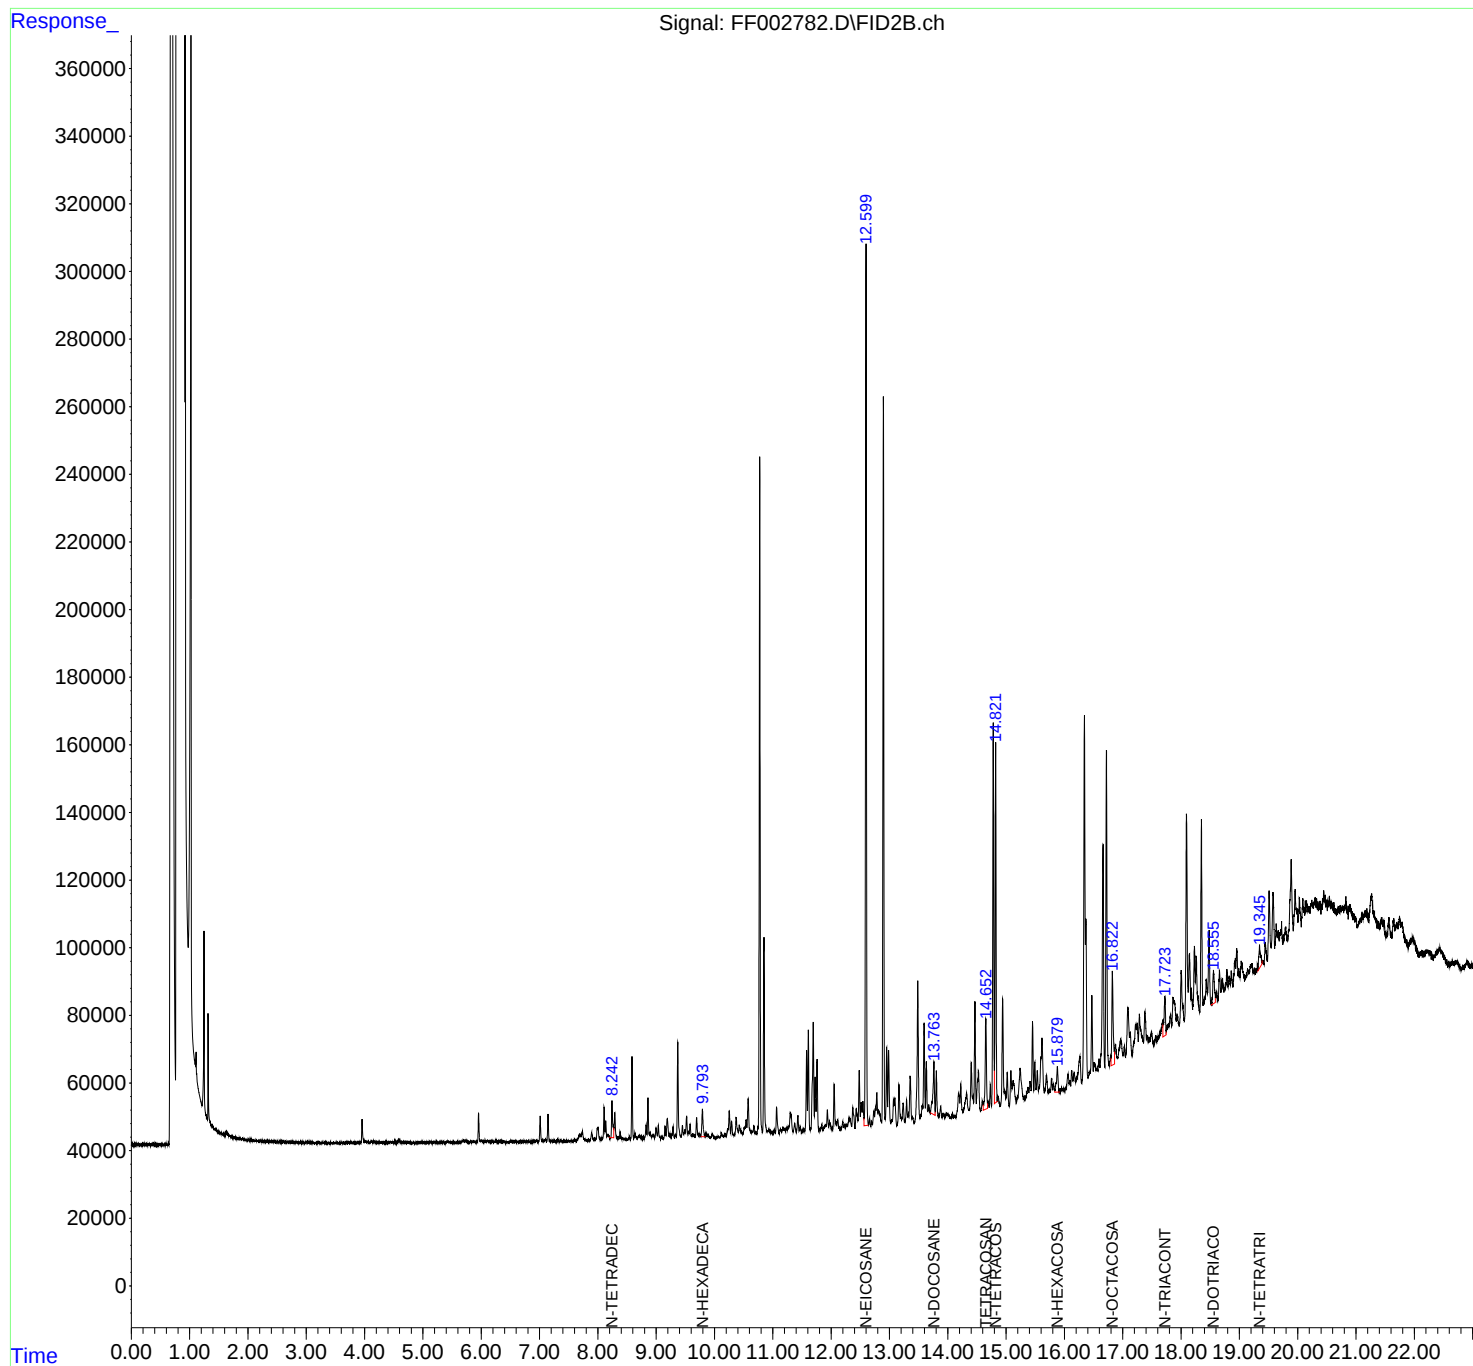

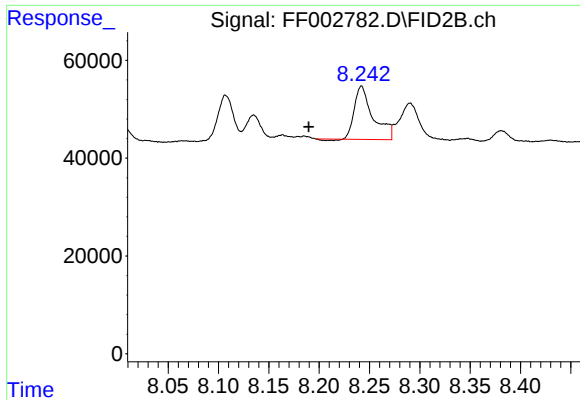


#4 N-TETRADECANE

R.T.: 8.242 min
Delta R.T.: 0.052 min
Response: 140382
Conc: 1.22 ug/ml

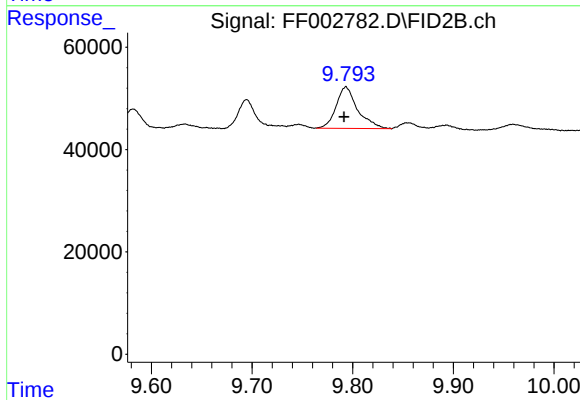


#5 N-HEXADECANE

R.T.: 9.793 min
Delta R.T.: 0.002 min
Response: 120589
Conc: 1.10 ug/ml

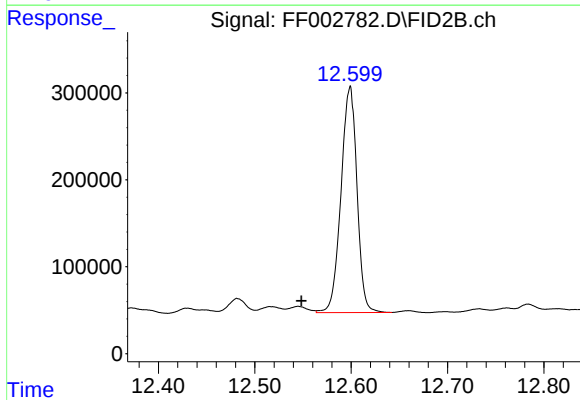


#7 N-EICOSANE

R.T.: 12.599 min
Delta R.T.: 0.051 min
Response: 2983892
Conc: 30.82 ug/ml

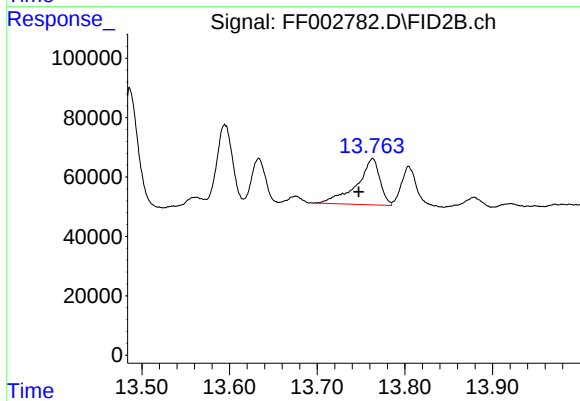


#8 N-DOCOSANE

R.T.: 13.763 min
Delta R.T.: 0.016 min
Response: 284946
Conc: 3.11 ug/ml

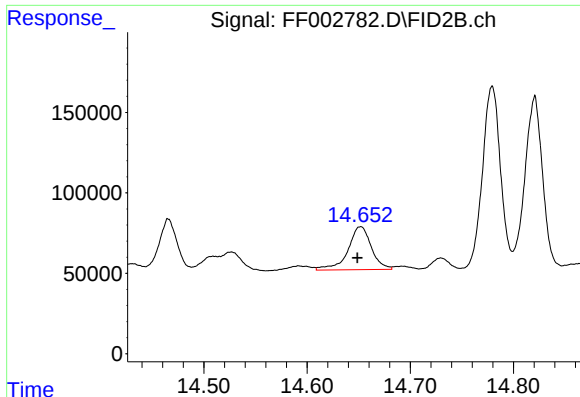


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.652 min
Delta R.T.: 0.003 min
Response: 421409
Conc: 5.39 ug/ml

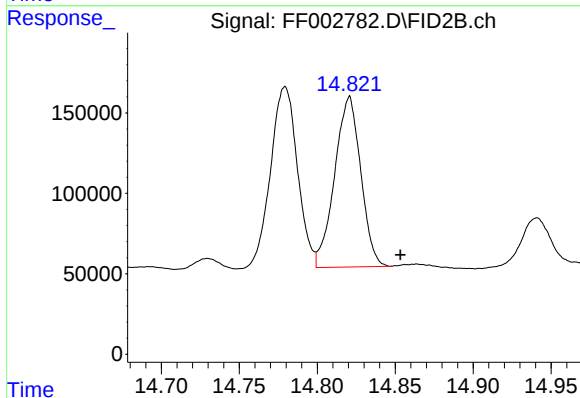


#10 N-TETRACOSANE

R.T.: 14.821 min
Delta R.T.: -0.033 min
Response: 1236157
Conc: 13.88 ug/ml

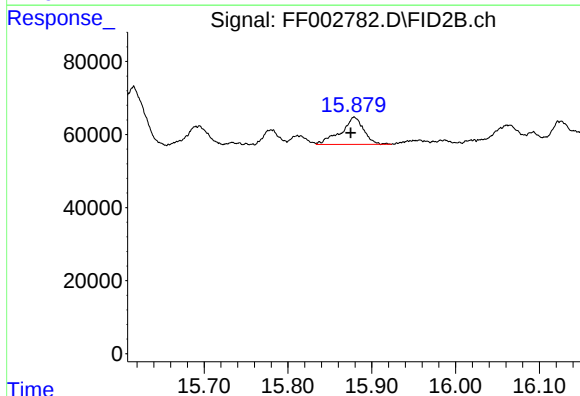


#11 N-HEXACOSANE

R.T.: 15.879 min
Delta R.T.: 0.004 min
Response: 141137
Conc: 1.56 ug/ml

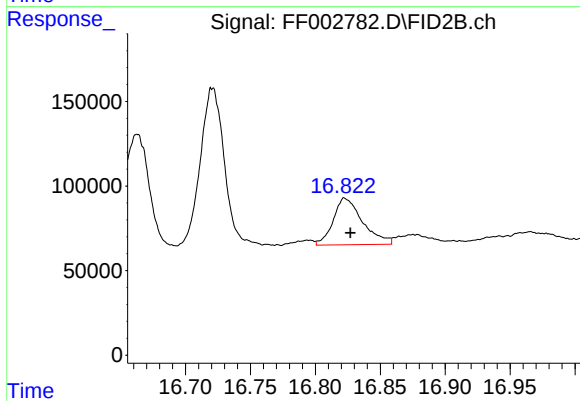


#12 N-OCTACOSANE

R.T.: 16.823 min
Delta R.T.: -0.004 min
Response: 433853
Conc: 4.55 ug/ml

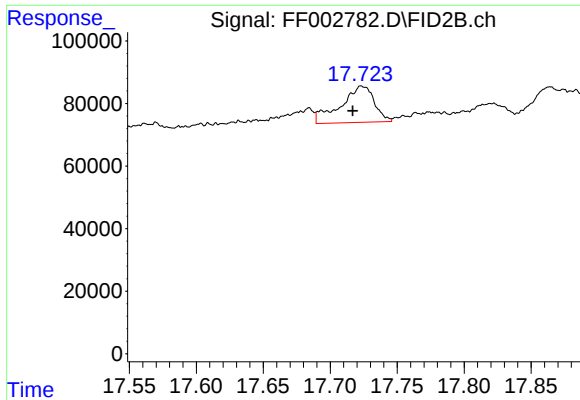


#13 N-TRIACONTANE

R.T.: 17.724 min
Delta R.T.: 0.007 min
Response: 202652
Conc: 2.04 ug/ml

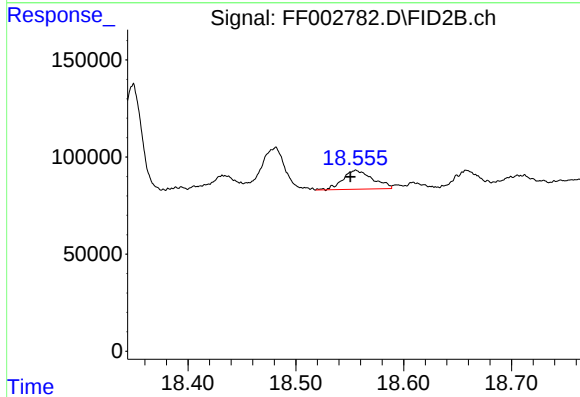

#14 N-DOTRIACONTANE

R.T.: 18.556 min
Delta R.T.: 0.005 min
Response: 185714
Conc: 1.88 ug/ml

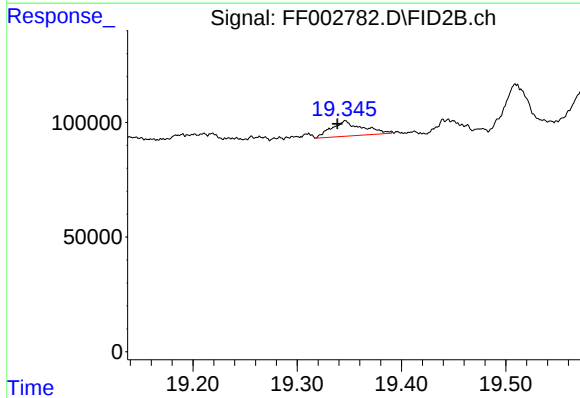

#15 N-TETRATRIACONTANE

R.T.: 19.346 min
Delta R.T.: 0.008 min
Response: 138262
Conc: 1.40 ug/ml