

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112618\
 Data File : FF002780.D
 Signal(s) : FID2B.ch
 Acq On : 26 Nov 2018 14:39
 Operator : AJ\SJ
 Sample : J5770-05MS 5X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 27 01:23:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.651	433555	5.550 ug/mlm
Target Compounds			
2) N-DECANE	4.375	357970	2.866 ug/ml
3) N-DODECANE	6.396	381516	3.148 ug/ml
4) N-TETRADECANE	8.190	403524	3.493 ug/ml
5) N-HEXADECANE	9.792	478297	4.374 ug/mlm
6) N-OCTADECANE	11.236	361789	3.485 ug/mlm
7) N-EICOSANE	12.549	481929	4.977 ug/ml
8) N-DOCOSANE	13.750	706836	7.720 ug/ml
10) N-TETRACOSANE	14.856	443591	4.979 ug/ml
11) N-HEXACOSANE	15.879	537940	5.928 ug/ml
12) N-OCTACOSANE	16.828	790741	8.290 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112618\
Data File : FF002780.D
Signal(s) : FID2B.ch
Acq On : 26 Nov 2018 14:39
Operator : AJ\SJ
Sample : J5770-05MS 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 27 01:23:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

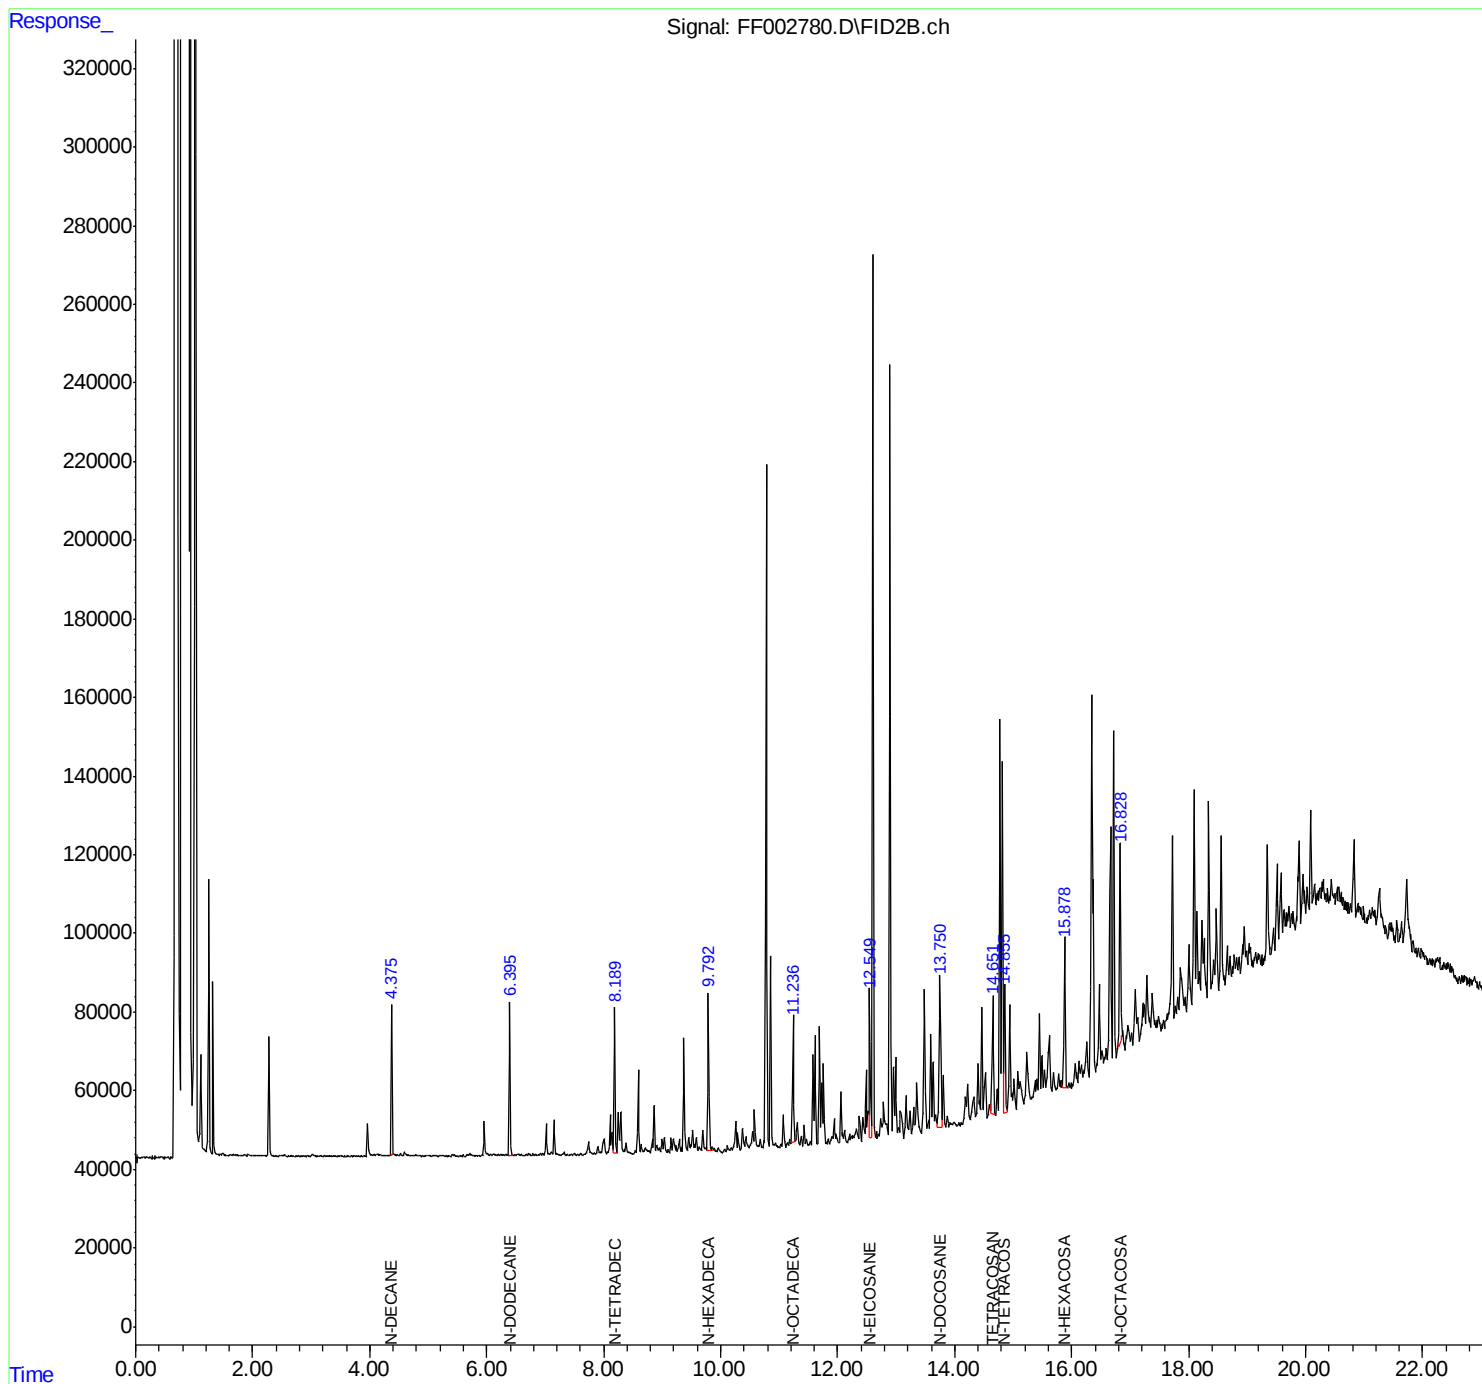

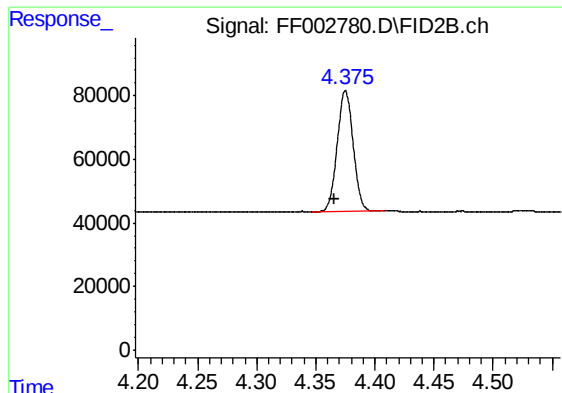


#2 N-DECANE

R.T.: 4.375 min
Delta R.T.: 0.009 min
Response: 357970
Conc: 2.87 ug/ml

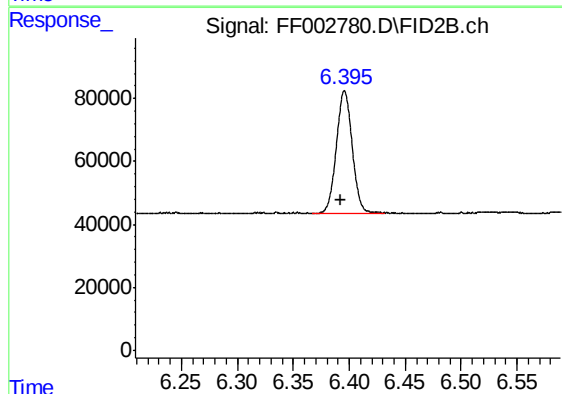


#3 N-DODECANE

R.T.: 6.396 min
Delta R.T.: 0.003 min
Response: 381516
Conc: 3.15 ug/ml

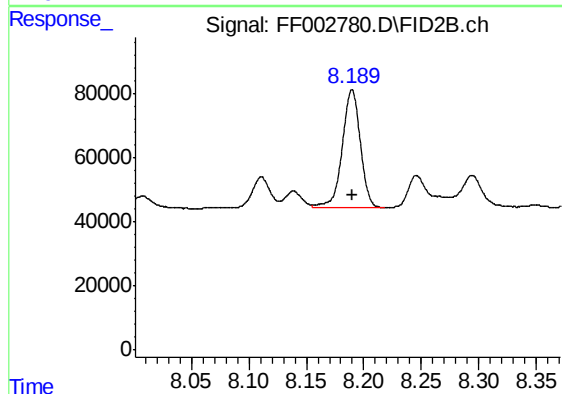


#4 N-TETRADECANE

R.T.: 8.190 min
Delta R.T.: 0.000 min
Response: 403524
Conc: 3.49 ug/ml

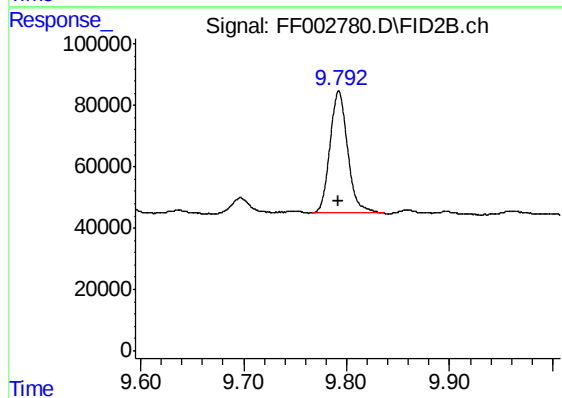


#5 N-HEXADECANE

R.T.: 9.792 min
Delta R.T.: 0.000 min
Response: 478297
Conc: 4.37 ug/ml m

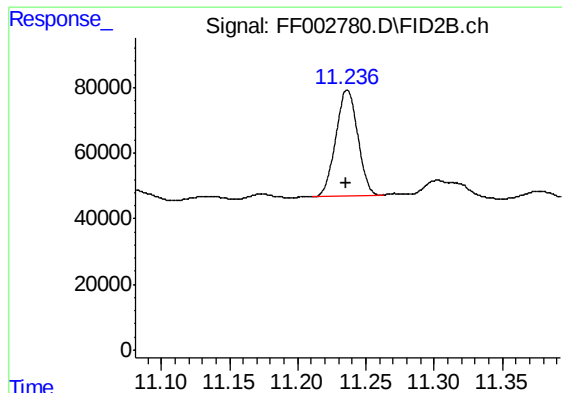


#6 N-OCTADECANE

R.T.: 11.236 min
Delta R.T.: 0.000 min
Response: 361789
Conc: 3.49 ug/ml m

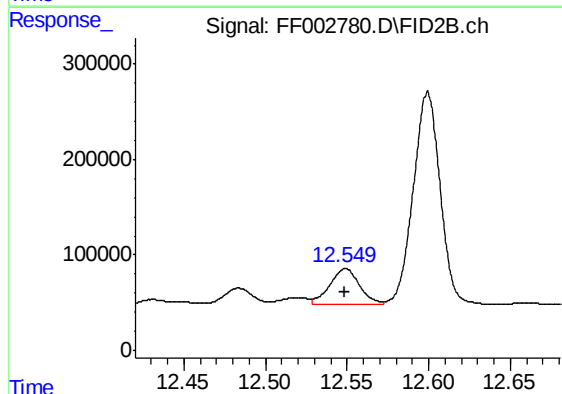


#7 N-EICOSANE

R.T.: 12.549 min
Delta R.T.: 0.000 min
Response: 481929
Conc: 4.98 ug/ml

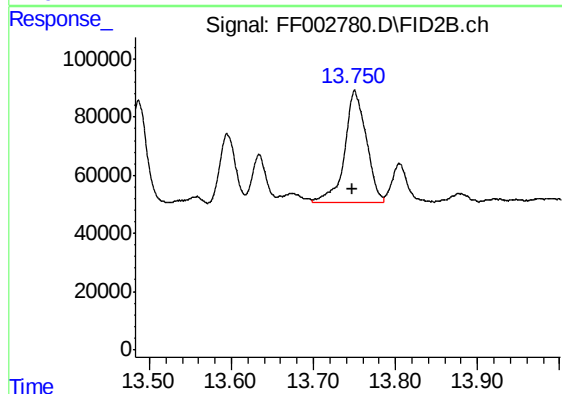


#8 N-DOCOSANE

R.T.: 13.750 min
Delta R.T.: 0.003 min
Response: 706836
Conc: 7.72 ug/ml

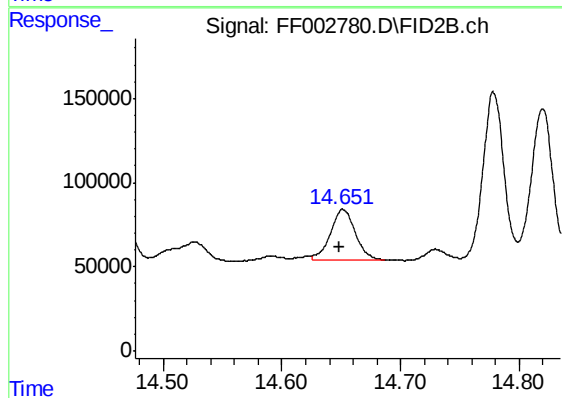


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.651 min
Delta R.T.: 0.002 min
Response: 433555
Conc: 5.55 ug/ml m

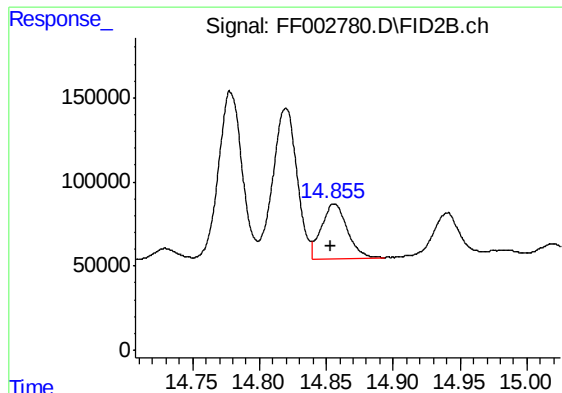


#10 N-TETRACOSANE

R.T.: 14.856 min
Delta R.T.: 0.003 min
Response: 443591
Conc: 4.98 ug/ml

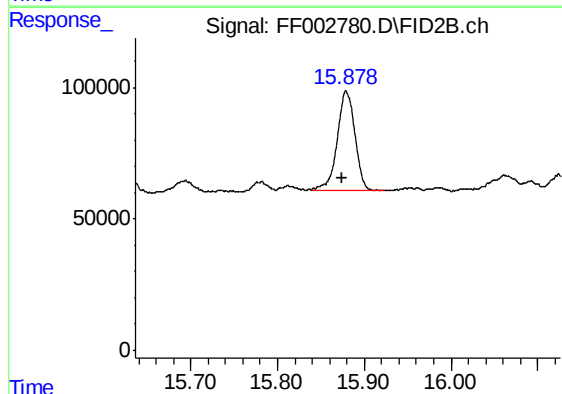

#11 N-HEXACOSANE

R.T.: 15.879 min
Delta R.T.: 0.004 min
Response: 537940
Conc: 5.93 ug/ml

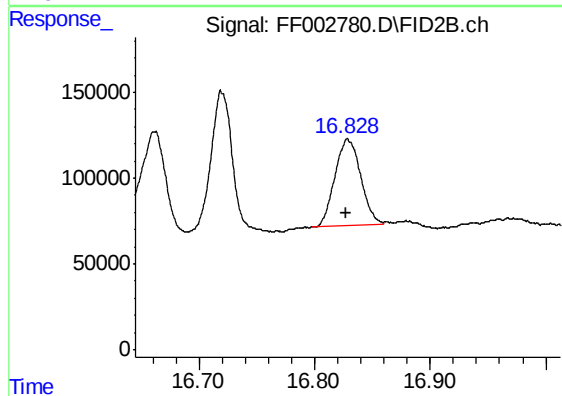

#12 N-OCTACOSANE

R.T.: 16.828 min
Delta R.T.: 0.001 min
Response: 790741
Conc: 8.29 ug/ml m