

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF112718\
Data File : FF002786.D
Signal(s) : FID2B.ch
Acq On : 27 Nov 2018 08:28
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 27 13:43:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.654	1764865	22.593 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.724	150725	1.520 ug/ml
14) N-DOTRIACONTANE	18.559	224430	2.267 ug/ml
15) N-TETRATRIACONTANE	19.344	199507	2.021 ug/ml
16) N-HEXATRIACONTANE	20.088	92539	0.971 ug/ml
18) N-TETRACONTANE	21.742	498886	5.695 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF112718\
Data File : FF002786.D
Signal(s) : FID2B.ch
Acq On : 27 Nov 2018 08:28
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 27 13:43:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

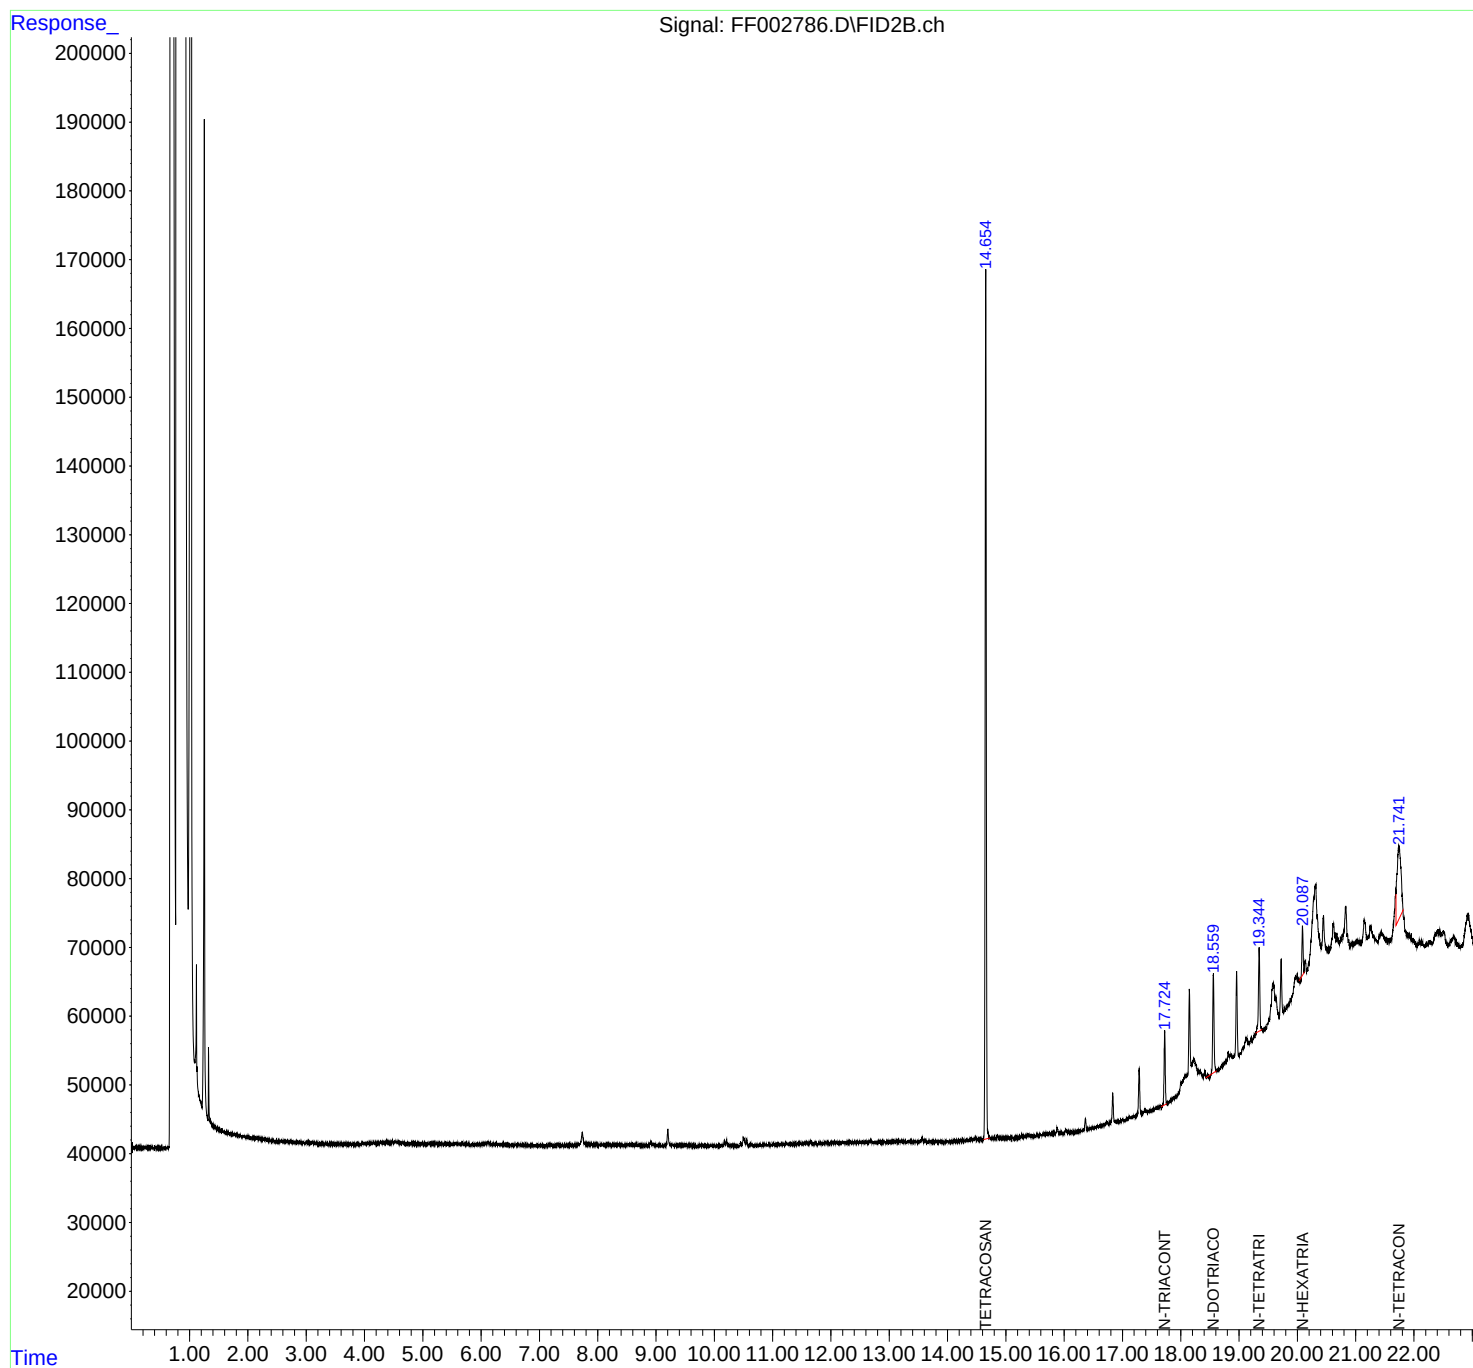


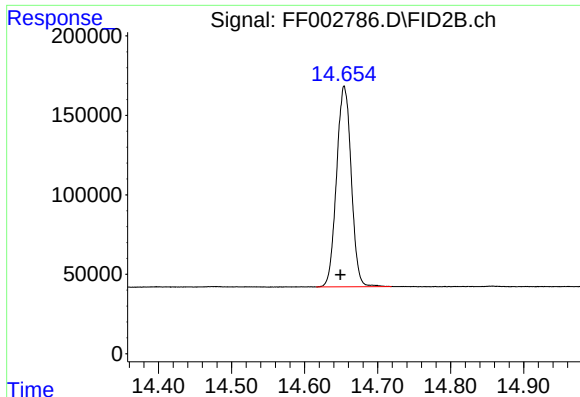

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.654 min
Delta R.T.: 0.005 min
Response: 1764865
Conc: 22.59 ug/ml

Instrument :
FID_F
ClientSampleId :

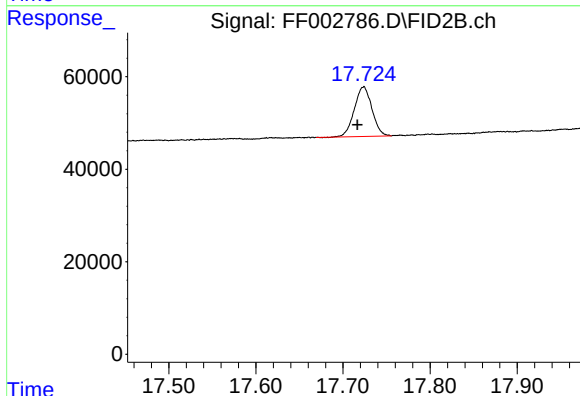


#13 N-TRIACONTANE

R.T.: 17.724 min
Delta R.T.: 0.007 min
Response: 150725
Conc: 1.52 ug/ml

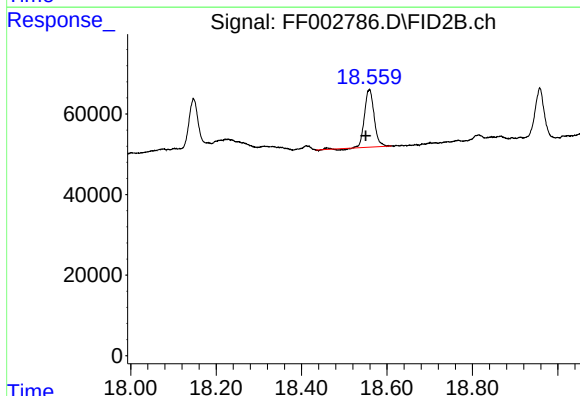


#14 N-DOTRIACONTANE

R.T.: 18.559 min
Delta R.T.: 0.008 min
Response: 224430
Conc: 2.27 ug/ml

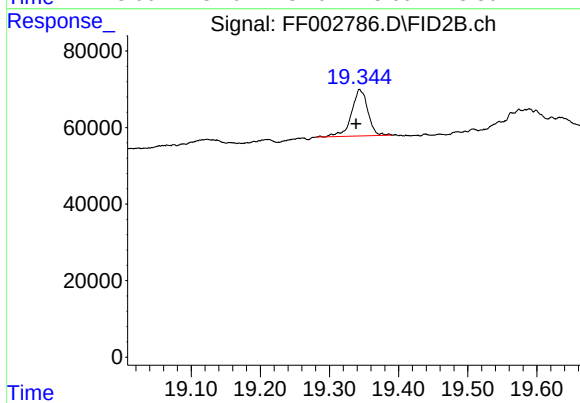

#15 N-TETRATRIACONTANE


R.T.: 19.344 min
Delta R.T.: 0.005 min
Response: 199507
Conc: 2.02 ug/ml

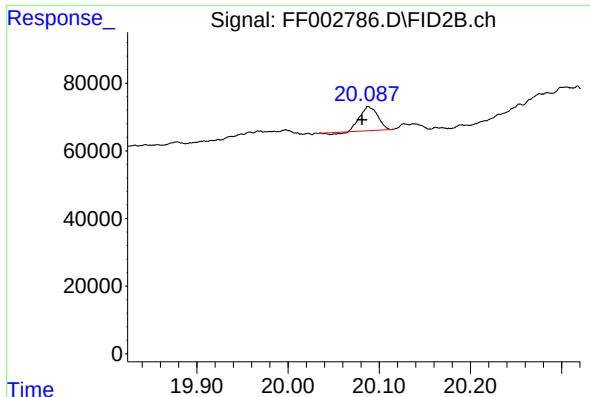

#16 N-HEXATRIACONTANE

R.T.: 20.088 min
Delta R.T.: 0.007 min
Response: 92539
Conc: 0.97 ug/ml

Instrument :
FID_F
ClientSampleId :

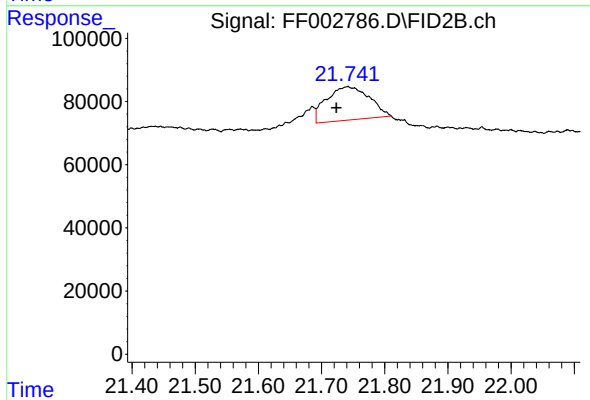

#18 N-TETRACONTANE

R.T.: 21.742 min
Delta R.T.: 0.018 min
Response: 498886
Conc: 5.70 ug/ml