

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112719\
Data File : FF005964.D
Signal(s) : FID2B.ch
Acq On : 27 Nov 2019 08:56
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 27 16:09:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.643	2334948	20.776 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.697	282583	2.328 ug/ml
14)	N-DOTRIACONTANE	18.529	209360	1.829 ug/ml
15)	N-TETRATRIACONTANE	19.311	146394	1.361 ug/ml
16)	N-HEXATRIACONTANE	20.052	76751	0.764 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112719\
Data File : FF005964.D
Signal(s) : FID2B.ch
Acq On : 27 Nov 2019 08:56
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 27 16:09:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF110619.M
Quant Title :
QLast Update : Wed Nov 06 11:58:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

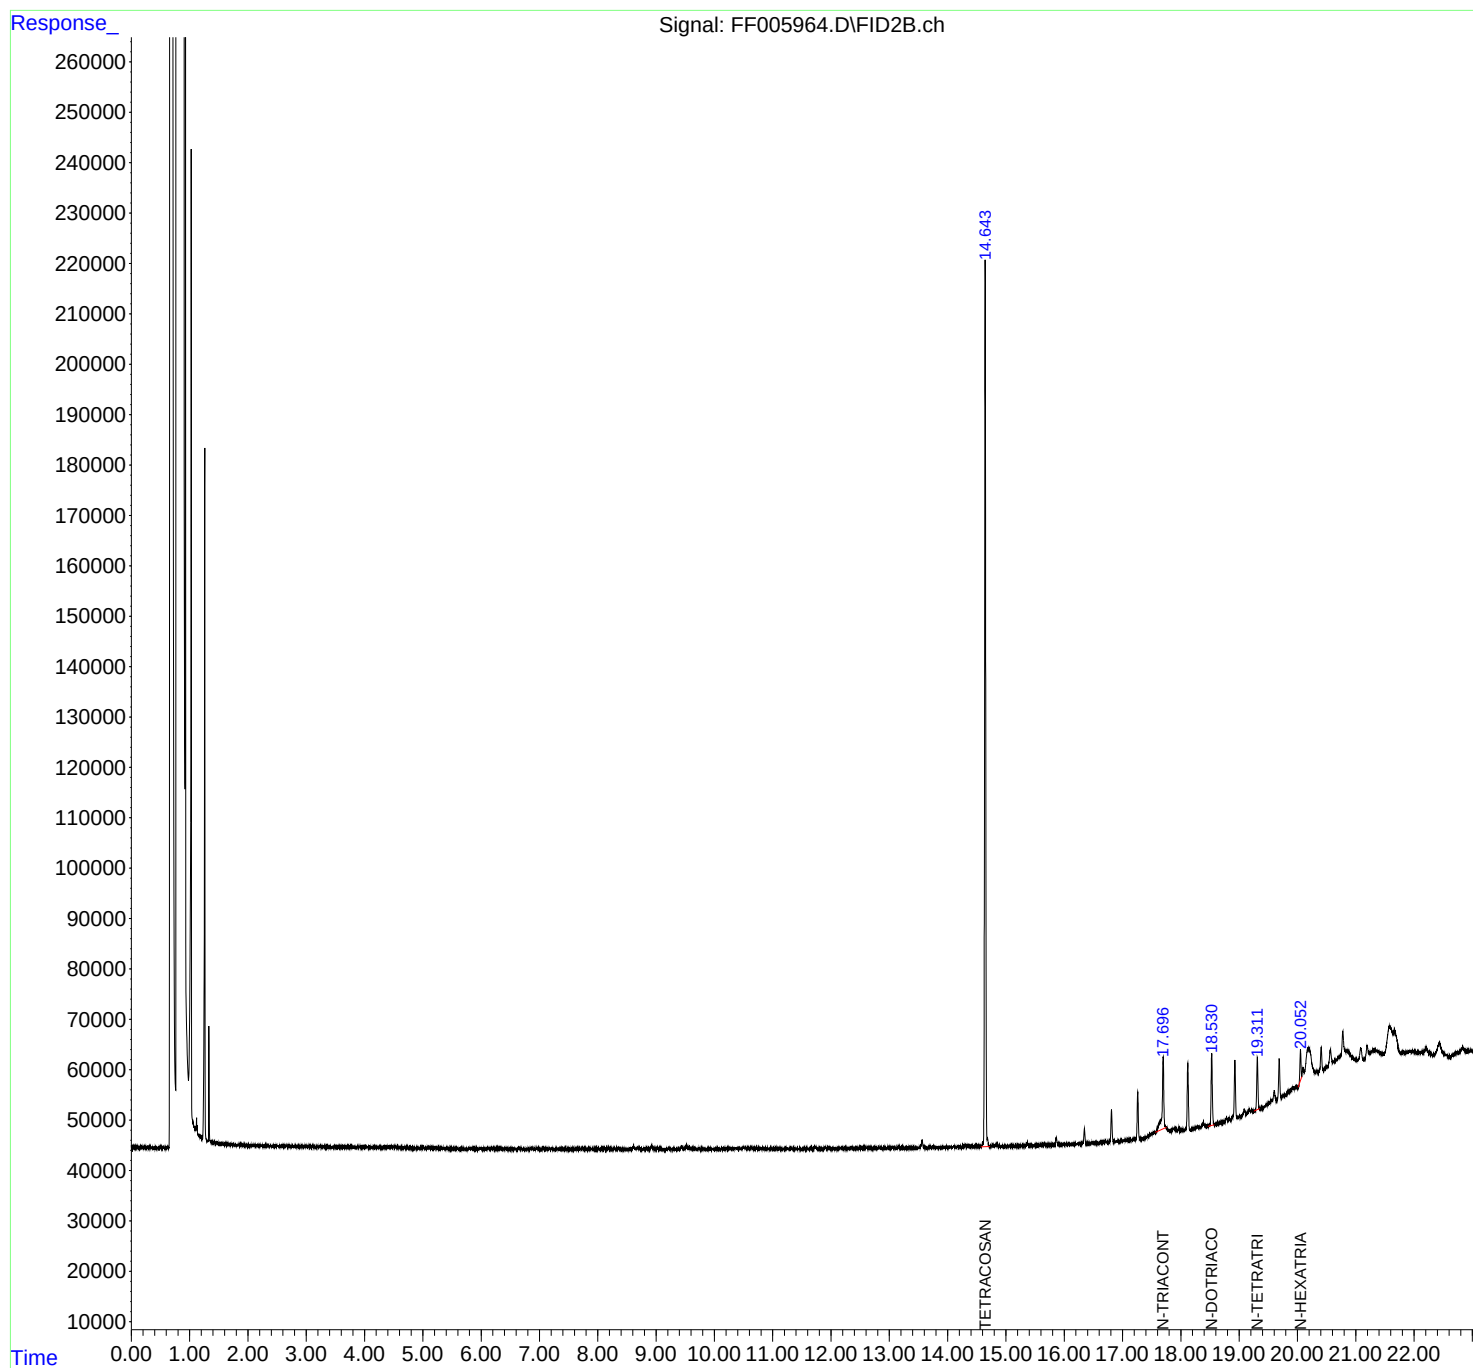

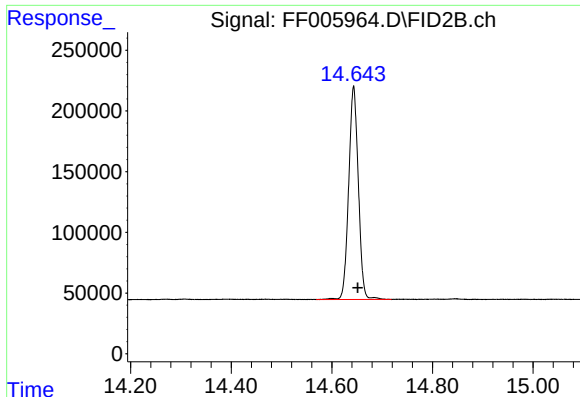


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.643 min
Delta R.T.: -0.008 min
Response: 2334948
Conc: 20.78 ug/ml

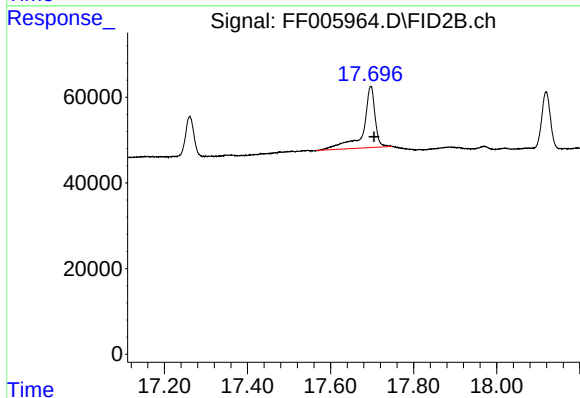


#13 N-TRIACONTANE

R.T.: 17.697 min
Delta R.T.: -0.008 min
Response: 282583
Conc: 2.33 ug/ml

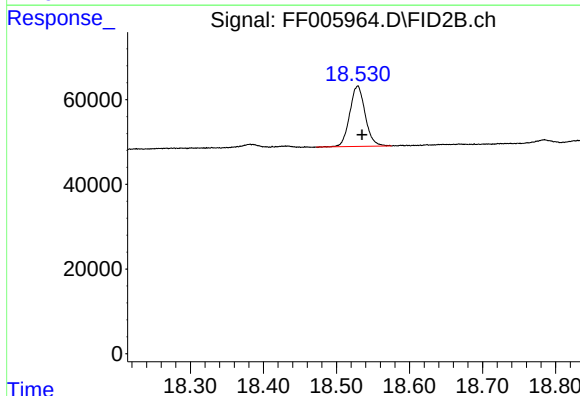


#14 N-DOTRIACONTANE

R.T.: 18.529 min
Delta R.T.: -0.006 min
Response: 209360
Conc: 1.83 ug/ml

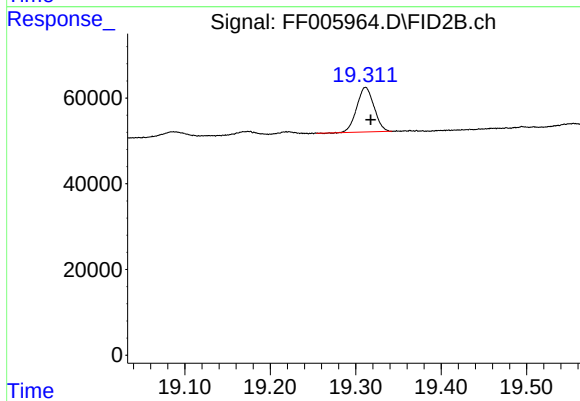

#15 N-TETRATRIACONTANE

R.T.: 19.311 min
Delta R.T.: -0.006 min
Response: 146394
Conc: 1.36 ug/ml

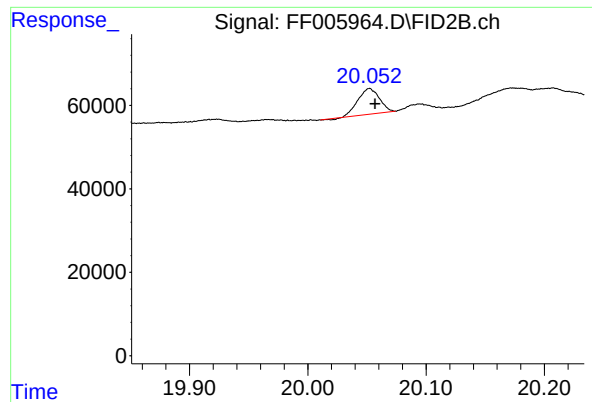

#16 N-HEXATRIACONTANE

R.T.: 20.052 min
Delta R.T.: -0.005 min
Response: 76751
Conc: 0.76 ug/ml