

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112724\
Data File : FF015120.D
Signal(s) : FID2B.ch
Acq On : 27 Nov 2024 06:36
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 00:03:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
Quant Title :
QLast Update : Thu Nov 21 01:46:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

8)	N-DOCOSANE	14.083	212515	1.712 ug/ml
10)	N-TETRACOSANE	15.206	185468	1.524 ug/ml
11)	N-HEXACOSANE	16.230	142127	1.203 ug/ml
12)	N-OCTACOSANE	17.182	98066	0.841 ug/ml
13)	N-TRIACONTANE	18.131f	178943	1.543 ug/ml
14)	N-DOTRIACONTANE	18.924	829028	7.368 ug/ml
15)	N-TETRATRIACONTANE	19.691	309633	3.182 ug/ml
16)	N-HEXATRIACONTANE	20.432	194909	2.494 ug/ml
17)	N-OCTATRIACONTANE	21.167	173246	2.525 ug/ml
18)	N-TETRACONTANE	22.132f	379445	5.804 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112724\
Data File : FF015120.D
Signal(s) : FID2B.ch
Acq On : 27 Nov 2024 06:36
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 00:03:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
Quant Title :
QLast Update : Thu Nov 21 01:46:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

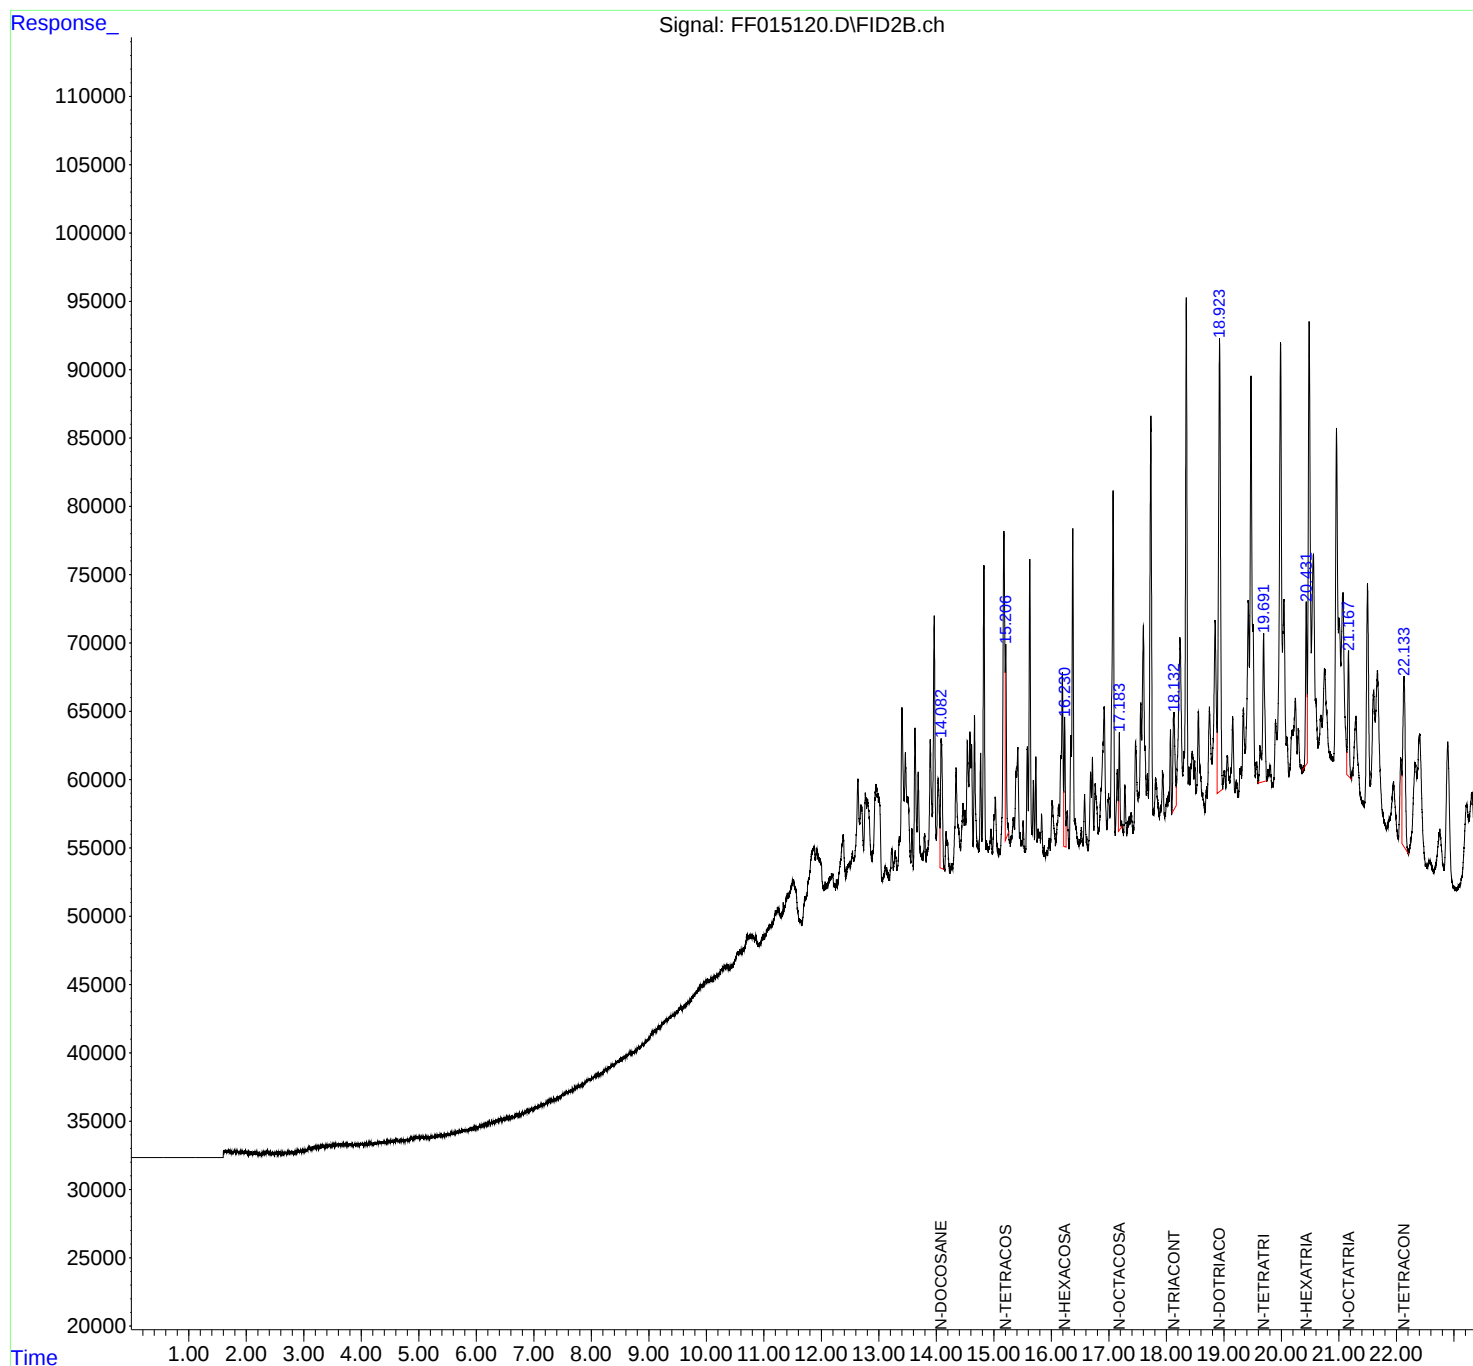


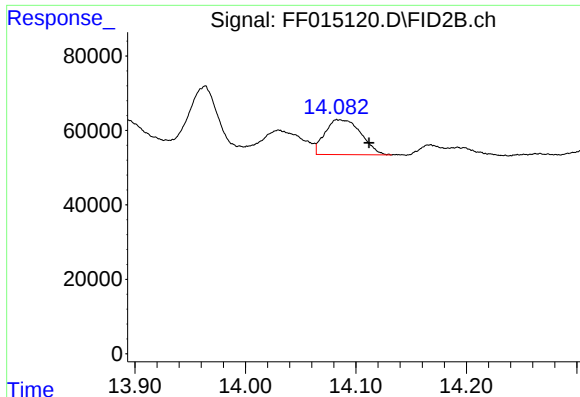

#8 N-DOCOSANE


R.T.: 14.083 min
Delta R.T.: -0.029 min
Response: 212515
Conc: 1.71 ug/ml

Instrument :
FID_F
ClientSampleId :

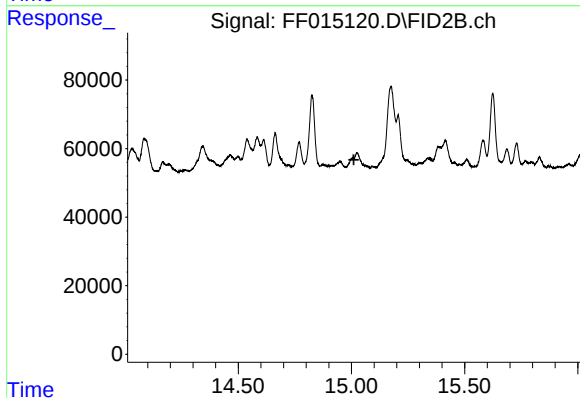


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.011 min
Response: 0
Conc: N.D.

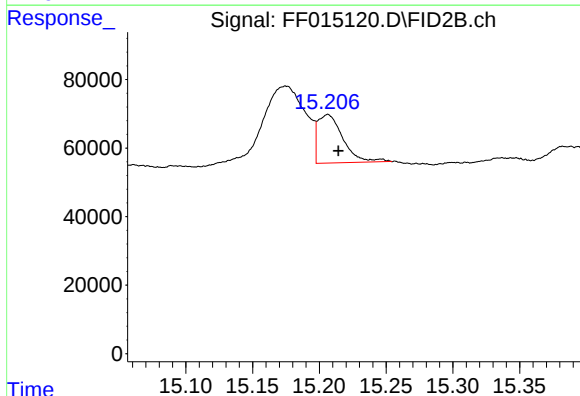


#10 N-TETRACOSANE

R.T.: 15.206 min
Delta R.T.: -0.008 min
Response: 185468
Conc: 1.52 ug/ml

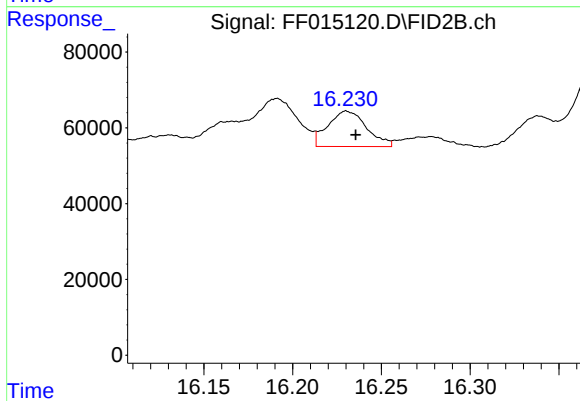

#11 N-HEXACOSANE


R.T.: 16.230 min
Delta R.T.: -0.005 min
Response: 142127
Conc: 1.20 ug/ml

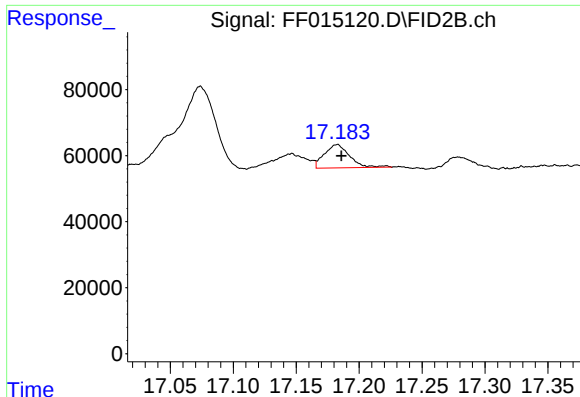

#12 N-OCTACOSANE


R.T.: 17.182 min
Delta R.T.: -0.003 min
Response: 98066
Conc: 0.84 ug/ml

Instrument :
FID_F
ClientSampleId :

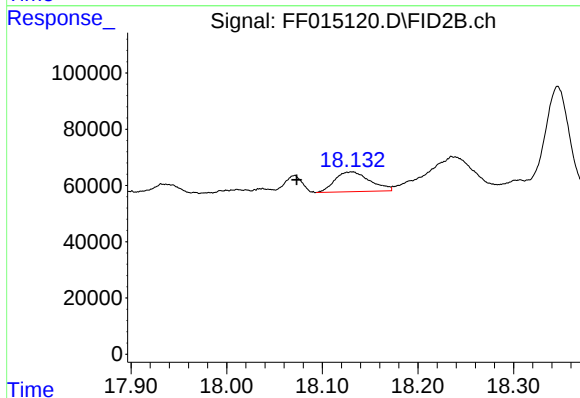


#13 N-TRIACONTANE

R.T.: 18.131 min
Delta R.T.: 0.058 min
Response: 178943
Conc: 1.54 ug/ml

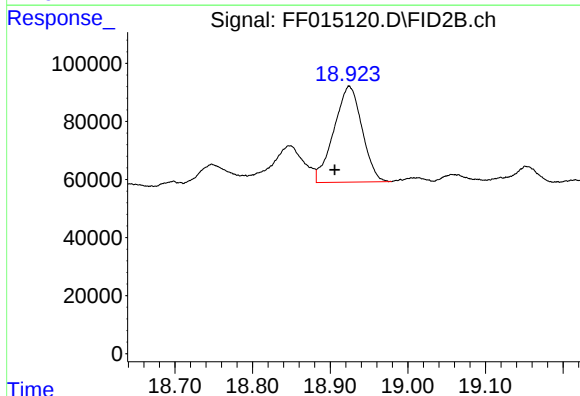


#14 N-DOTRIACONTANE

R.T.: 18.924 min
Delta R.T.: 0.019 min
Response: 829028
Conc: 7.37 ug/ml

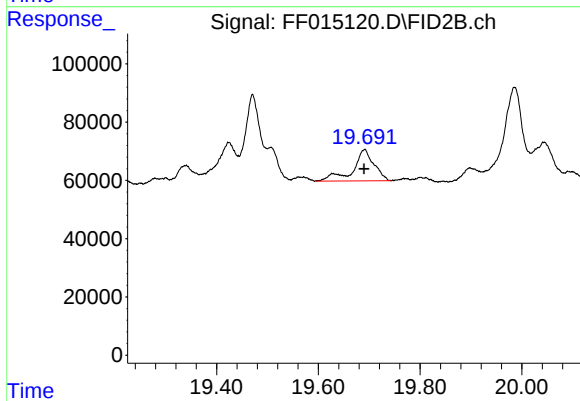

#15 N-TETRATRIACONTANE


R.T.: 19.691 min
Delta R.T.: 0.001 min
Response: 309633
Conc: 3.18 ug/ml

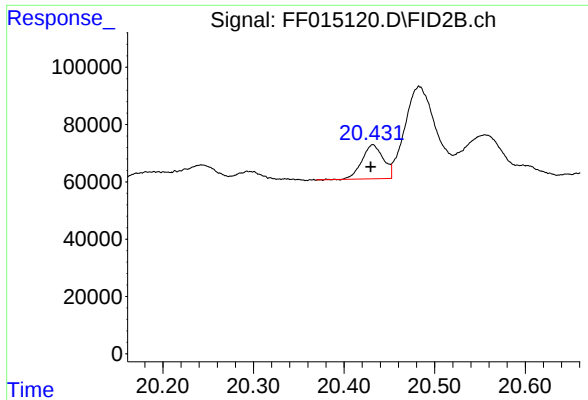

#16 N-HEXATRIACONTANE


R.T.: 20.432 min
Delta R.T.: 0.002 min
Response: 194909
Conc: 2.49 ug/ml

Instrument :
FID_F
ClientSampleId :

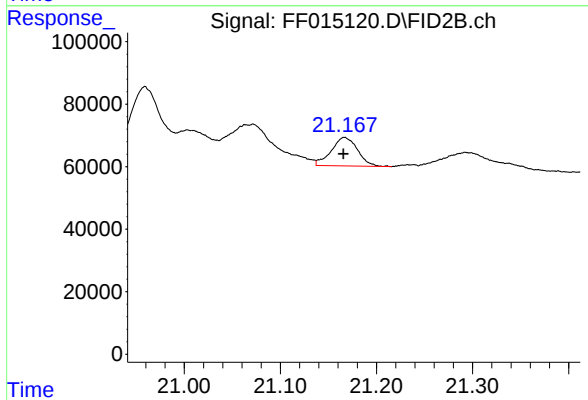

#17 N-OCTATRIACONTANE

R.T.: 21.167 min
Delta R.T.: 0.001 min
Response: 173246
Conc: 2.52 ug/ml

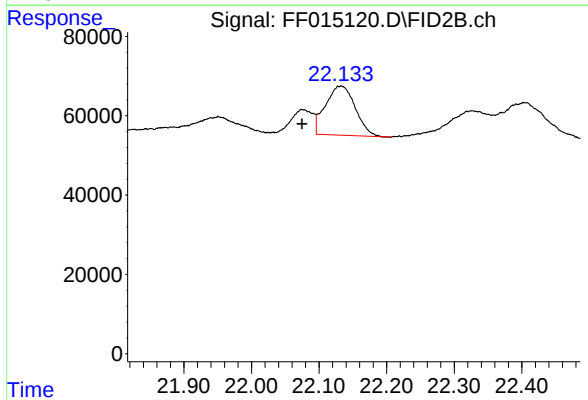

#18 N-TETRACONTANE

R.T.: 22.132 min
Delta R.T.: 0.057 min
Response: 379445
Conc: 5.80 ug/ml