

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112724\
 Data File : FF015130.D
 Signal(s) : FID2B.ch
 Acq On : 27 Nov 2024 12:13
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 00:10:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
 Quant Title :
 QLast Update : Thu Nov 21 01:46:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.016	1978307	17.899 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.915	192711	1.713 ug/ml
15) N-TETRATRIACONTANE	19.678	8279	0.085 ug/ml
16) N-HEXATRIACONTANE	20.428	83989	1.075 ug/ml
17) N-OCTATRIACONTANE	21.119	34654	0.505 ug/ml
18) N-TETRACONTANE	22.092	482824	7.385 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112724\
 Data File : FF015130.D
 Signal(s) : FID2B.ch
 Acq On : 27 Nov 2024 12:13
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 00:10:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF112124.M
 Quant Title :
 QLast Update : Thu Nov 21 01:46:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

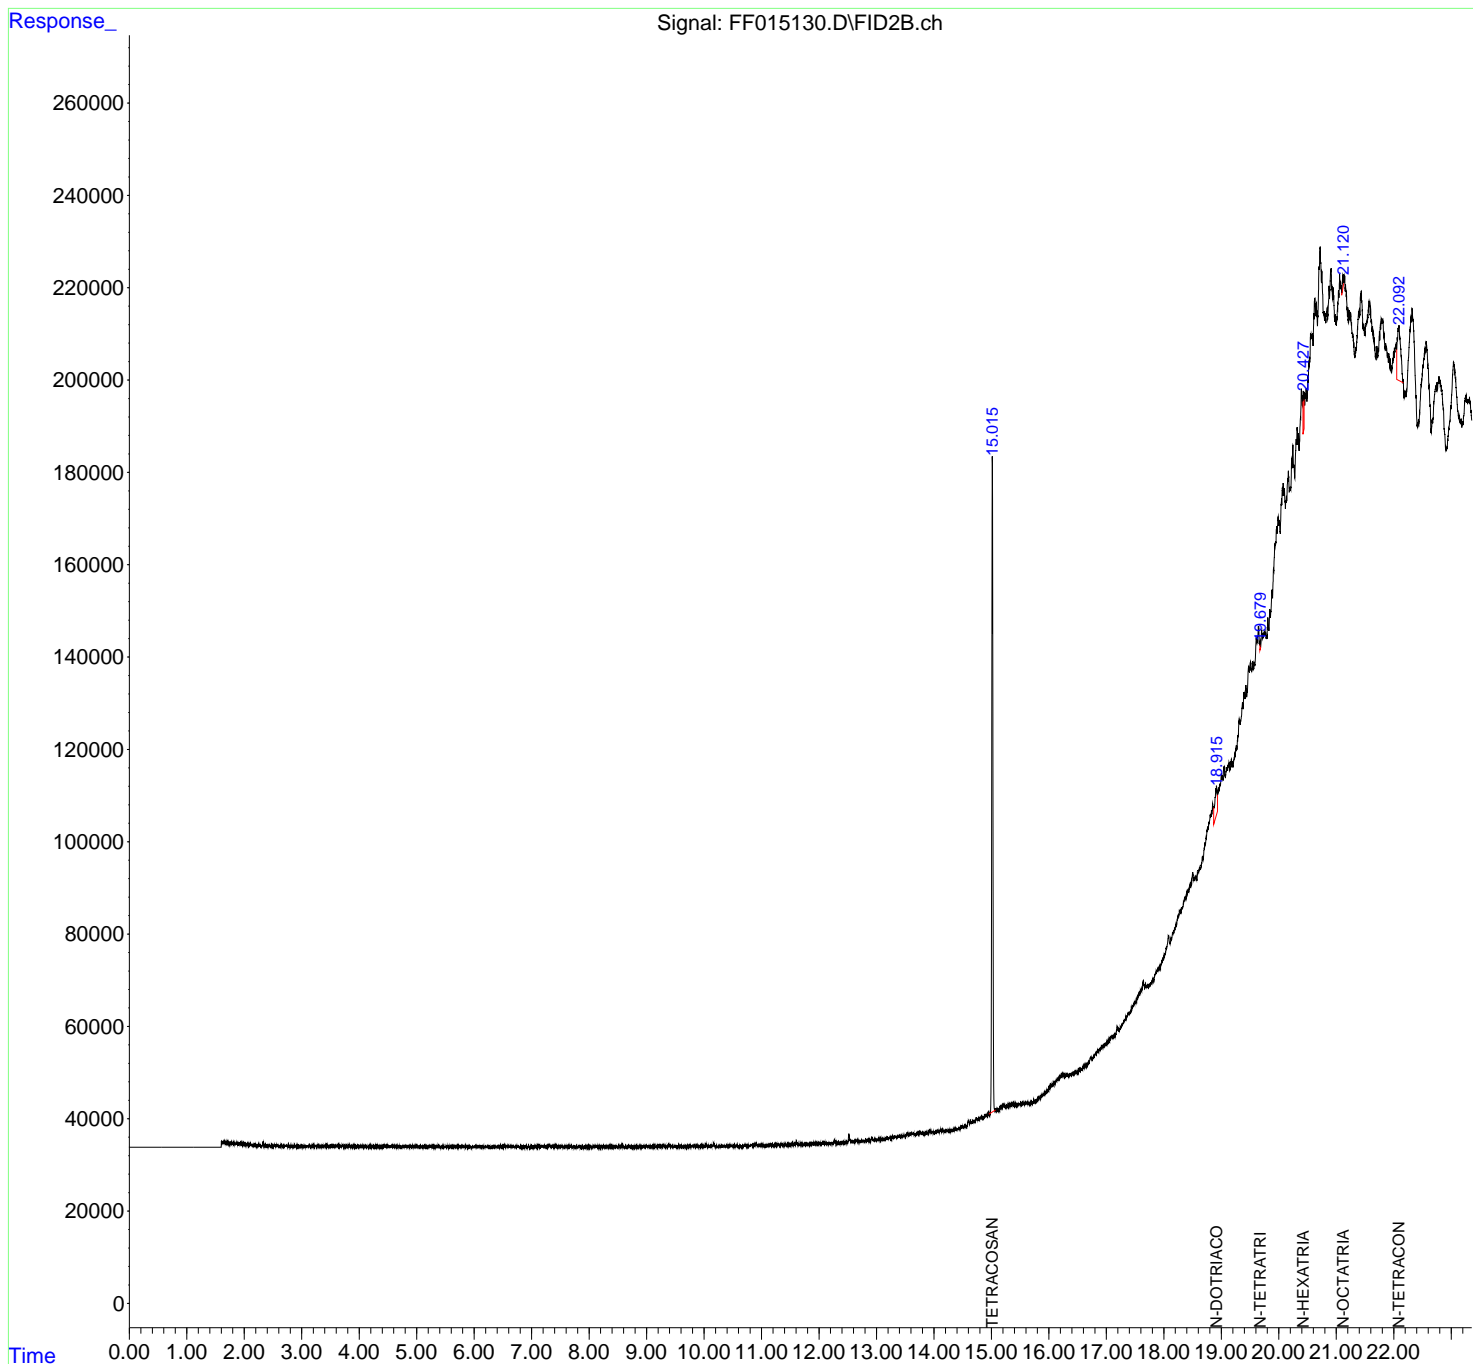


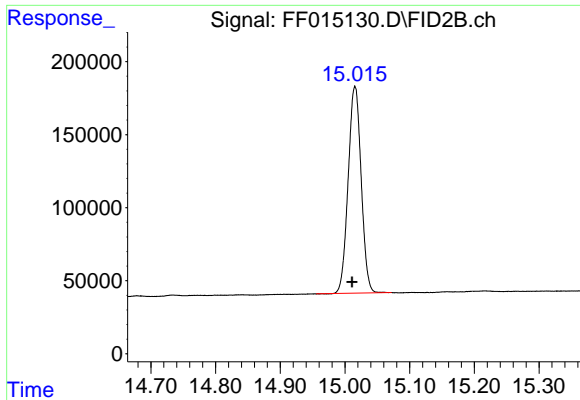

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.016 min
 Delta R.T.: 0.005 min
 Response: 1978307
 Conc: 17.90 ug/ml

Instrument :
 FID_F
 ClientSampleId :

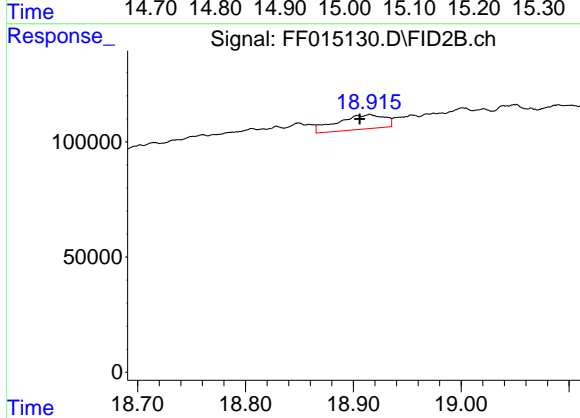


#14 N-DOTRIACONTANE

R.T.: 18.915 min
 Delta R.T.: 0.010 min
 Response: 192711
 Conc: 1.71 ug/ml

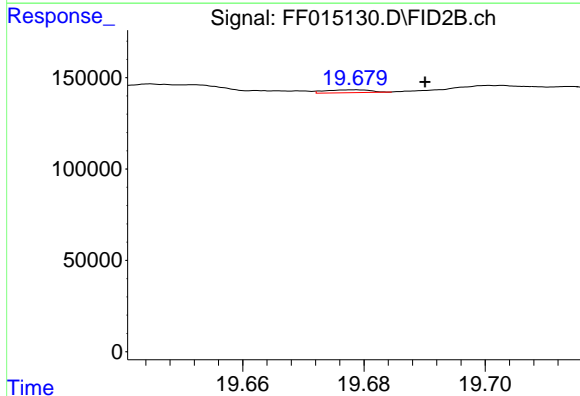


#15 N-TETRATRIACONTANE

R.T.: 19.678 min
 Delta R.T.: -0.012 min
 Response: 8279
 Conc: 0.09 ug/ml

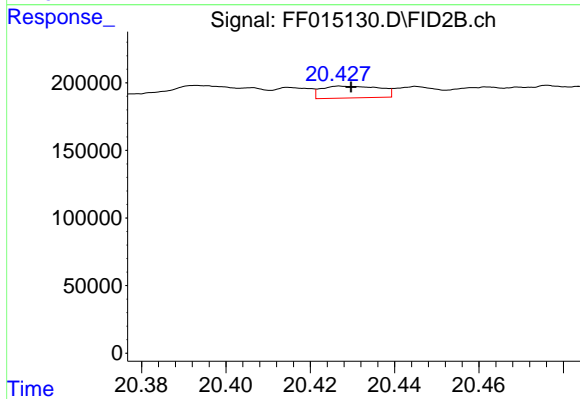

#16 N-HEXATRIACONTANE


R.T.: 20.428 min
 Delta R.T.: -0.002 min
 Response: 83989
 Conc: 1.07 ug/ml

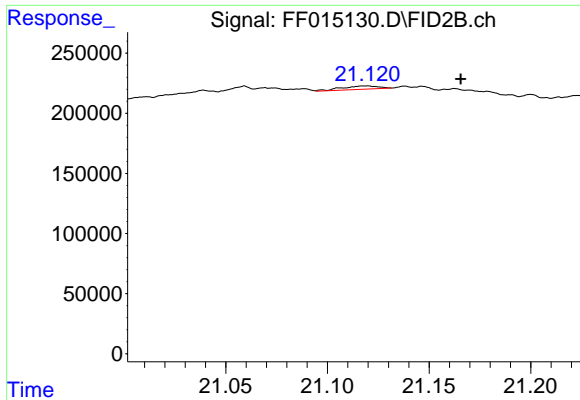

#17 N-OCTATRIACONTANE

R.T.: 21.119 min
Delta R.T.: -0.047 min
Response: 34654
Conc: 0.51 ug/ml

Instrument :
FID_F
ClientSampleId :

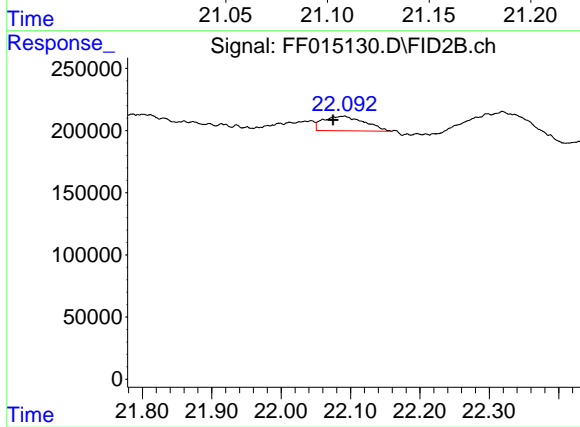

#18 N-TETRACONTANE

R.T.: 22.092 min
Delta R.T.: 0.017 min
Response: 482824
Conc: 7.38 ug/ml