

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002804.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 13:53
 Operator : AJ\SJ
 Sample : J6028-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 00:55:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.654	1585429	20.296 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243f	267040	2.312 ug/ml
7) N-EICOSANE	12.545	111963	1.156 ug/ml
8) N-DOCOSANE	13.761	443672	4.846 ug/ml
10) N-TETRACOSANE	14.862	140060	1.572 ug/ml
11) N-HEXACOSANE	15.888	582037	6.413 ug/ml
12) N-OCTACOSANE	16.832	1409530	14.778 ug/ml
13) N-TRIACONTANE	17.713	1280580	12.917 ug/ml
14) N-DOTRIACONTANE	18.543	550601	5.562 ug/ml
15) N-TETRATRIACONTANE	19.343	210884	2.137 ug/ml
16) N-HEXATRIACONTANE	20.100	131094	1.376 ug/ml
17) N-OCTATRIACONTANE	20.799	601757	6.847 ug/ml
18) N-TETRACONTANE	21.746	197909	2.259 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002804.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 13:53
Operator : AJ\SJ
Sample : J6028-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 29 00:55:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

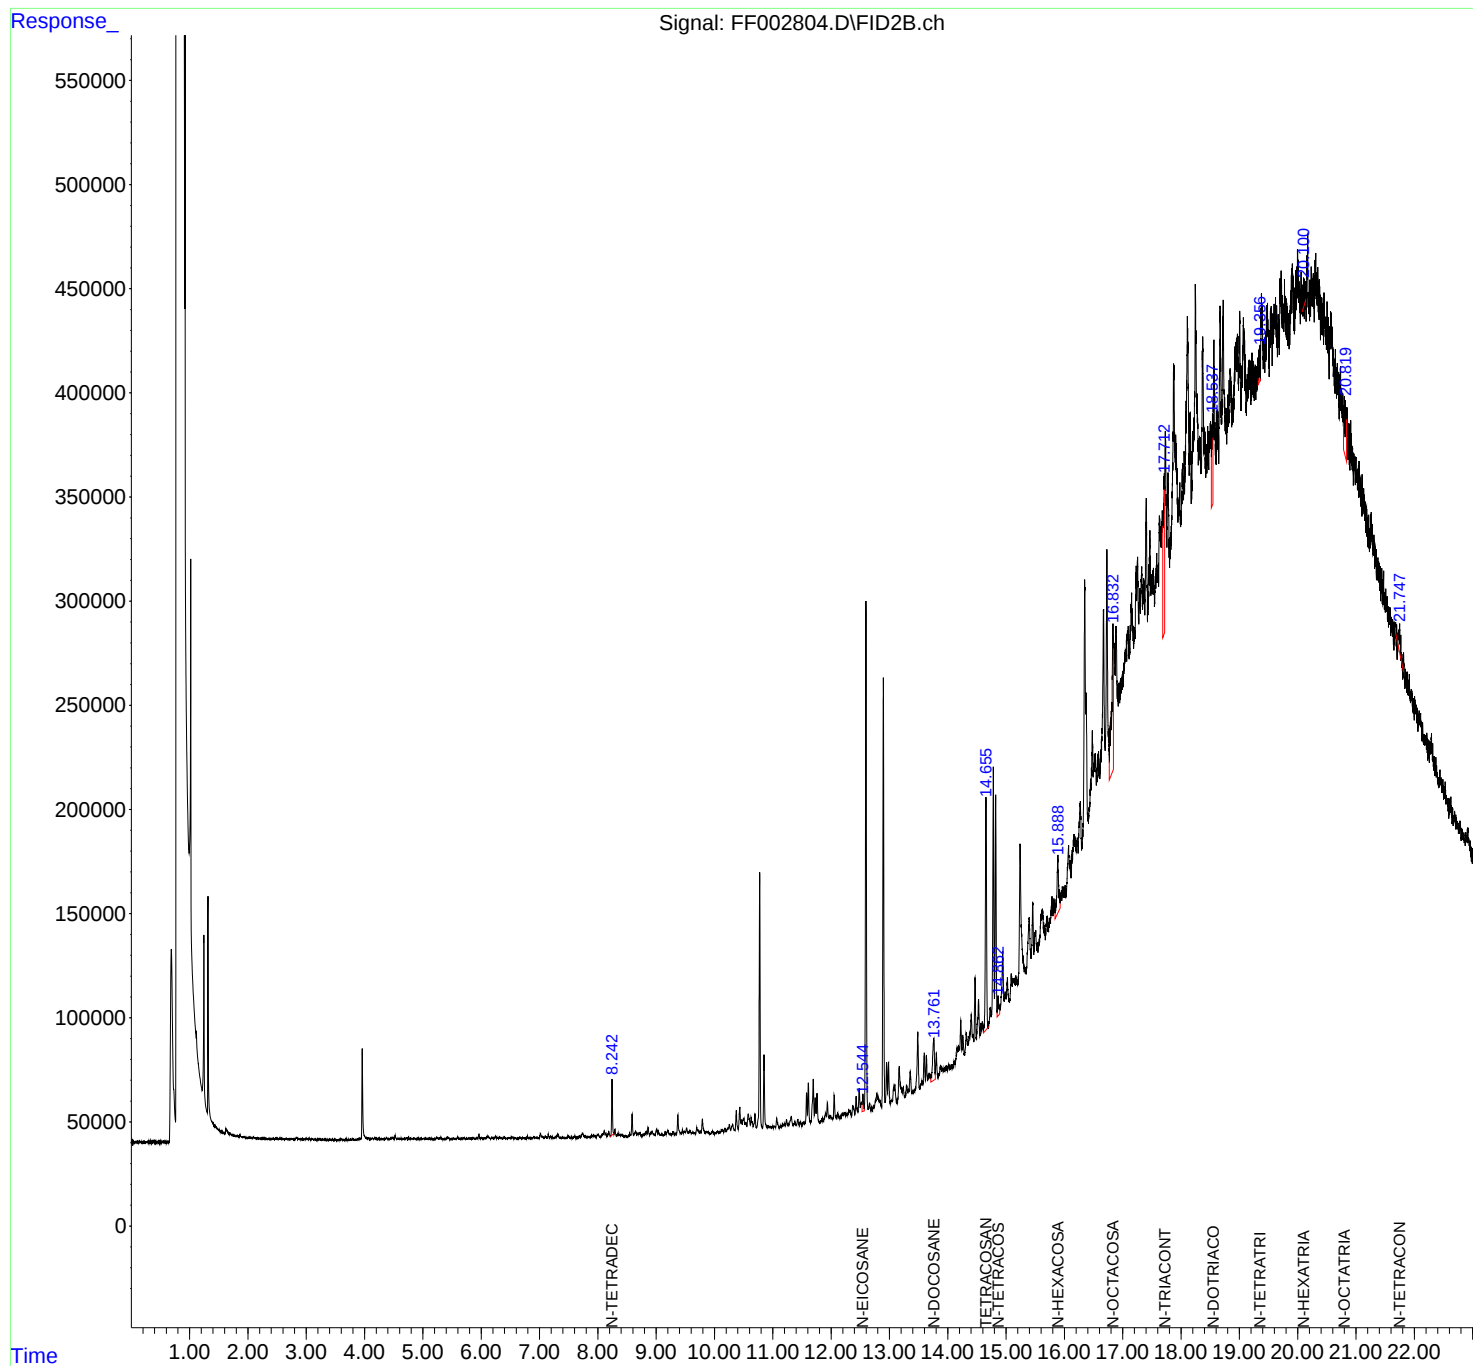


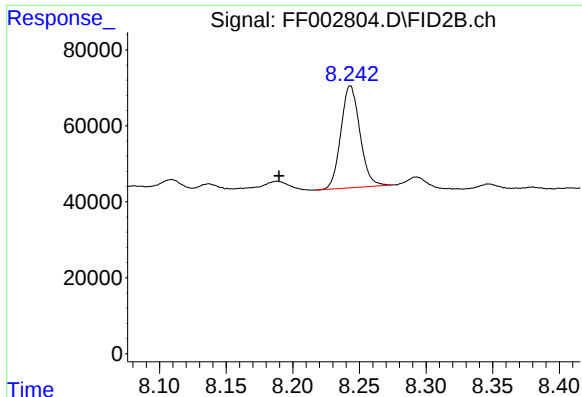

#4 N-TETRADECANE


R.T.: 8.243 min
Delta R.T.: 0.054 min
Response: 267040
Conc: 2.31 ug/ml

Instrument :
FID_F
ClientSampleId :

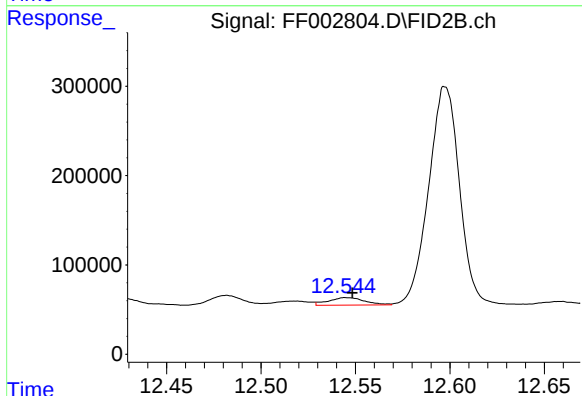


#7 N-EICOSANE

R.T.: 12.545 min
Delta R.T.: -0.003 min
Response: 111963
Conc: 1.16 ug/ml

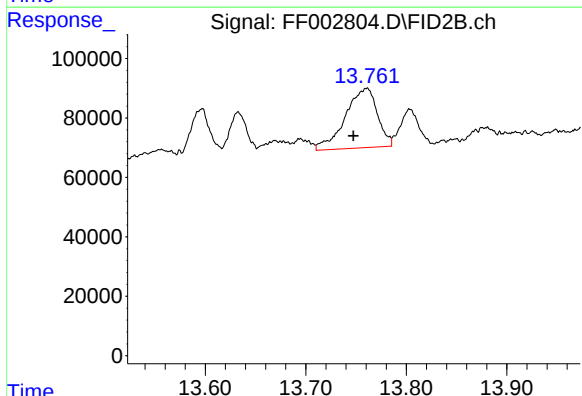


#8 N-DOCOSANE

R.T.: 13.761 min
Delta R.T.: 0.013 min
Response: 443672
Conc: 4.85 ug/ml

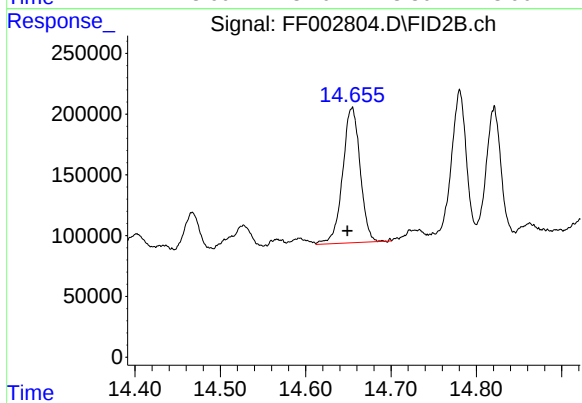

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.654 min
Delta R.T.: 0.005 min
Response: 1585429
Conc: 20.30 ug/ml

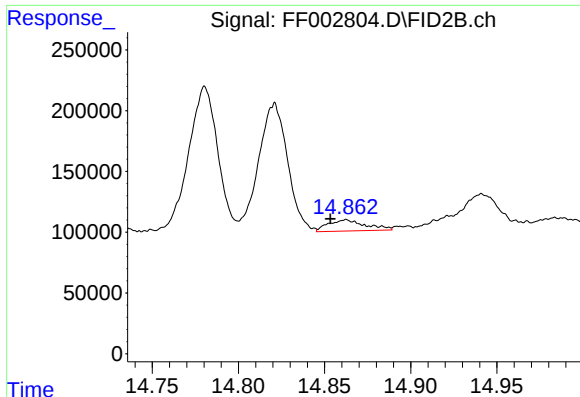

#10 N-TETRACOSANE


R.T.: 14.862 min
Delta R.T.: 0.009 min
Response: 140060
Conc: 1.57 ug/ml

Instrument :
FID_F
ClientSampleId :

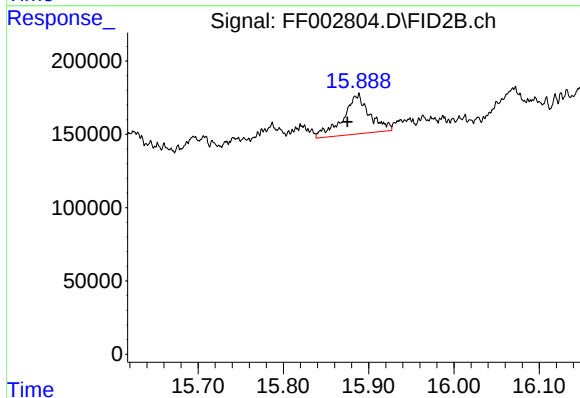


#11 N-HEXACOSANE

R.T.: 15.888 min
Delta R.T.: 0.013 min
Response: 582037
Conc: 6.41 ug/ml

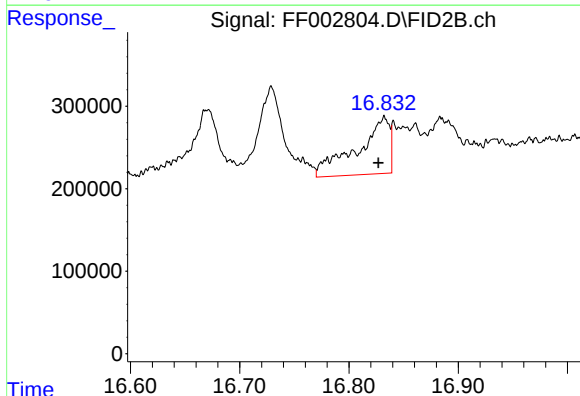


#12 N-OCTACOSANE

R.T.: 16.832 min
Delta R.T.: 0.005 min
Response: 1409530
Conc: 14.78 ug/ml

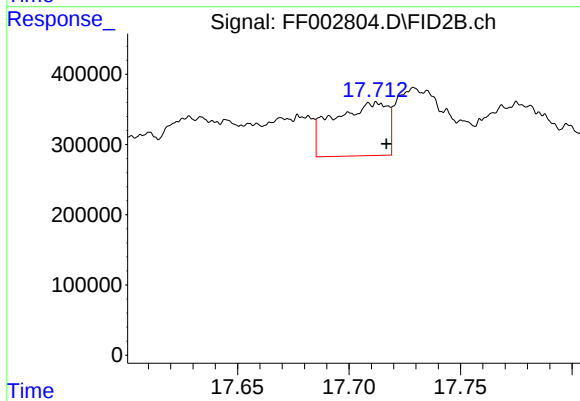

#13 N-TRIACONTANE


R.T.: 17.713 min
Delta R.T.: -0.004 min
Response: 1280580
Conc: 12.92 ug/ml

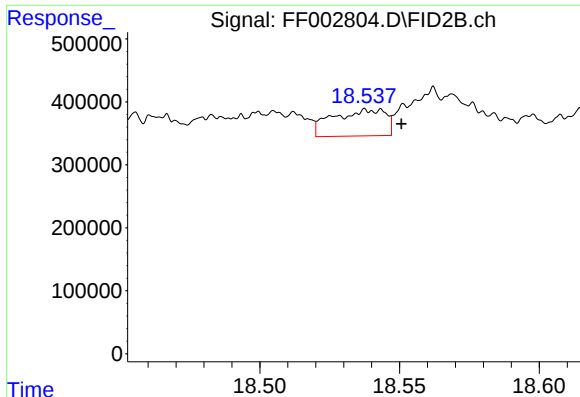

#14 N-DOTRIACONTANE


R.T.: 18.543 min
Delta R.T.: -0.008 min
Response: 550601
Conc: 5.56 ug/ml

Instrument :
FID_F
ClientSampleId :

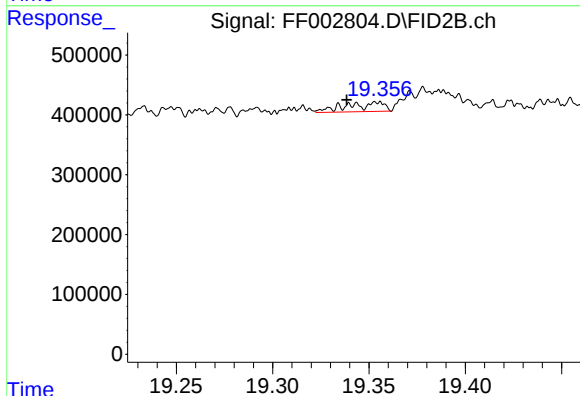


#15 N-TETRATRIACONTANE

R.T.: 19.343 min
Delta R.T.: 0.005 min
Response: 210884
Conc: 2.14 ug/ml

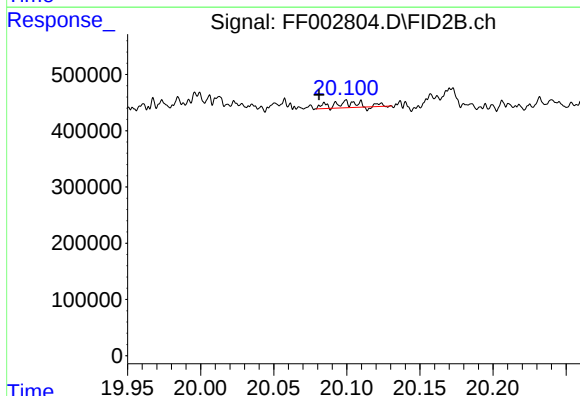


#16 N-HEXATRIACONTANE

R.T.: 20.100 min
Delta R.T.: 0.019 min
Response: 131094
Conc: 1.38 ug/ml

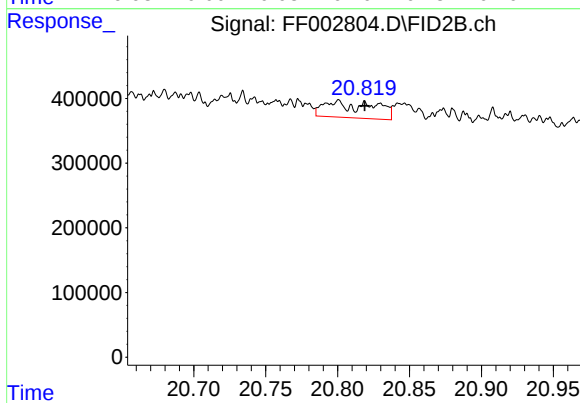

#17 N-OCTATRIACONTANE

R.T.: 20.799 min
Delta R.T.: -0.019 min
Response: 601757
Conc: 6.85 ug/ml

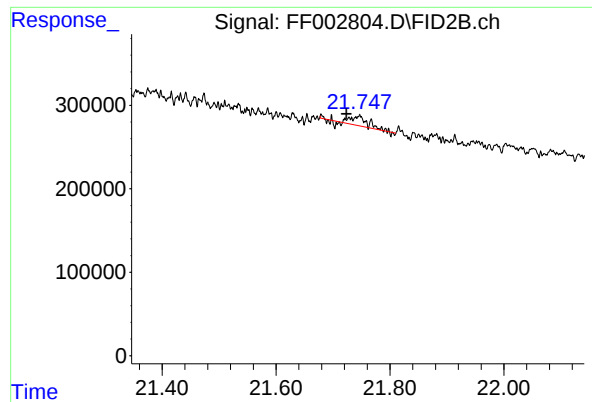

#18 N-TETRACONTANE

R.T.: 21.746 min
Delta R.T.: 0.023 min
Response: 197909
Conc: 2.26 ug/ml

Instrument :
FID_F
ClientSampleId :