

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002805.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 14:24
 Operator : AJ\SJ
 Sample : J6028-06
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 00:56:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	1969046	25.207 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243f	296809	2.569 ug/ml
5) N-HEXADECANE	9.791	95077	0.870 ug/ml
7) N-EICOSANE	12.545	148977	1.539 ug/ml
8) N-DOCOSANE	13.760	427877	4.673 ug/ml
10) N-TETRACOSANE	14.855	173553	1.948 ug/ml
11) N-HEXACOSANE	15.880	365193	4.024 ug/ml
12) N-OCTACOSANE	16.826	888456	9.315 ug/ml
13) N-TRIACONTANE	17.723	618668	6.241 ug/ml
14) N-DOTRIACONTANE	18.559	538369	5.438 ug/ml
15) N-TETRATRIACONTANE	19.375	257664	2.611 ug/ml
16) N-HEXATRIACONTANE	20.086	175673	1.843 ug/ml
17) N-OCTATRIACONTANE	20.817	419683	4.775 ug/ml
18) N-TETRACONTANE	21.733	178716	2.040 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002805.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 14:24
Operator : AJ\SJ
Sample : J6028-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 29 00:56:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

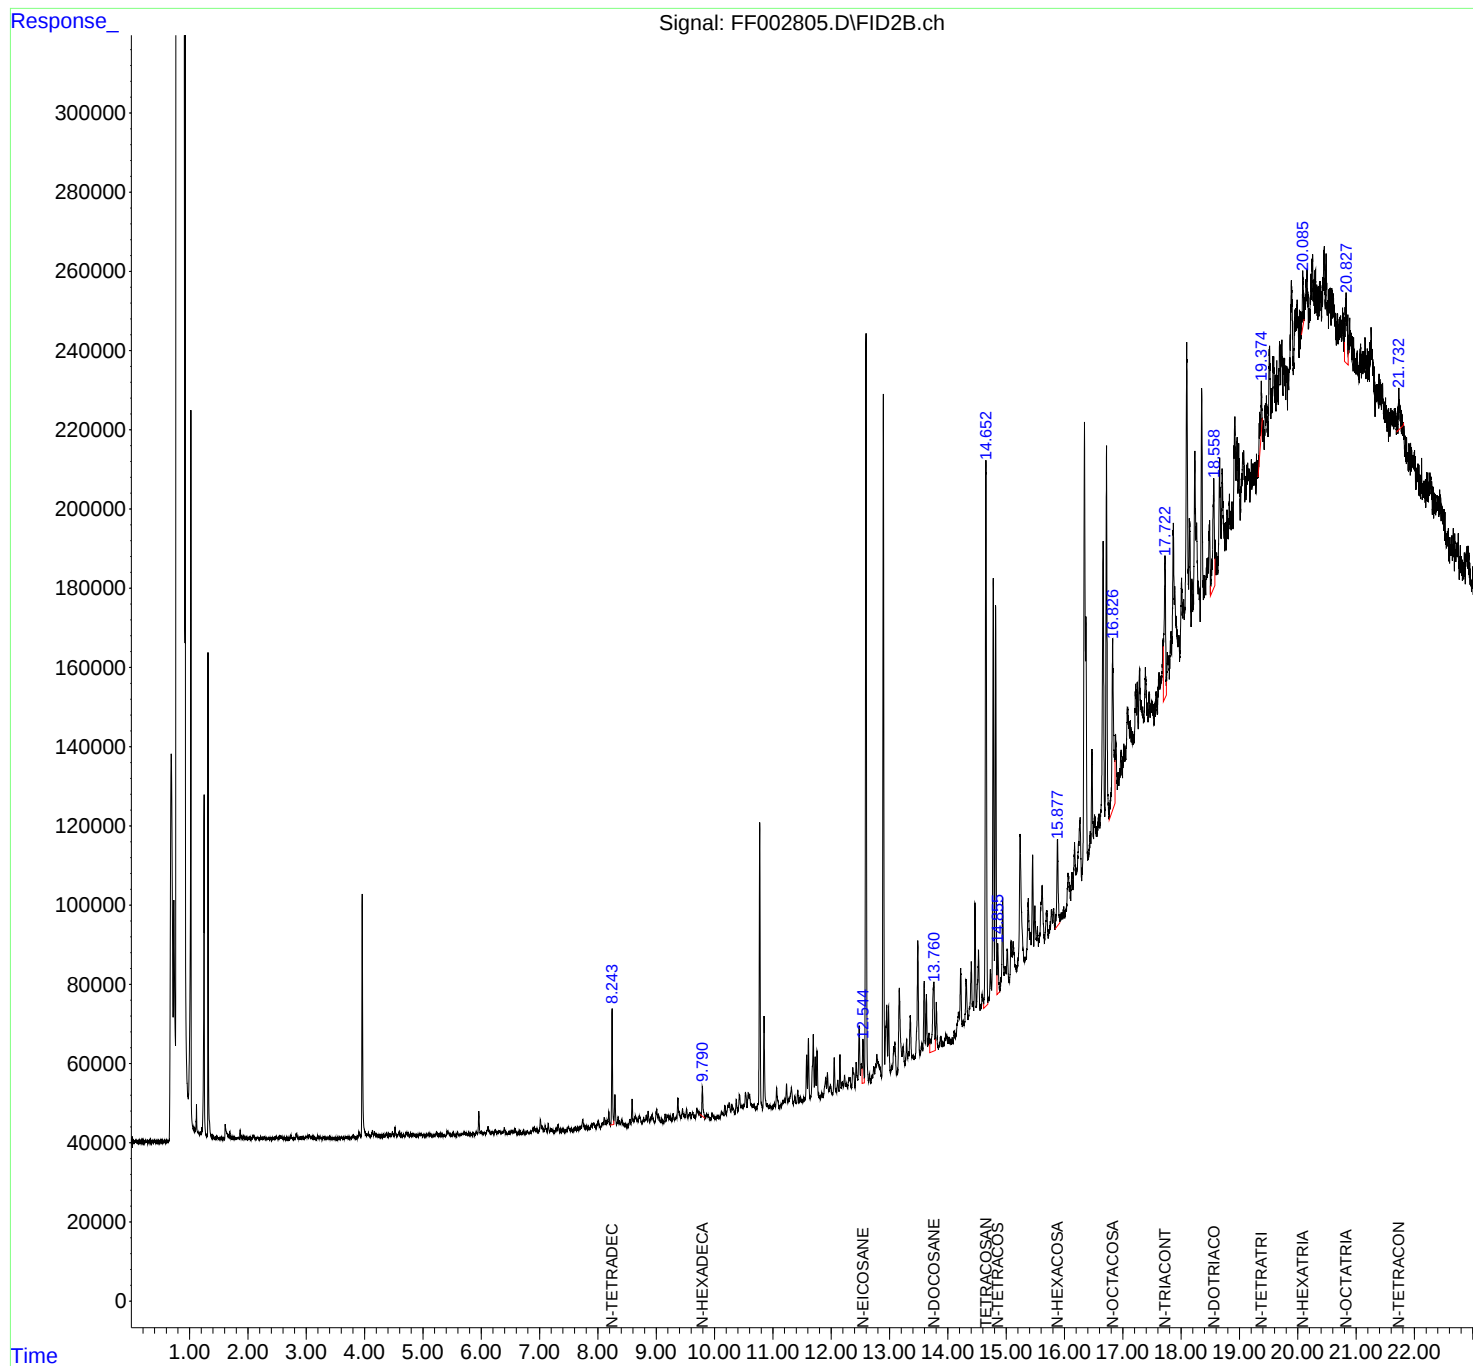


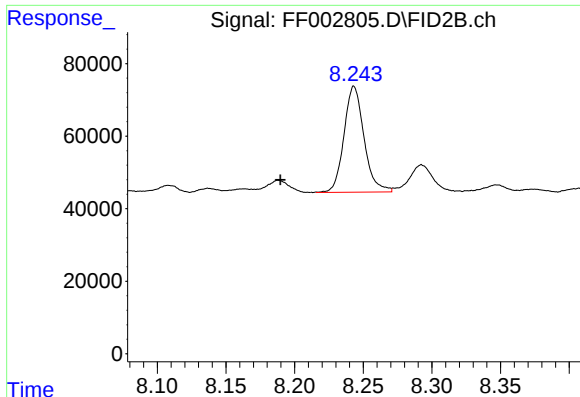

#4 N-TETRADECANE


R.T.: 8.243 min
Delta R.T.: 0.054 min
Response: 296809
Conc: 2.57 ug/ml

Instrument :
FID_F
ClientSampleId :

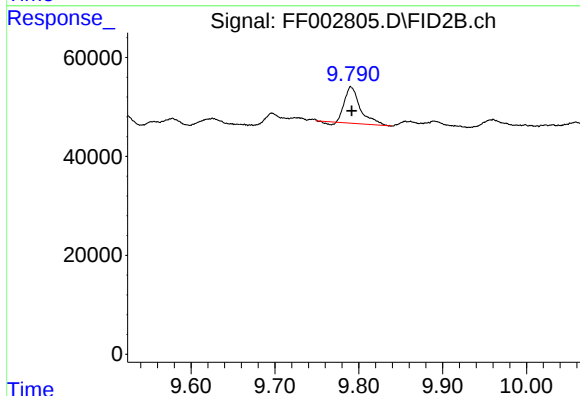


#5 N-HEXADECANE

R.T.: 9.791 min
Delta R.T.: 0.000 min
Response: 95077
Conc: 0.87 ug/ml

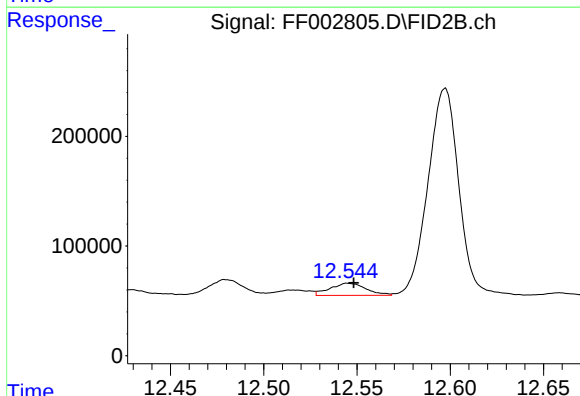


#7 N-EICOSANE

R.T.: 12.545 min
Delta R.T.: -0.003 min
Response: 148977
Conc: 1.54 ug/ml

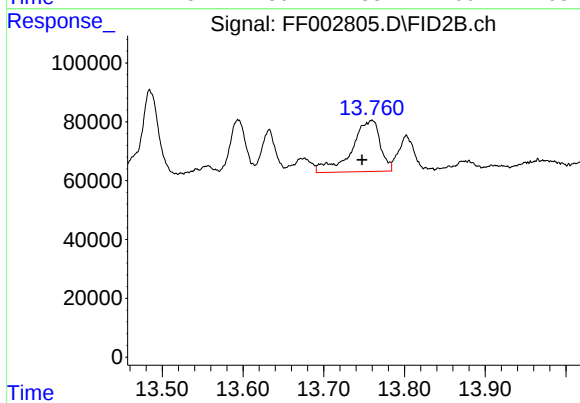

#8 N-DOCOSANE


R.T.: 13.760 min
Delta R.T.: 0.012 min
Response: 427877
Conc: 4.67 ug/ml

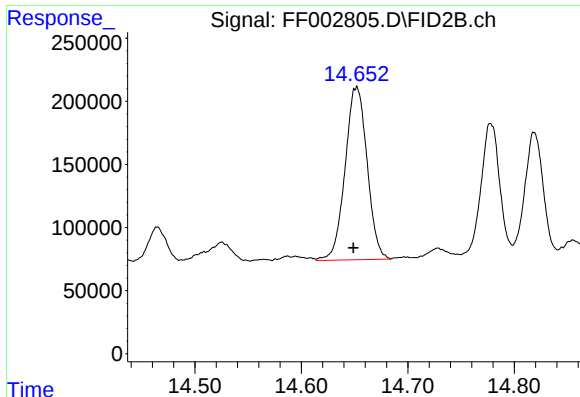

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.652 min
Delta R.T.: 0.003 min
Response: 1969046
Conc: 25.21 ug/ml

Instrument :
FID_F
ClientSampleId :

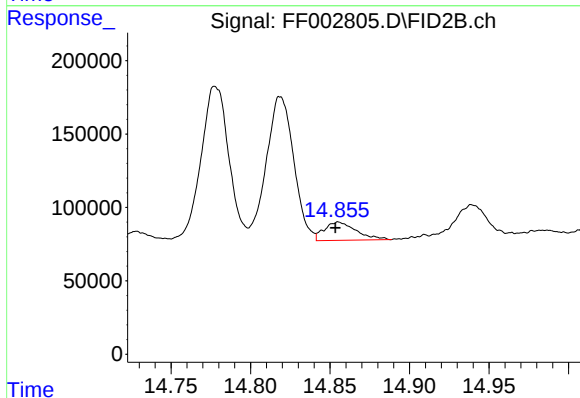


#10 N-TETRACOSANE

R.T.: 14.855 min
Delta R.T.: 0.002 min
Response: 173553
Conc: 1.95 ug/ml

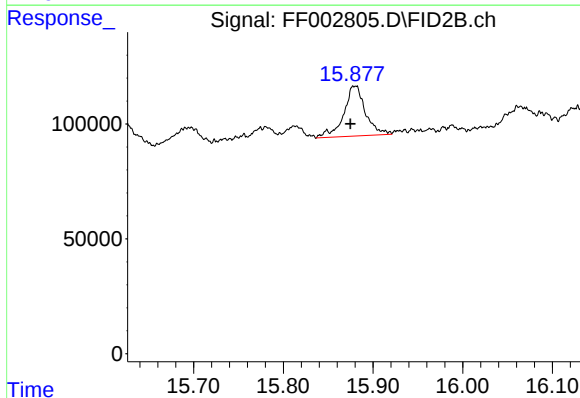


#11 N-HEXACOSANE

R.T.: 15.880 min
Delta R.T.: 0.005 min
Response: 365193
Conc: 4.02 ug/ml

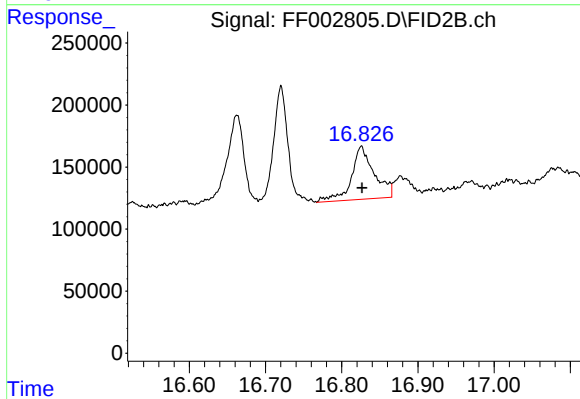

#12 N-OCTACOSANE


R.T.: 16.826 min
Delta R.T.: -0.001 min
Response: 888456
Conc: 9.31 ug/ml

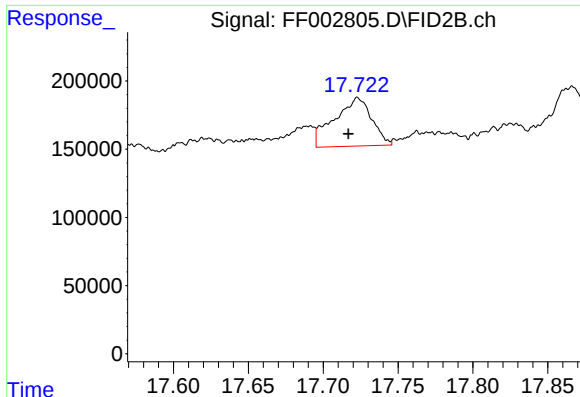

#13 N-TRIACONTANE


R.T.: 17.723 min
Delta R.T.: 0.006 min
Response: 618668
Conc: 6.24 ug/ml

Instrument :
FID_F
ClientSampleId :

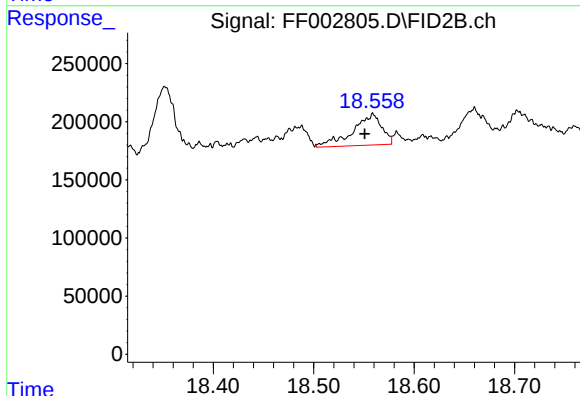


#14 N-DOTRIACONTANE

R.T.: 18.559 min
Delta R.T.: 0.009 min
Response: 538369
Conc: 5.44 ug/ml

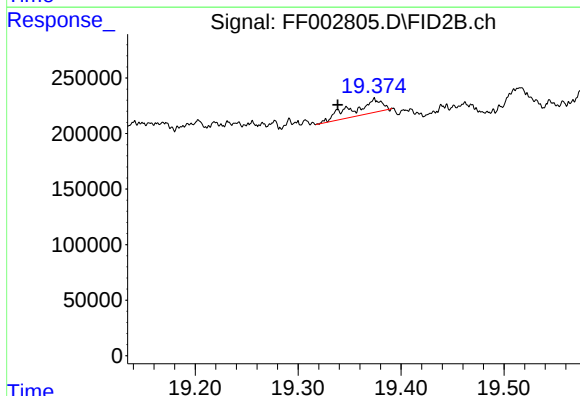


#15 N-TETRATRIACONTANE

R.T.: 19.375 min
Delta R.T.: 0.036 min
Response: 257664
Conc: 2.61 ug/ml

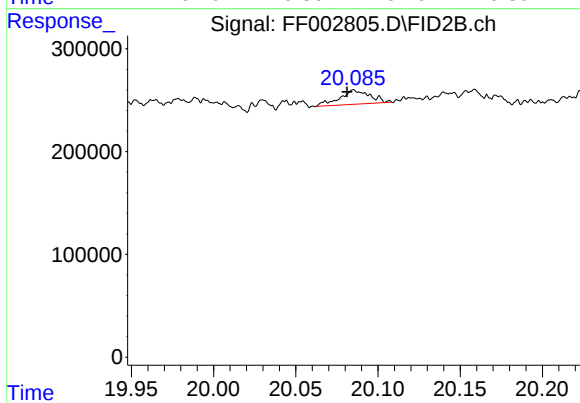

#16 N-HEXATRIACONTANE


R.T.: 20.086 min
Delta R.T.: 0.005 min
Response: 175673
Conc: 1.84 ug/ml

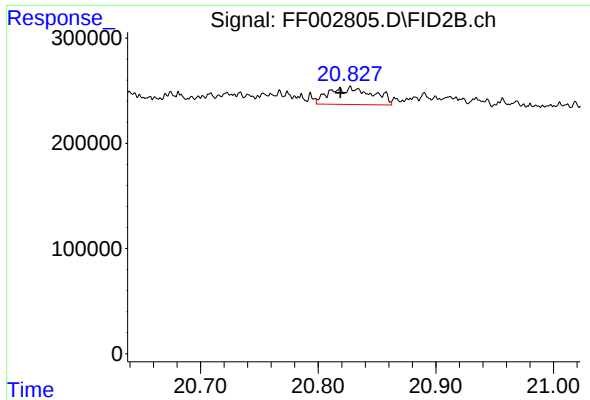

#17 N-OCTATRIACONTANE

R.T.: 20.817 min
Delta R.T.: -0.002 min
Response: 419683
Conc: 4.78 ug/ml

Instrument :
FID_F
ClientSampleId :

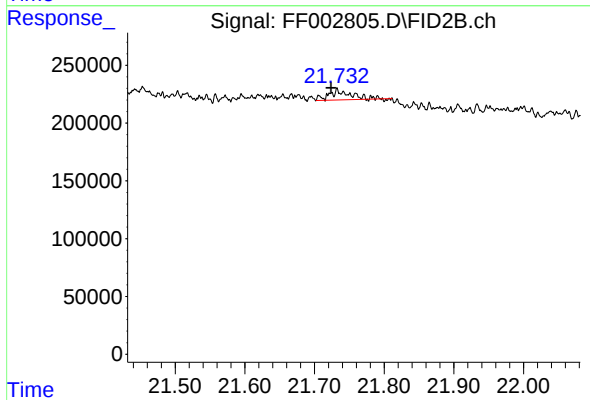

#18 N-TETRACONTANE

R.T.: 21.733 min
Delta R.T.: 0.009 min
Response: 178716
Conc: 2.04 ug/ml