

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002808.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 15:56
 Operator : AJ\SJ
 Sample : J6080-04
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 00:56:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.653	1651564	21.142 ug/ml
Target Compounds			
4) N-TETRADECANE	8.244f	437210	3.785 ug/ml
5) N-HEXADECANE	9.792	106443	0.974 ug/ml
7) N-EICOSANE	12.547	107791	1.113 ug/ml
8) N-DOCOSANE	13.762	236844	2.587 ug/ml
10) N-TETRACOSANE	14.820	608893	6.835 ug/ml
11) N-HEXACOSANE	15.881	218129	2.404 ug/ml
12) N-OCTACOSANE	16.828	659078	6.910 ug/ml
13) N-TRIACONTANE	17.723	398993	4.025 ug/ml
14) N-DOTRIACONTANE	18.552	863501	8.723 ug/ml
15) N-TETRATRIACONTANE	19.349	188181	1.907 ug/ml
17) N-OCTATRIACONTANE	20.806	546859	6.222 ug/ml
18) N-TETRACONTANE	21.759	1864876	21.290 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002808.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 15:56
Operator : AJ\SJ
Sample : J6080-04
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 00:56:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

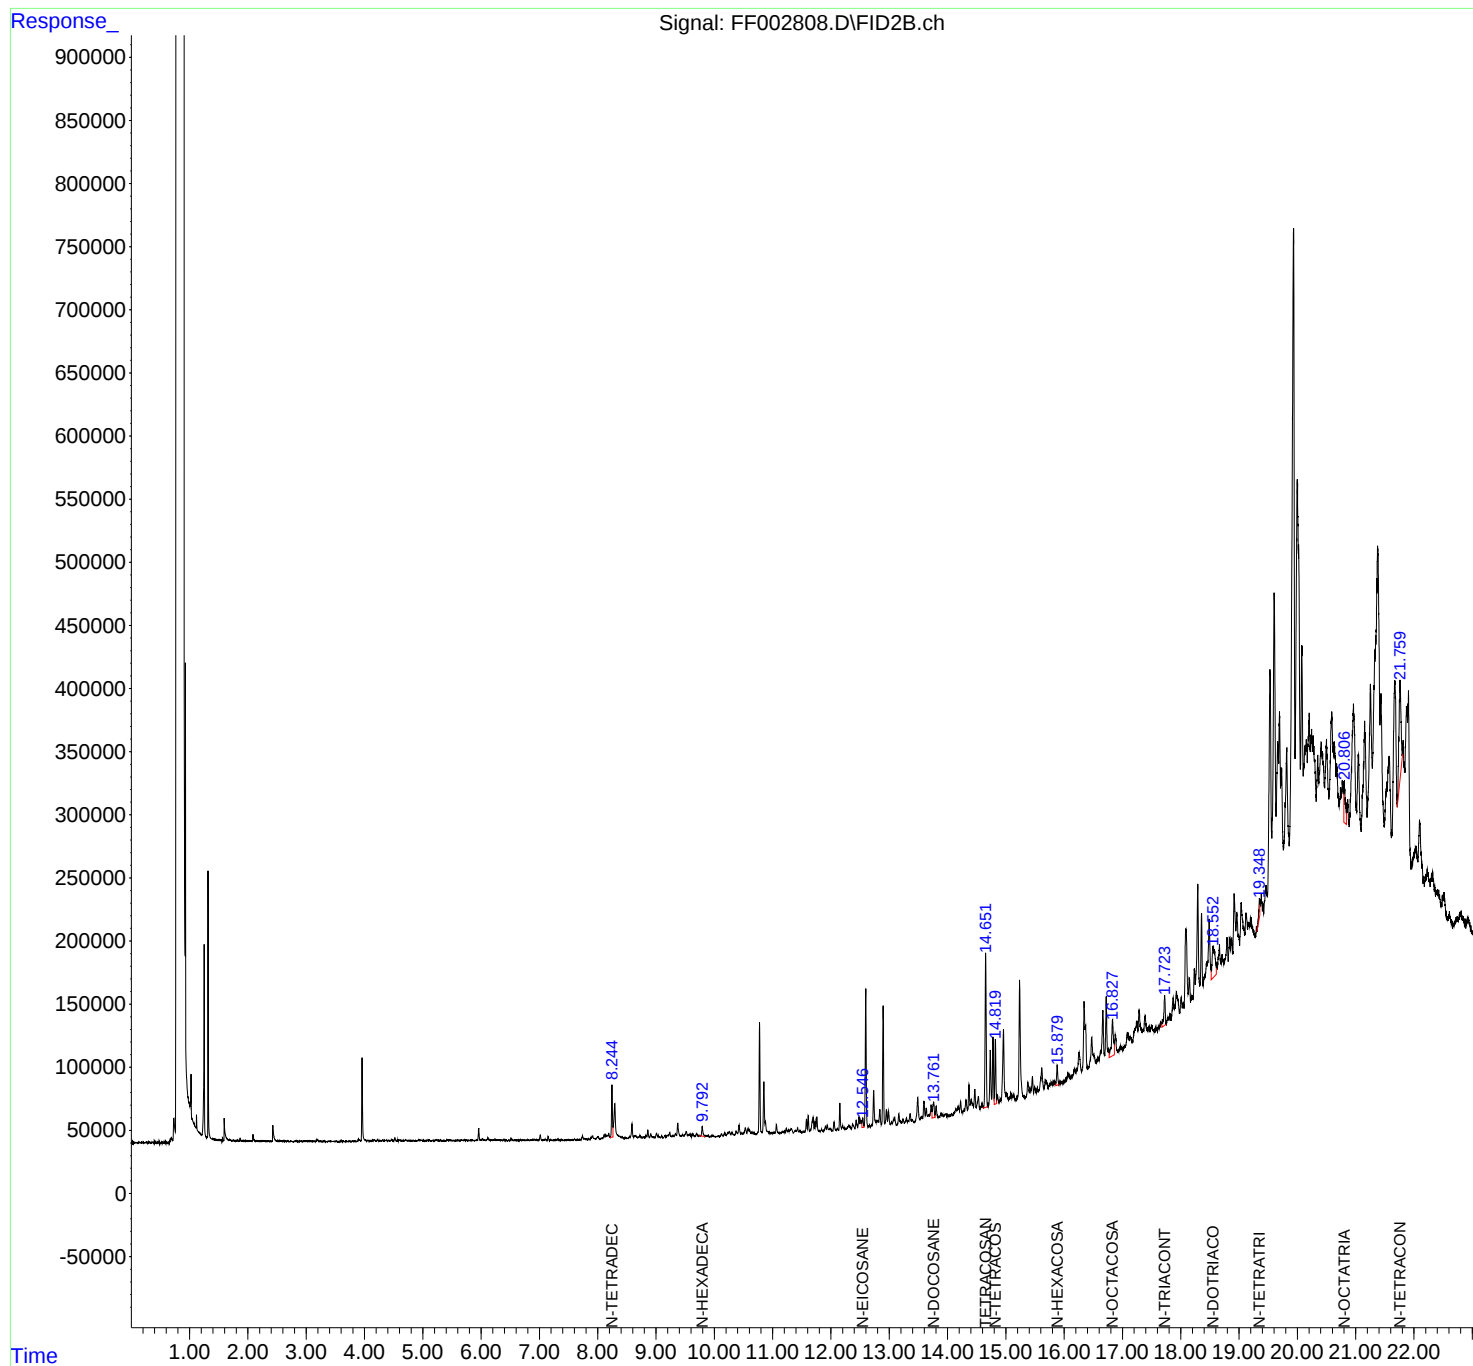


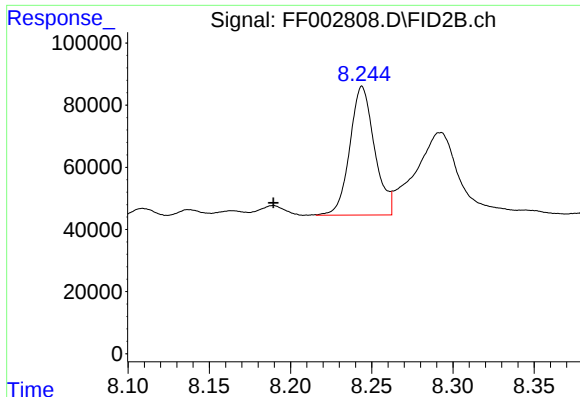

#4 N-TETRADECANE


R.T.: 8.244 min
Delta R.T.: 0.055 min
Response: 437210
Conc: 3.78 ug/ml

Instrument :
FID_F
ClientSampleId :

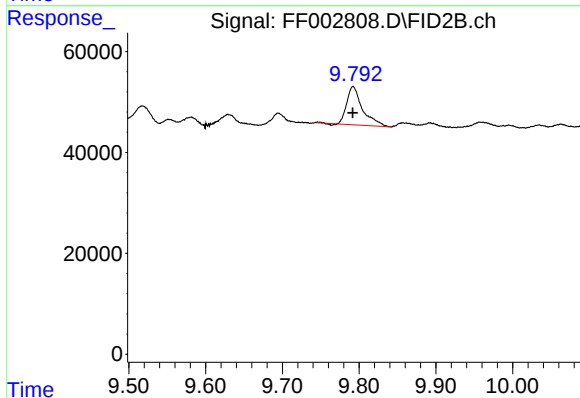


#5 N-HEXADECANE

R.T.: 9.792 min
Delta R.T.: 0.000 min
Response: 106443
Conc: 0.97 ug/ml

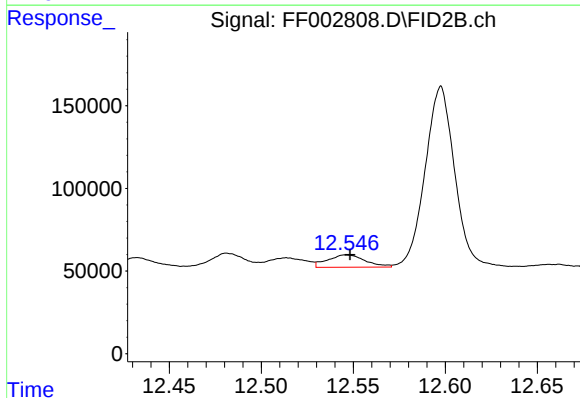


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: -0.002 min
Response: 107791
Conc: 1.11 ug/ml

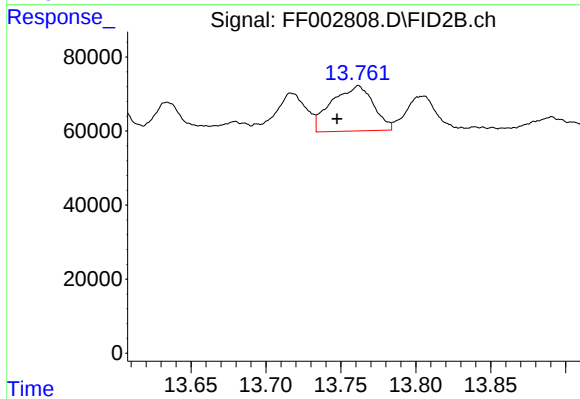

#8 N-DOCOSANE


R.T.: 13.762 min
Delta R.T.: 0.014 min
Response: 236844
Conc: 2.59 ug/ml

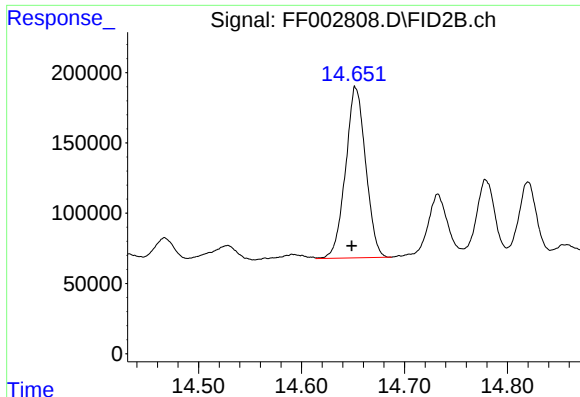

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.653 min
Delta R.T.: 0.004 min
Response: 1651564
Conc: 21.14 ug/ml

Instrument :
FID_F
ClientSampleId :

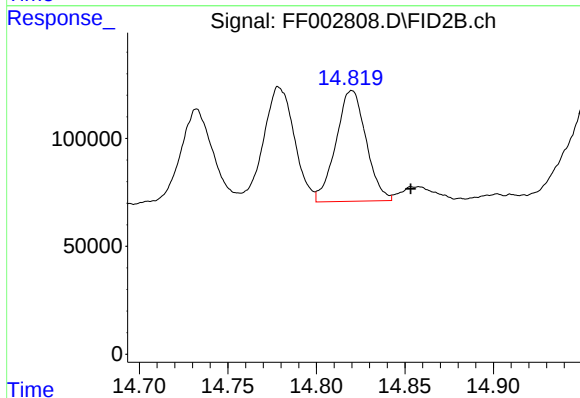


#10 N-TETRACOSANE

R.T.: 14.820 min
Delta R.T.: -0.033 min
Response: 608893
Conc: 6.83 ug/ml

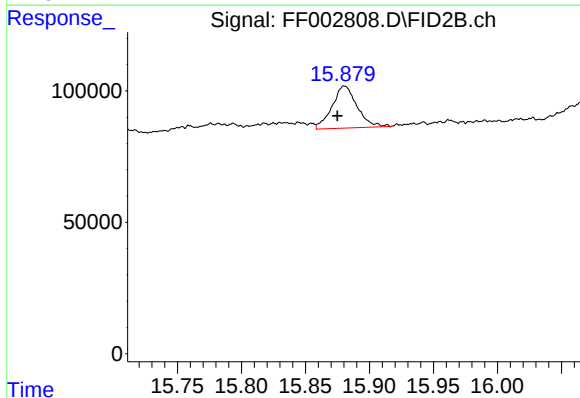


#11 N-HEXACOSANE

R.T.: 15.881 min
Delta R.T.: 0.006 min
Response: 218129
Conc: 2.40 ug/ml

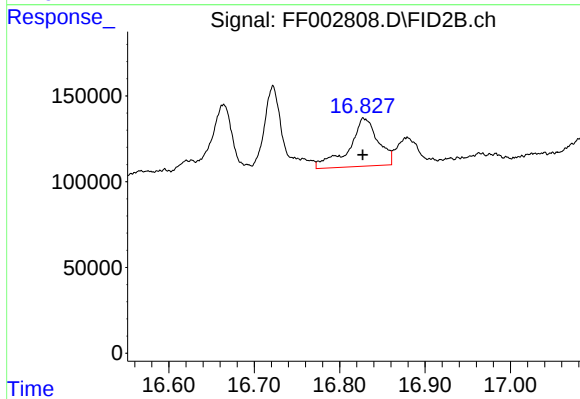

#12 N-OCTACOSANE


R.T.: 16.828 min
Delta R.T.: 0.000 min
Response: 659078
Conc: 6.91 ug/ml

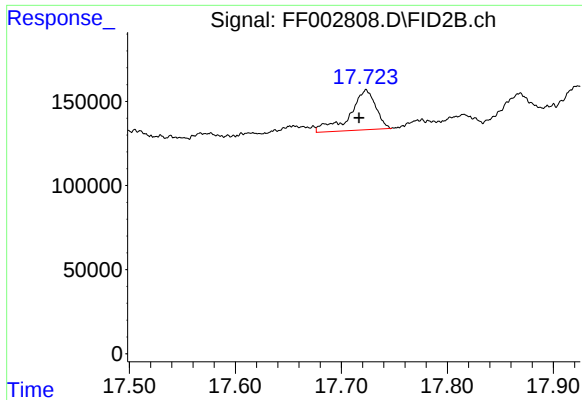

#13 N-TRIACONTANE


R.T.: 17.723 min
Delta R.T.: 0.007 min
Response: 398993
Conc: 4.02 ug/ml

Instrument :
FID_F
ClientSampleId :

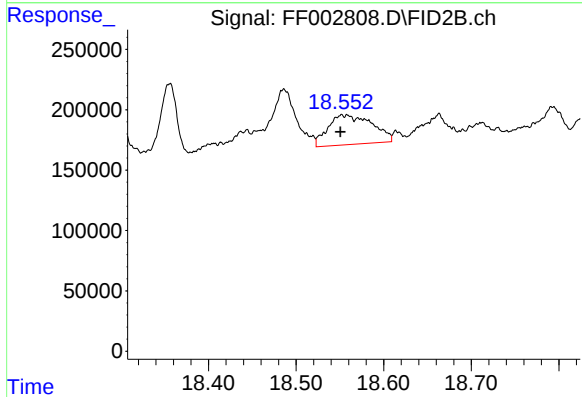


#14 N-DOTRIACONTANE

R.T.: 18.552 min
Delta R.T.: 0.001 min
Response: 863501
Conc: 8.72 ug/ml

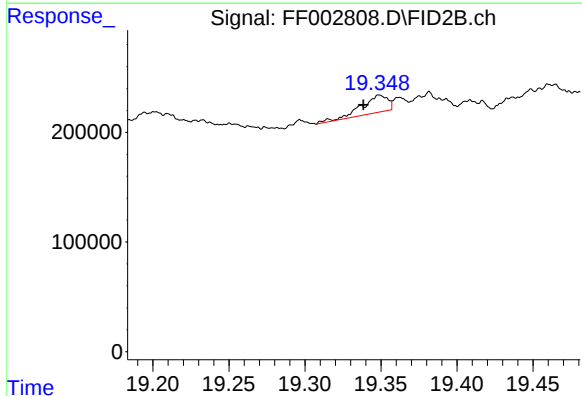


#15 N-TETRATRIACONTANE

R.T.: 19.349 min
Delta R.T.: 0.011 min
Response: 188181
Conc: 1.91 ug/ml

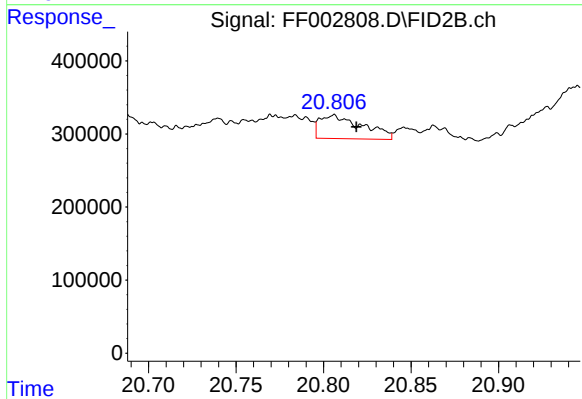

#17 N-OCTATRIACONTANE

R.T.: 20.806 min
Delta R.T.: -0.013 min
Response: 546859
Conc: 6.22 ug/ml

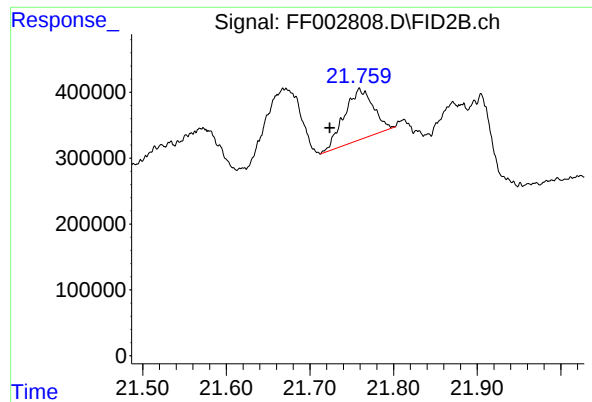

#18 N-TETRACONTANE

R.T.: 21.759 min
Delta R.T.: 0.035 min
Response: 1864876
Conc: 21.29 ug/ml

Instrument :
FID_F
ClientSampleId :