

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002809.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 16:27
 Operator : AJ\SJ
 Sample : J6080-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 00:57:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	1491066	19.088 ug/ml
Target Compounds			
4) N-TETRADECANE	8.244f	269244	2.331 ug/ml
5) N-HEXADECANE	9.793	120086	1.098 ug/ml
7) N-EICOSANE	12.548	100024	1.033 ug/ml
8) N-DOCOSANE	13.761	223745	2.444 ug/ml
10) N-TETRACOSANE	14.819	584522	6.561 ug/ml
11) N-HEXACOSANE	15.880	137347	1.513 ug/ml
12) N-OCTACOSANE	16.827	357017	3.743 ug/ml
13) N-TRIACONTANE	17.722	382839	3.862 ug/ml
14) N-DOTRIACONTANE	18.550	561599	5.673 ug/ml
15) N-TETRATRIACONTANE	19.339	121751	1.234 ug/ml
16) N-HEXATRIACONTANE	20.088	58571	0.615 ug/ml
17) N-OCTATRIACONTANE	20.838	261059	2.970 ug/ml
18) N-TETRACONTANE	21.731	1935259	22.093 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002809.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 16:27
Operator : AJ\SJ
Sample : J6080-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 29 00:57:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

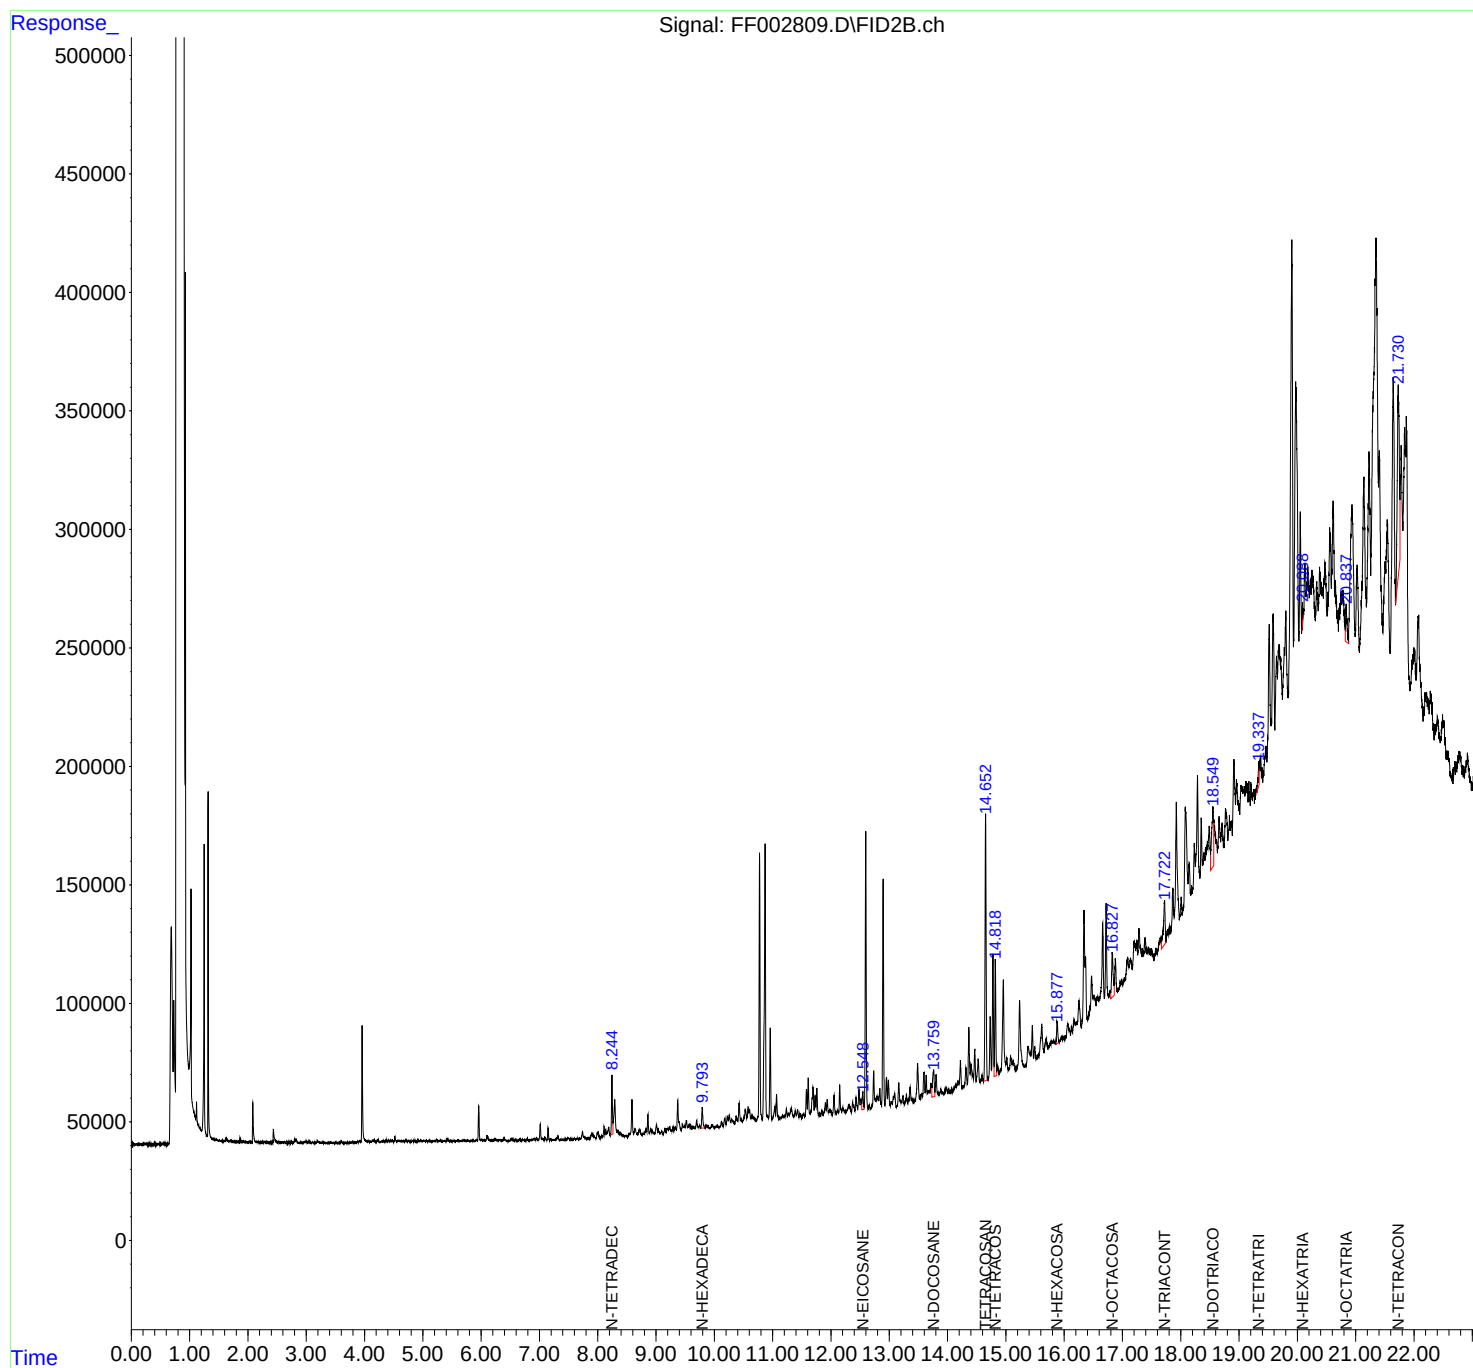


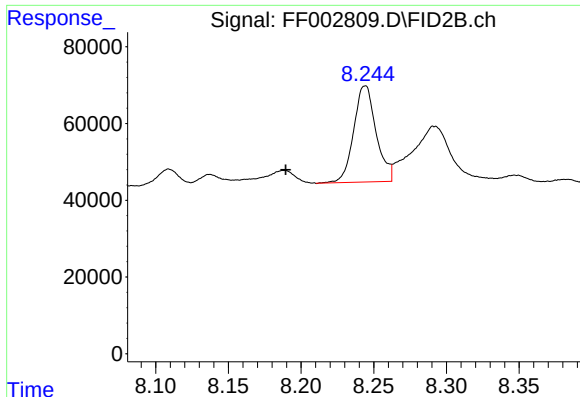

#4 N-TETRADECANE


R.T.: 8.244 min
Delta R.T.: 0.055 min
Response: 269244
Conc: 2.33 ug/ml

Instrument :
FID_F
ClientSampleId :

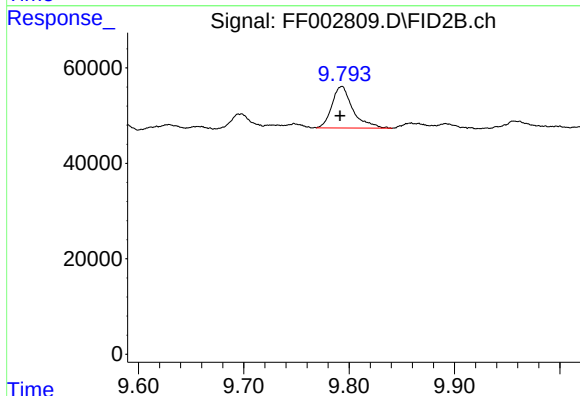


#5 N-HEXADECANE

R.T.: 9.793 min
Delta R.T.: 0.002 min
Response: 120086
Conc: 1.10 ug/ml

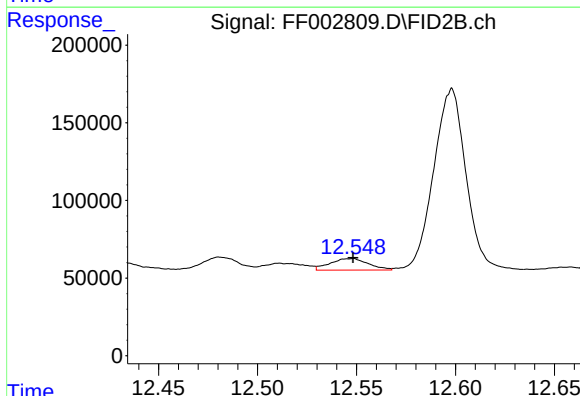


#7 N-EICOSANE

R.T.: 12.548 min
Delta R.T.: 0.000 min
Response: 100024
Conc: 1.03 ug/ml

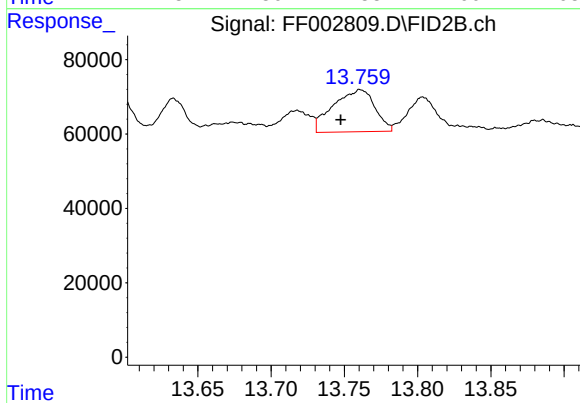

#8 N-DOCOSANE


R.T.: 13.761 min
Delta R.T.: 0.013 min
Response: 223745
Conc: 2.44 ug/ml

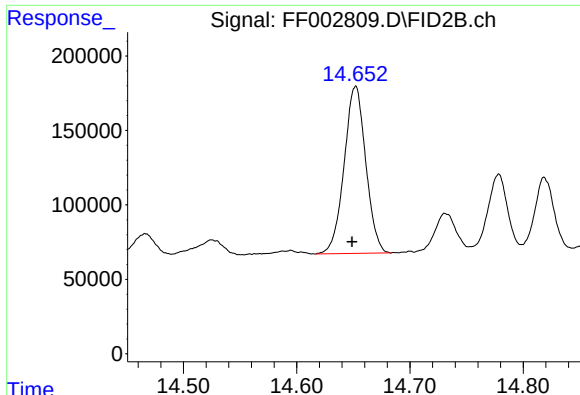

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.652 min
Delta R.T.: 0.003 min
Response: 1491066
Conc: 19.09 ug/ml

Instrument :
FID_F
ClientSampleId :

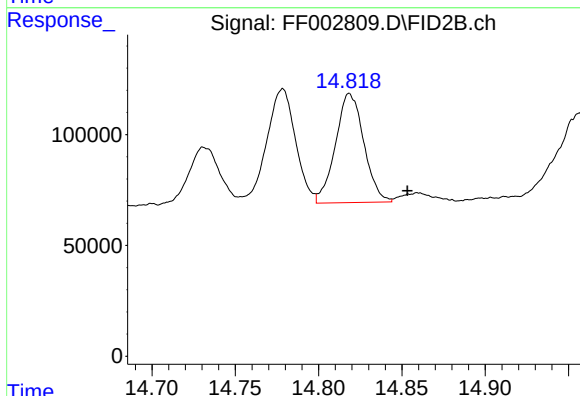


#10 N-TETRACOSANE

R.T.: 14.819 min
Delta R.T.: -0.035 min
Response: 584522
Conc: 6.56 ug/ml

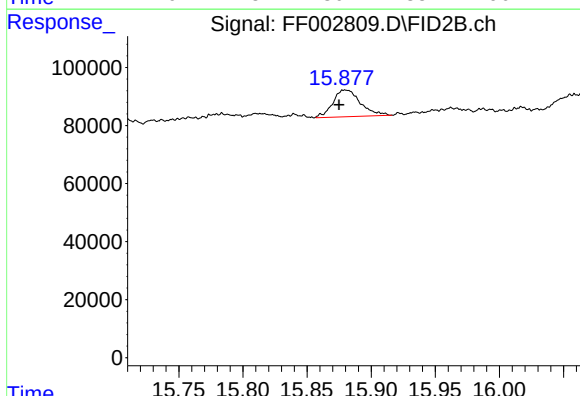


#11 N-HEXACOSANE

R.T.: 15.880 min
Delta R.T.: 0.005 min
Response: 137347
Conc: 1.51 ug/ml

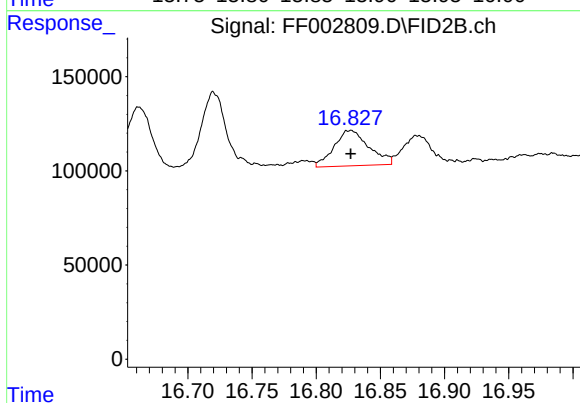

#12 N-OCTACOSANE


R.T.: 16.827 min
Delta R.T.: 0.000 min
Response: 357017
Conc: 3.74 ug/ml

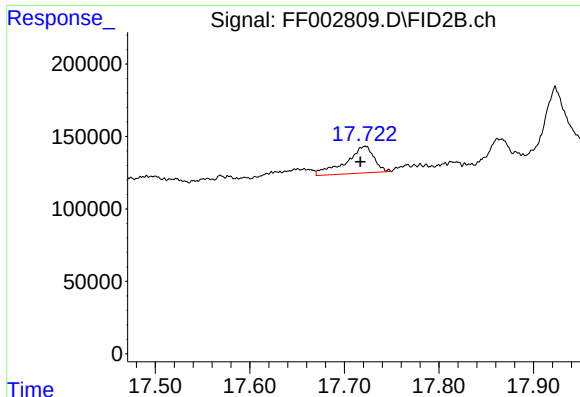

#13 N-TRIACONTANE


R.T.: 17.722 min
Delta R.T.: 0.005 min
Response: 382839
Conc: 3.86 ug/ml

Instrument :
FID_F
ClientSampleId :

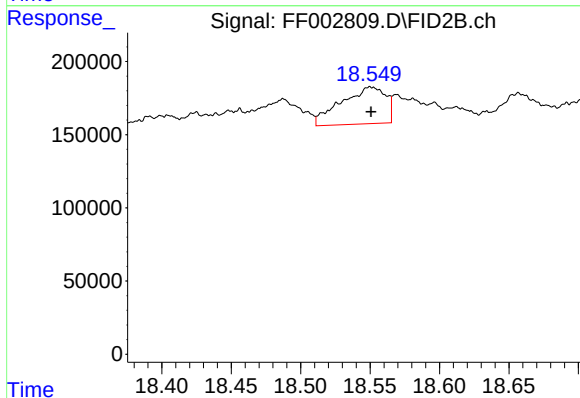


#14 N-DOTRIACONTANE

R.T.: 18.550 min
Delta R.T.: 0.000 min
Response: 561599
Conc: 5.67 ug/ml

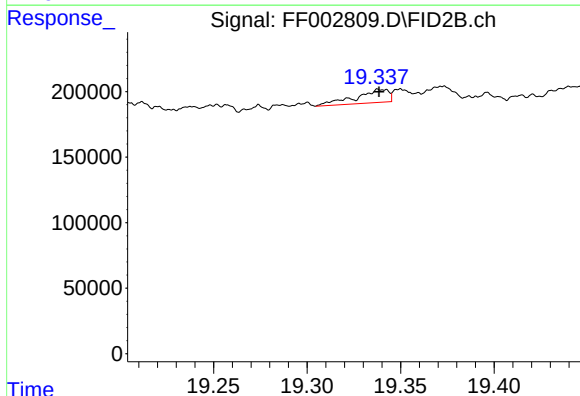


#15 N-TETRATRIACONTANE

R.T.: 19.339 min
Delta R.T.: 0.000 min
Response: 121751
Conc: 1.23 ug/ml

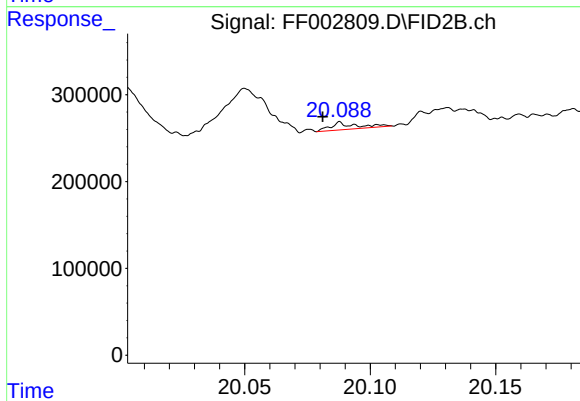

#16 N-HEXATRIACONTANE


R.T.: 20.088 min
Delta R.T.: 0.007 min
Response: 58571
Conc: 0.61 ug/ml

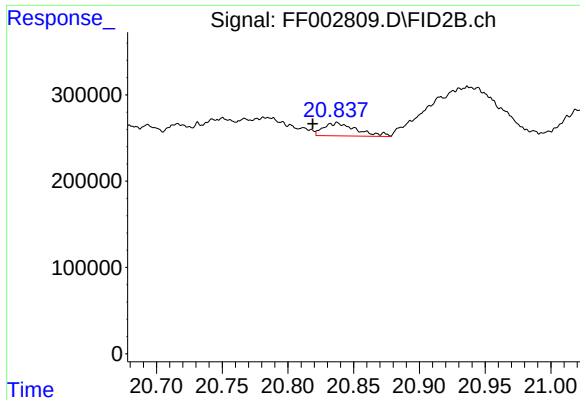

#17 N-OCTATRIACONTANE

R.T.: 20.838 min
Delta R.T.: 0.019 min
Response: 261059
Conc: 2.97 ug/ml

Instrument :
FID_F
ClientSampleId :

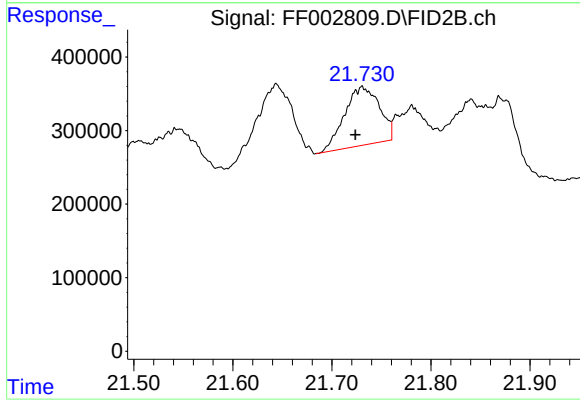

#18 N-TETRACONTANE

R.T.: 21.731 min
Delta R.T.: 0.007 min
Response: 1935259
Conc: 22.09 ug/ml