

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002810.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 16:57
 Operator : AJ\SJ
 Sample : J6080-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:00:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.653	1372614	17.571 ug/ml
Target Compounds			
4) N-TETRADECANE	8.244f	255720	2.214 ug/ml
7) N-EICOSANE	12.597	1113905	11.504 ug/ml
10) N-TETRACOSANE	14.819	465008	5.220 ug/ml
11) N-HEXACOSANE	15.879	127221	1.402 ug/ml
12) N-OCTACOSANE	16.826	310924	3.260 ug/ml
13) N-TRIACONTANE	17.721	249947	2.521 ug/ml
14) N-DOTRIACONTANE	18.554	787619	7.956 ug/ml
15) N-TETRATRIACONTANE	19.360	61220	0.620 ug/ml
16) N-HEXATRIACONTANE	20.040	155749	1.634 ug/ml
17) N-OCTATRIACONTANE	20.776	316741	3.604 ug/ml
18) N-TETRACONTANE	21.708	1438671	16.424 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002810.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 16:57
Operator : AJ\SJ
Sample : J6080-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:00:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

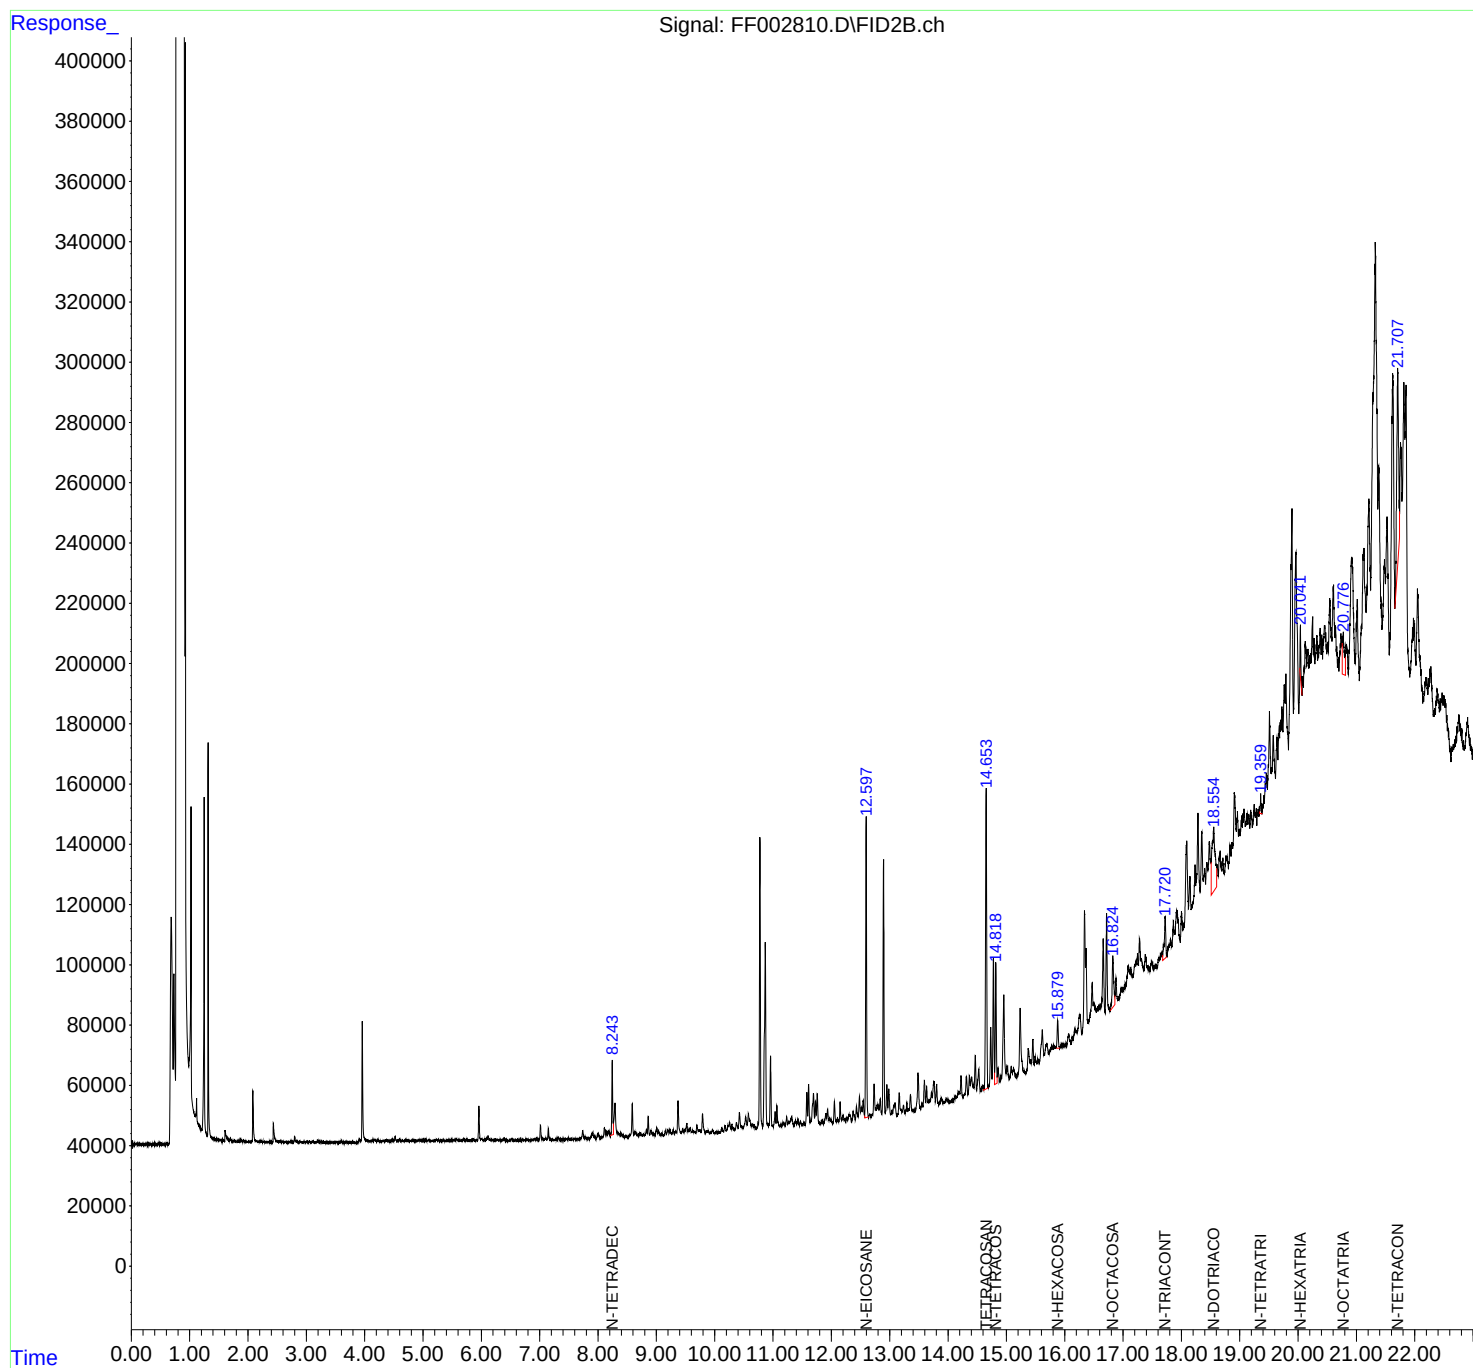


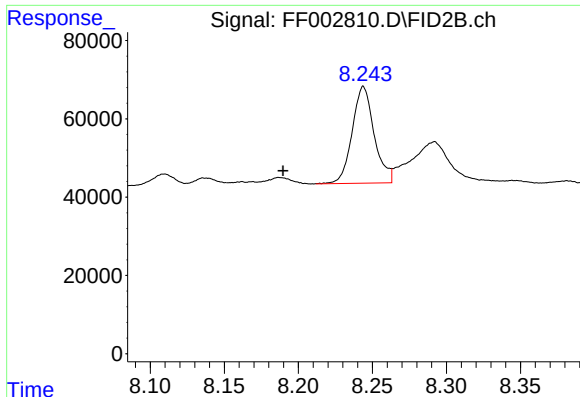

#4 N-TETRADECANE


R.T.: 8.244 min
Delta R.T.: 0.054 min
Response: 255720
Conc: 2.21 ug/ml

Instrument :
FID_F
ClientSampleId :

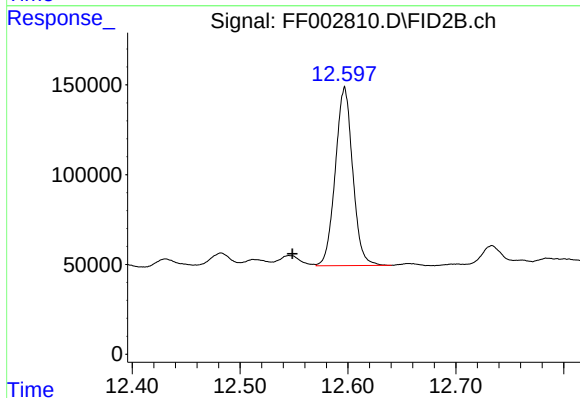


#7 N-EICOSANE

R.T.: 12.597 min
Delta R.T.: 0.049 min
Response: 1113905
Conc: 11.50 ug/ml

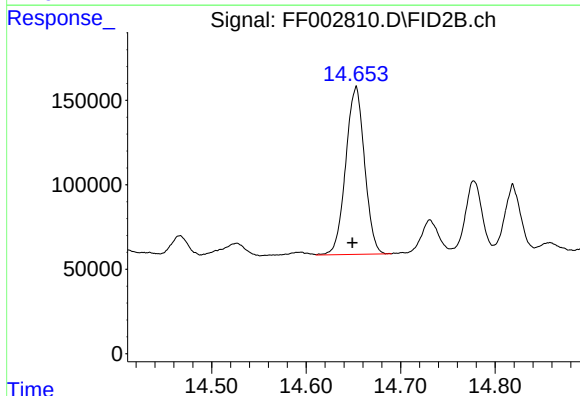


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.653 min
Delta R.T.: 0.004 min
Response: 1372614
Conc: 17.57 ug/ml

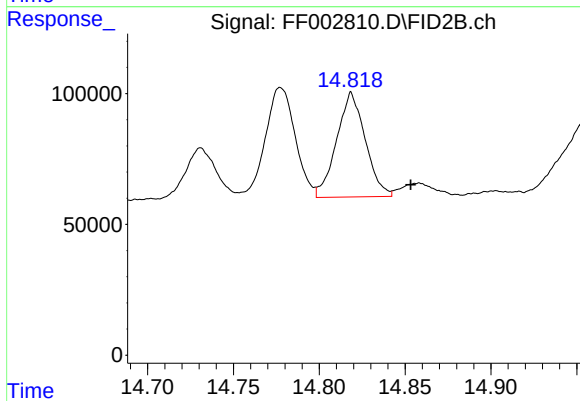

#10 N-TETRACOSANE


R.T.: 14.819 min
Delta R.T.: -0.035 min
Response: 465008
Conc: 5.22 ug/ml

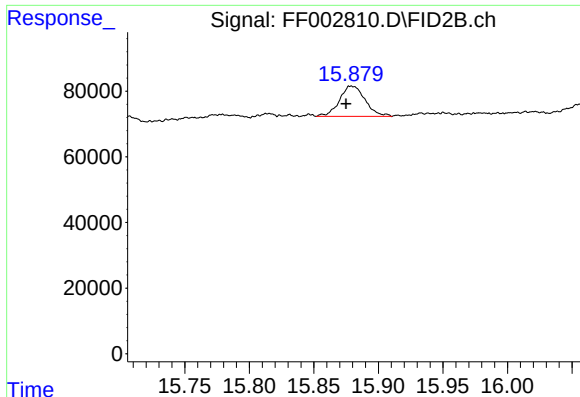

#11 N-HEXACOSANE


R.T.: 15.879 min
Delta R.T.: 0.004 min
Response: 127221
Conc: 1.40 ug/ml

Instrument :
FID_F
ClientSampleId :

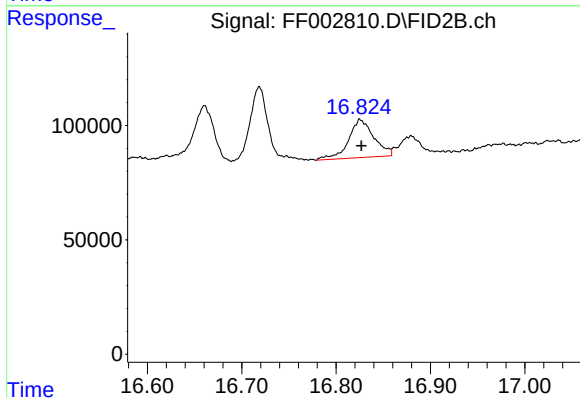


#12 N-OCTACOSANE

R.T.: 16.826 min
Delta R.T.: -0.001 min
Response: 310924
Conc: 3.26 ug/ml

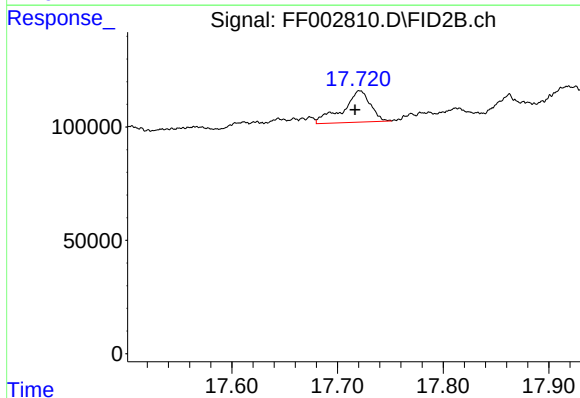


#13 N-TRIACONTANE

R.T.: 17.721 min
Delta R.T.: 0.004 min
Response: 249947
Conc: 2.52 ug/ml

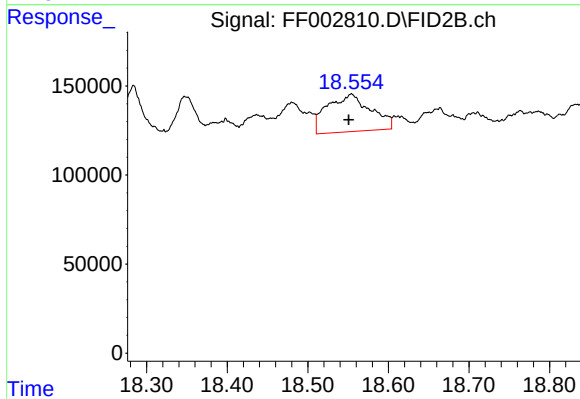

#14 N-DOTRIACONTANE


R.T.: 18.554 min
Delta R.T.: 0.003 min
Response: 787619
Conc: 7.96 ug/ml

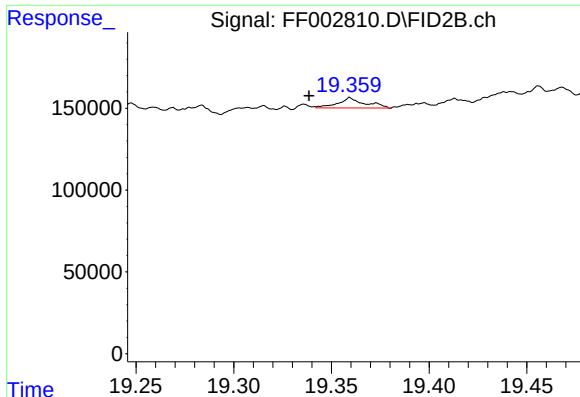

#15 N-TETRATRIACONTANE


R.T.: 19.360 min
Delta R.T.: 0.021 min
Response: 61220
Conc: 0.62 ug/ml

Instrument :
FID_F
ClientSampleId :

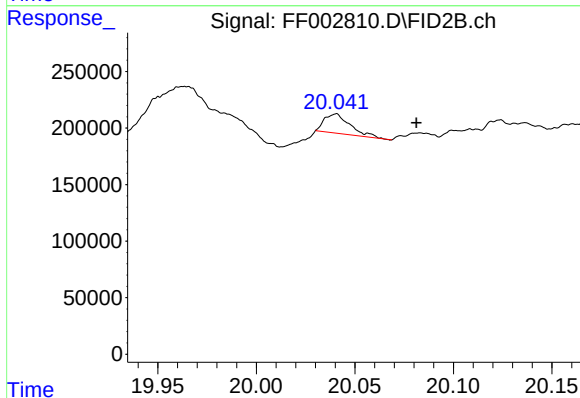


#16 N-HEXATRIACONTANE

R.T.: 20.040 min
Delta R.T.: -0.041 min
Response: 155749
Conc: 1.63 ug/ml

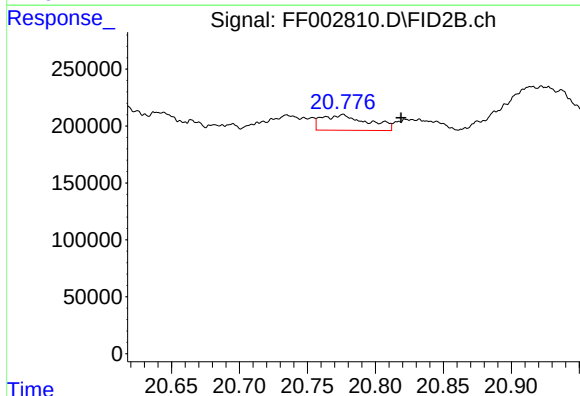

#17 N-OCTATRIACONTANE

R.T.: 20.776 min
Delta R.T.: -0.042 min
Response: 316741
Conc: 3.60 ug/ml

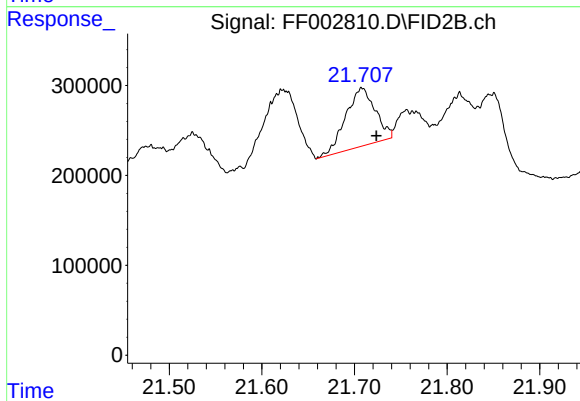

#18 N-TETRACONTANE

R.T.: 21.708 min
Delta R.T.: -0.015 min
Response: 1438671
Conc: 16.42 ug/ml