

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002811.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 17:28
 Operator : AJ\SJ
 Sample : J6080-01
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:00:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.652	1753849	22.452 ug/ml
Target Compounds			
4) N-TETRADECANE	8.244f	282145	2.442 ug/ml
5) N-HEXADECANE	9.791	117314	1.073 ug/ml
7) N-EICOSANE	12.547	95439	0.986 ug/ml
8) N-DOCOSANE	13.752	145357	1.588 ug/ml
10) N-TETRACOSANE	14.819	354504	3.979 ug/ml
11) N-HEXACOSANE	15.879	193403	2.131 ug/ml
12) N-OCTACOSANE	16.828	479154	5.024 ug/ml
13) N-TRIACONTANE	17.722	409515	4.131 ug/ml
14) N-DOTRIACONTANE	18.553	793436	8.015 ug/ml
15) N-TETRATRIACONTANE	19.340	81862	0.829 ug/ml
16) N-HEXATRIACONTANE	20.091	7711	0.081 ug/ml
17) N-OCTATRIACONTANE	20.828	265358	3.019 ug/ml
18) N-TETRACONTANE	21.747	269206	3.073 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002811.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 17:28
Operator : AJ\SJ
Sample : J6080-01
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 29 01:00:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

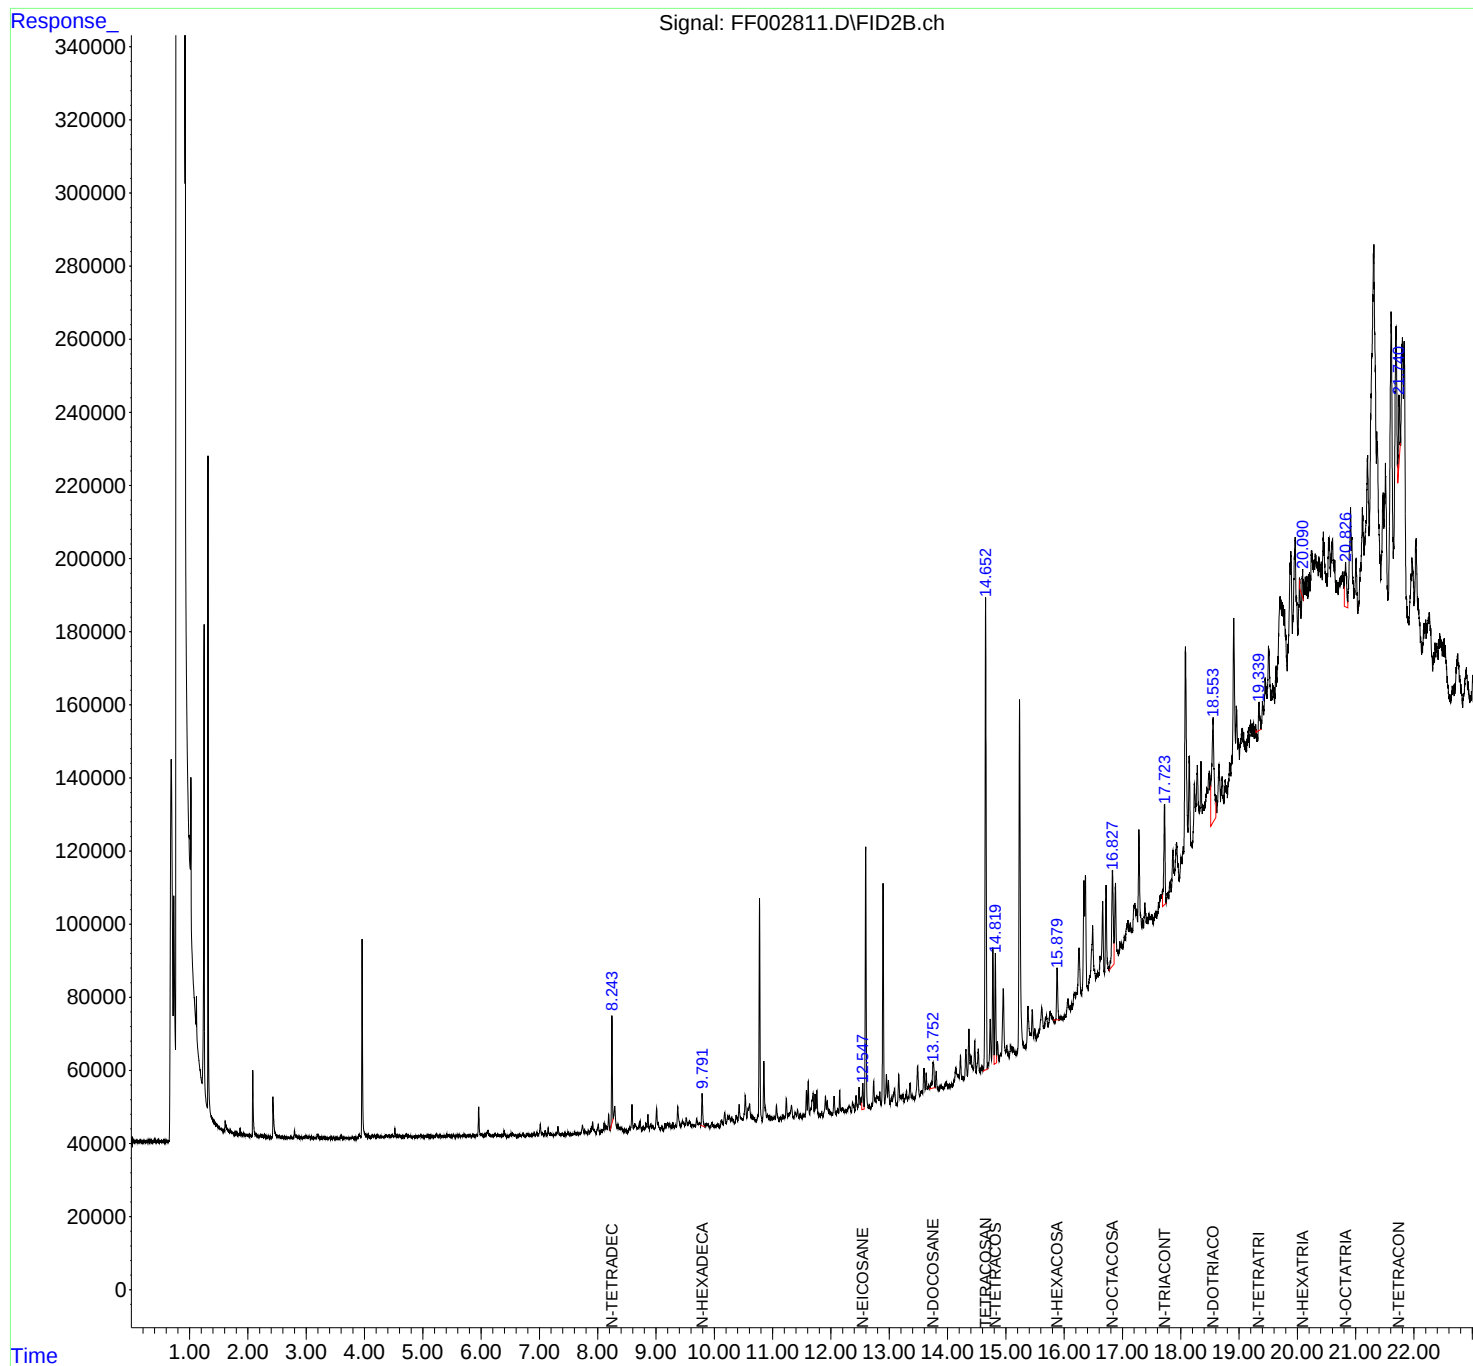


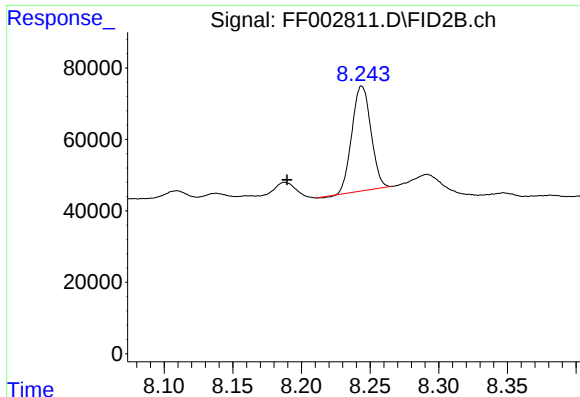

#4 N-TETRADECANE


R.T.: 8.244 min
Delta R.T.: 0.054 min
Response: 282145
Conc: 2.44 ug/ml

Instrument :
FID_F
ClientSampleId :

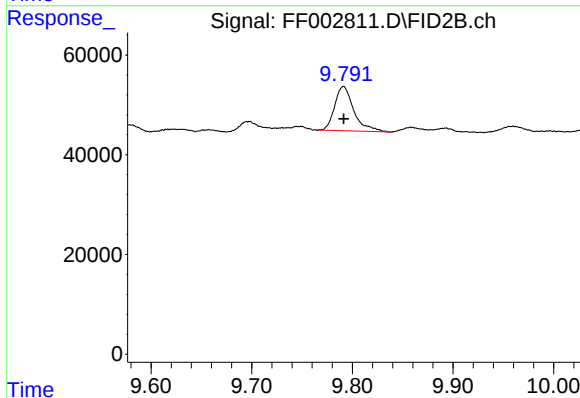


#5 N-HEXADECANE

R.T.: 9.791 min
Delta R.T.: 0.000 min
Response: 117314
Conc: 1.07 ug/ml

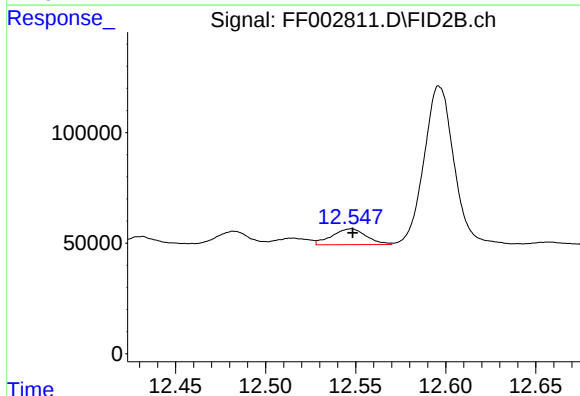


#7 N-EICOSANE

R.T.: 12.547 min
Delta R.T.: 0.000 min
Response: 95439
Conc: 0.99 ug/ml

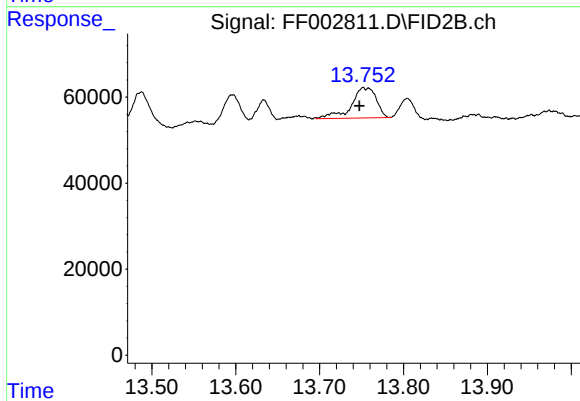

#8 N-DOCOSANE


R.T.: 13.752 min
Delta R.T.: 0.004 min
Response: 145357
Conc: 1.59 ug/ml

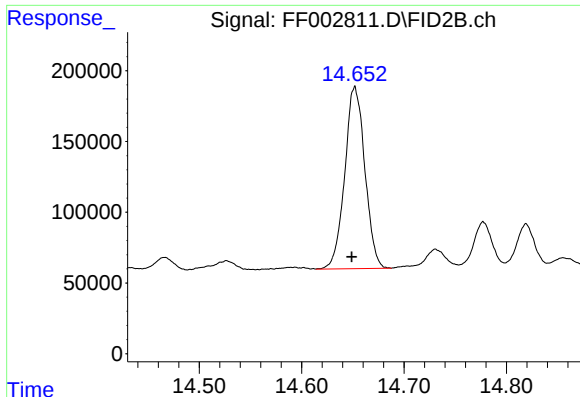

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.652 min
Delta R.T.: 0.003 min
Response: 1753849
Conc: 22.45 ug/ml

Instrument :
FID_F
ClientSampleId :

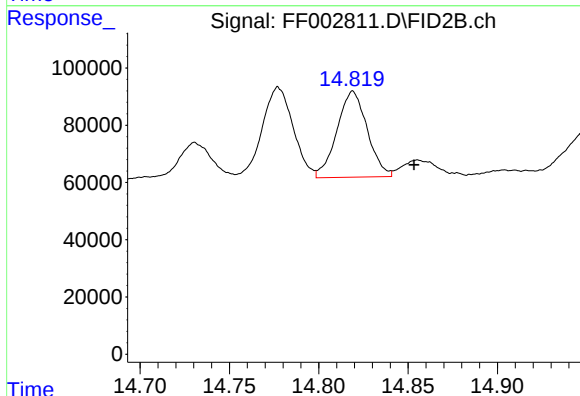


#10 N-TETRACOSANE

R.T.: 14.819 min
Delta R.T.: -0.034 min
Response: 354504
Conc: 3.98 ug/ml

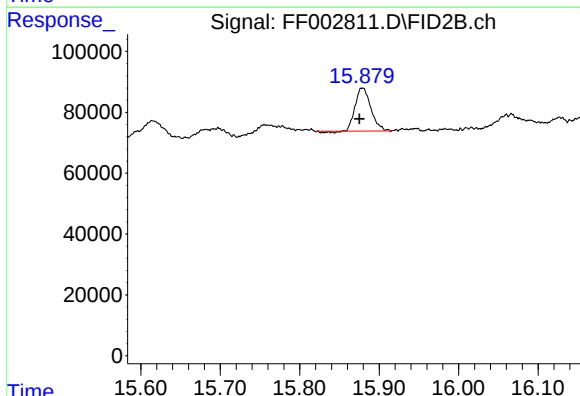


#11 N-HEXACOSANE

R.T.: 15.879 min
Delta R.T.: 0.004 min
Response: 193403
Conc: 2.13 ug/ml

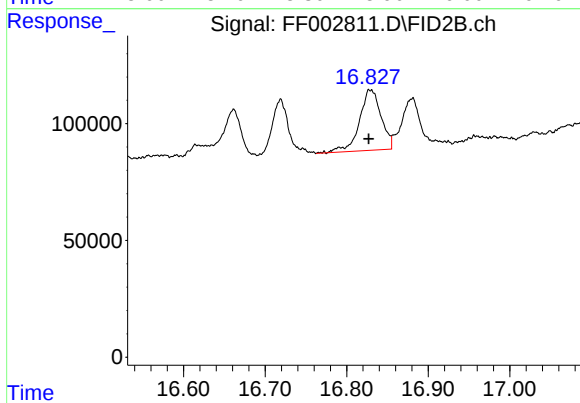

#12 N-OCTACOSANE


R.T.: 16.828 min
Delta R.T.: 0.001 min
Response: 479154
Conc: 5.02 ug/ml

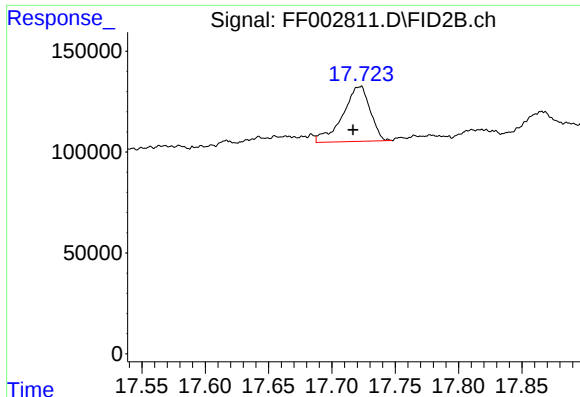

#13 N-TRIACONTANE


R.T.: 17.722 min
Delta R.T.: 0.005 min
Response: 409515
Conc: 4.13 ug/ml

Instrument :
FID_F
ClientSampleId :

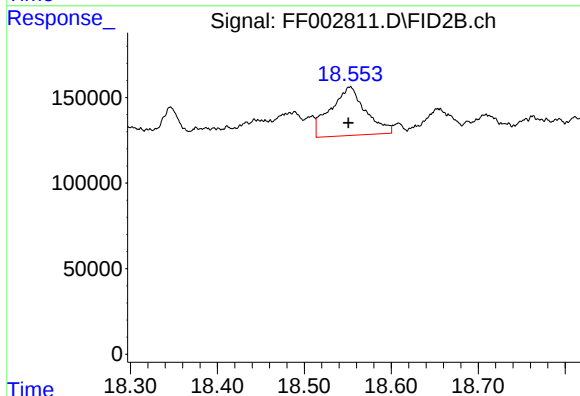


#14 N-DOTRIACONTANE

R.T.: 18.553 min
Delta R.T.: 0.002 min
Response: 793436
Conc: 8.01 ug/ml

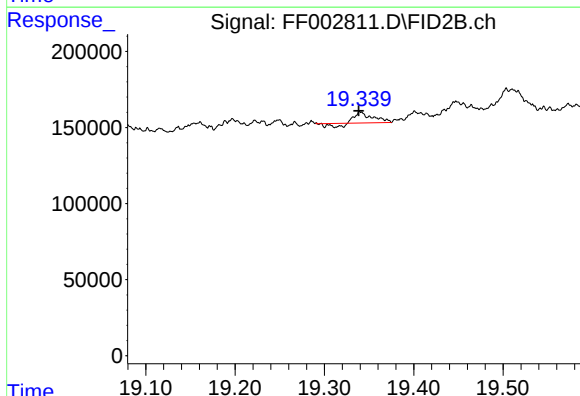


#15 N-TETRATRIACONTANE

R.T.: 19.340 min
Delta R.T.: 0.002 min
Response: 81862
Conc: 0.83 ug/ml

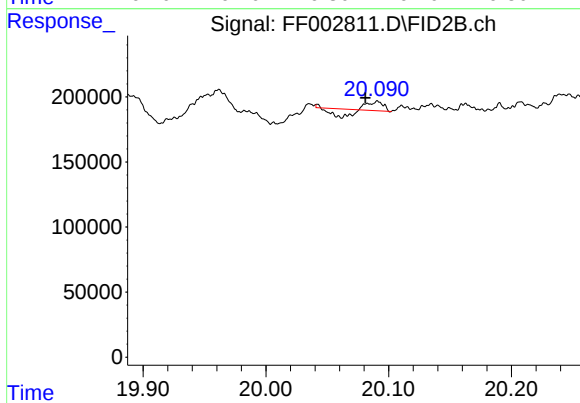

#16 N-HEXATRIACONTANE


R.T.: 20.091 min
Delta R.T.: 0.010 min
Response: 7711
Conc: 0.08 ug/ml

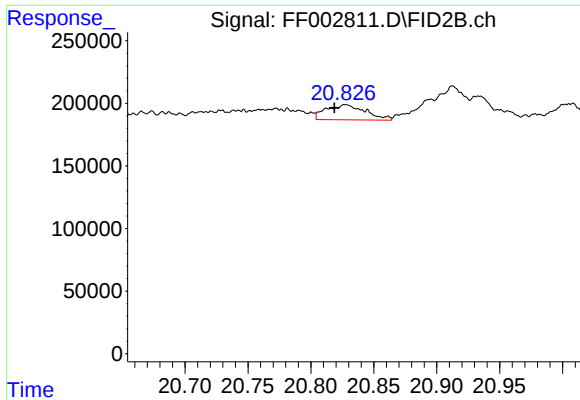

#17 N-OCTATRIACONTANE

R.T.: 20.828 min
Delta R.T.: 0.009 min
Response: 265358
Conc: 3.02 ug/ml

Instrument :
FID_F
ClientSampleId :

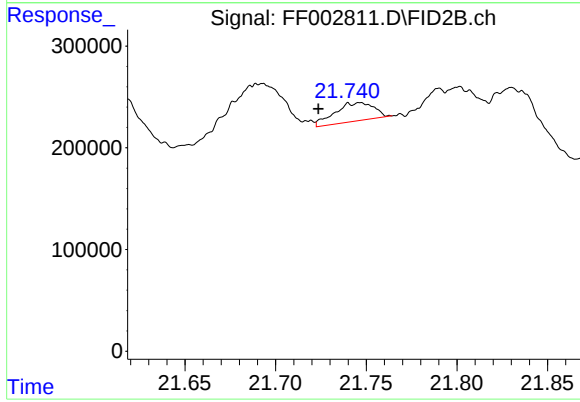

#18 N-TETRACONTANE

R.T.: 21.747 min
Delta R.T.: 0.023 min
Response: 269206
Conc: 3.07 ug/ml