

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002812.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 17:59
 Operator : AJ\SJ
 Sample : J6083-01
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:00:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.651	2044959	26.178 ug/ml
Target Compounds			
4) N-TETRADECANE	8.244f	310322	2.686 ug/ml
11) N-HEXACOSANE	15.878	108624	1.197 ug/ml
12) N-OCTACOSANE	16.831	188493	1.976 ug/ml
13) N-TRIACONTANE	17.720	190340	1.920 ug/ml
14) N-DOTRIACONTANE	18.548	391334	3.953 ug/ml
18) N-TETRACONTANE	21.724	266904	3.047 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002812.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 17:59
Operator : AJ\SJ
Sample : J6083-01
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:00:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

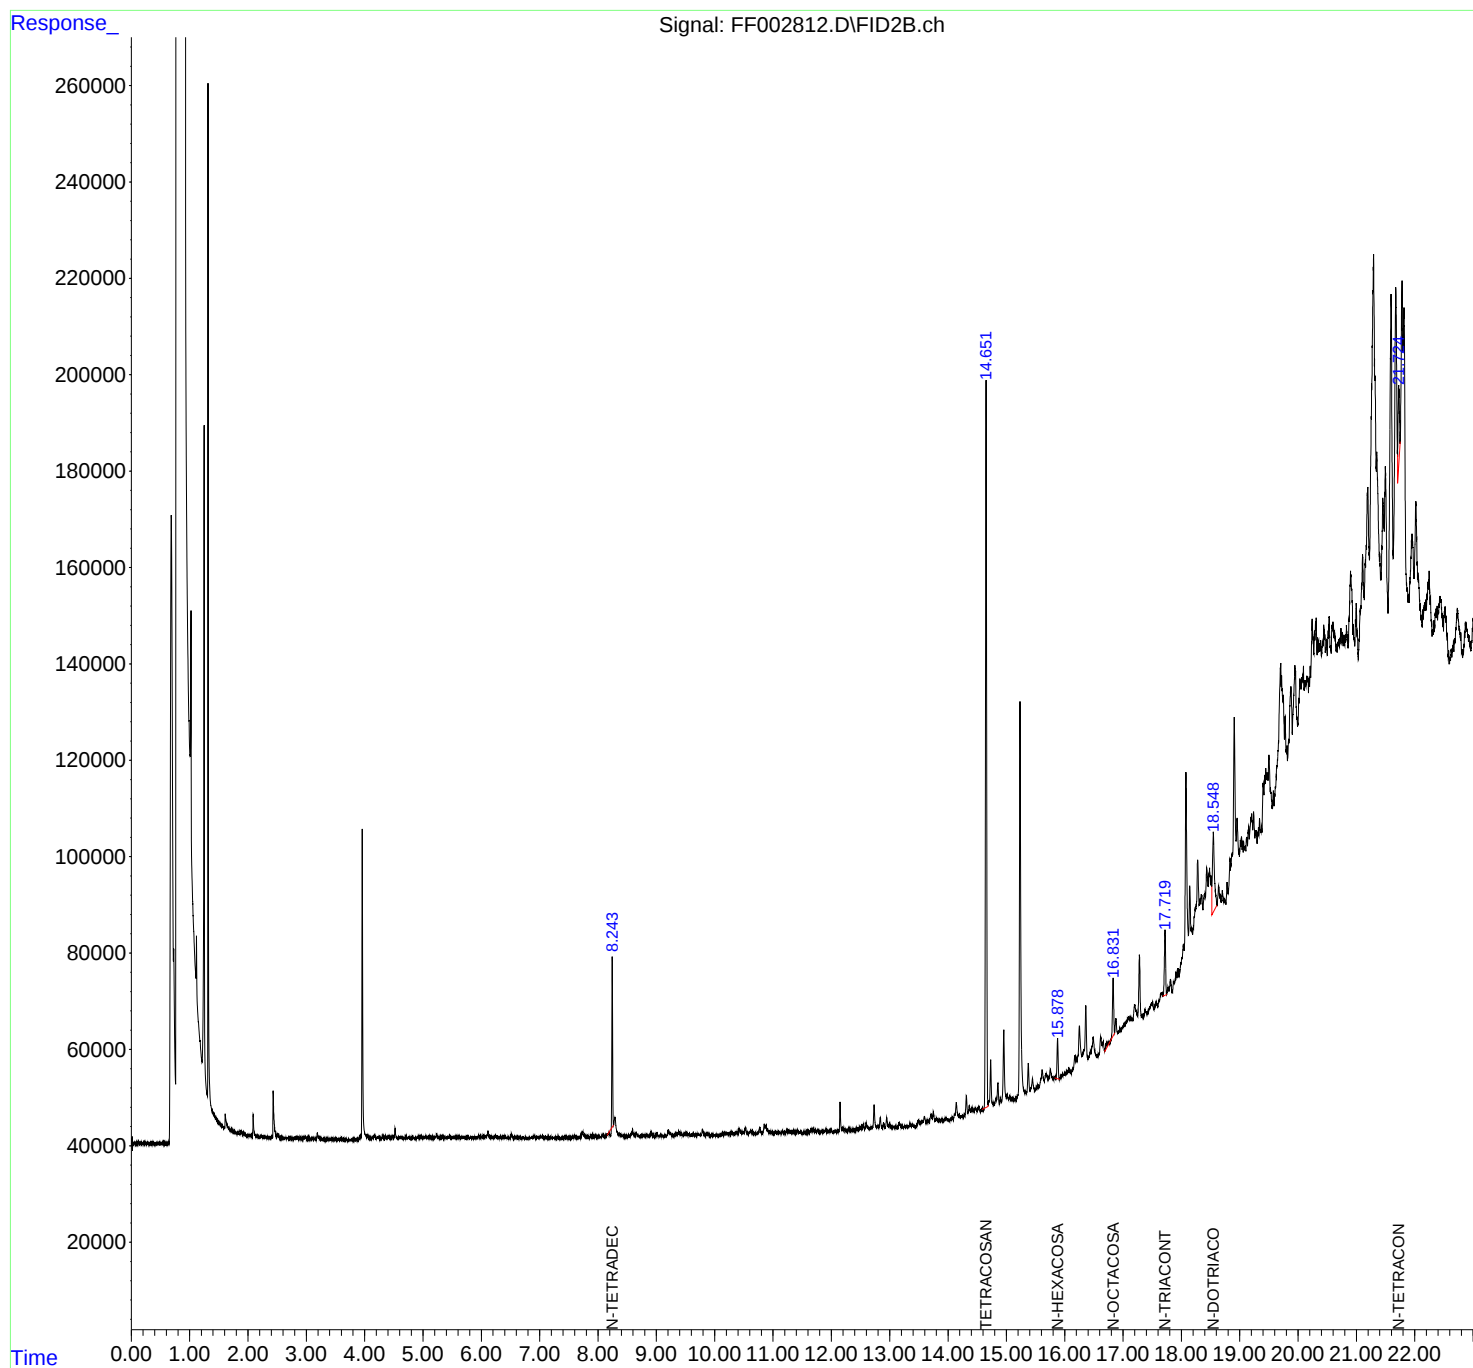


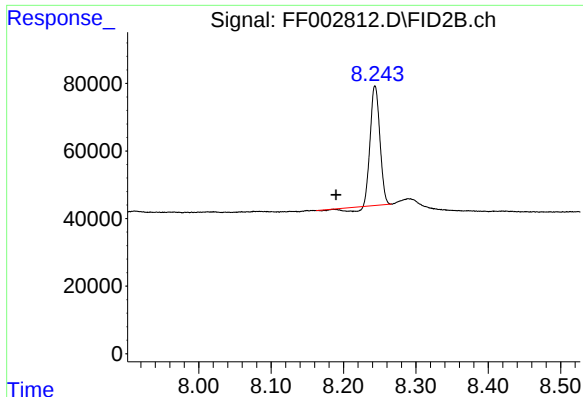

#4 N-TETRADECANE


R.T.: 8.244 min
Delta R.T.: 0.054 min
Response: 310322
Conc: 2.69 ug/ml

Instrument :
FID_F
ClientSampleId :

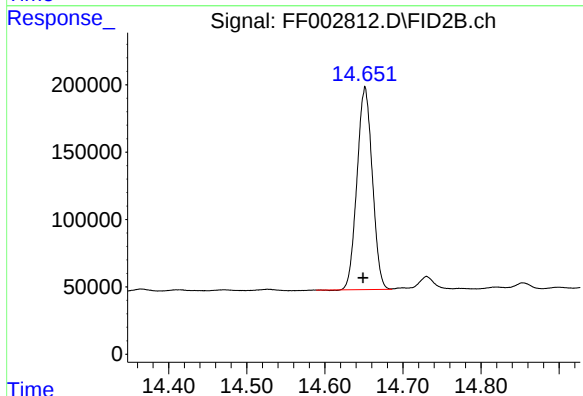


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.651 min
Delta R.T.: 0.003 min
Response: 2044959
Conc: 26.18 ug/ml

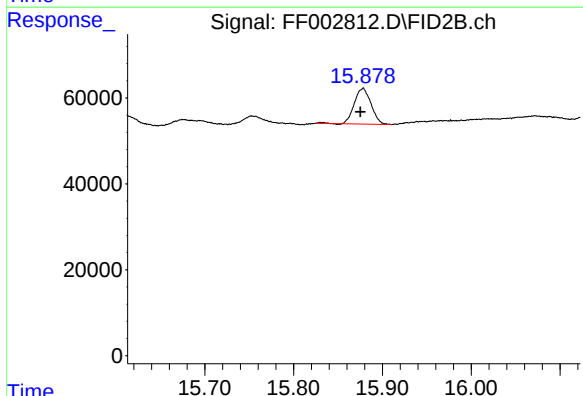


#11 N-HEXACOSANE

R.T.: 15.878 min
Delta R.T.: 0.003 min
Response: 108624
Conc: 1.20 ug/ml

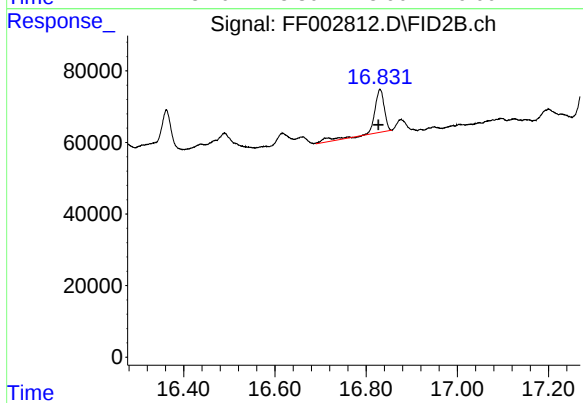

#12 N-OCTACOSANE


R.T.: 16.831 min
Delta R.T.: 0.004 min
Response: 188493
Conc: 1.98 ug/ml

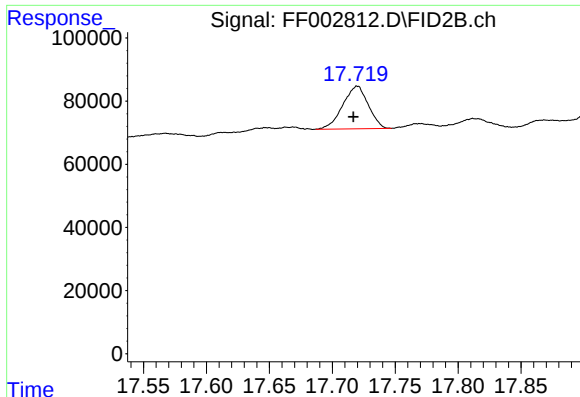

#13 N-TRIACONTANE


R.T.: 17.720 min
Delta R.T.: 0.003 min
Response: 190340
Conc: 1.92 ug/ml

Instrument :
FID_F
ClientSampleId :

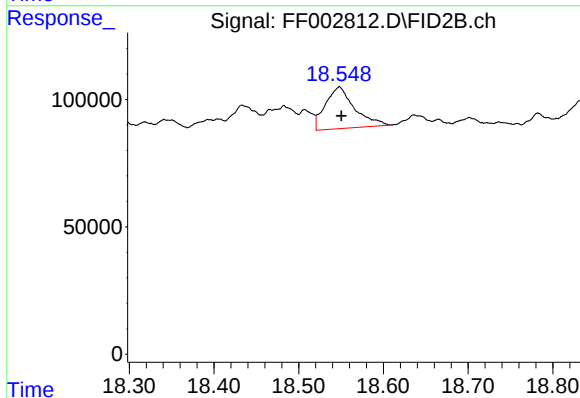

#14 N-DOTRIACONTANE

R.T.: 18.548 min
Delta R.T.: -0.003 min
Response: 391334
Conc: 3.95 ug/ml

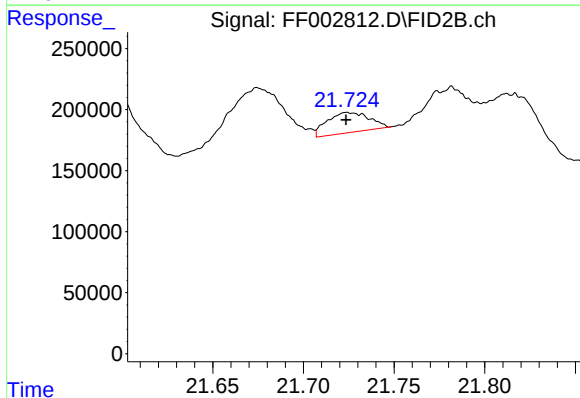

#18 N-TETRACONTANE

R.T.: 21.724 min
Delta R.T.: 0.000 min
Response: 266904
Conc: 3.05 ug/ml