

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002815.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 19:31
 Operator : AJ\SJ
 Sample : J6083-03
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:00:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.651	1696603	21.719 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243f	275031	2.381 ug/ml
10) N-TETRACOSANE	14.854	106283	1.193 ug/ml
11) N-HEXACOSANE	15.878	194706	2.145 ug/ml
12) N-OCTACOSANE	16.829	262910	2.756 ug/ml
13) N-TRIACONTANE	17.718	327704	3.306 ug/ml
14) N-DOTRIACONTANE	18.555	325485	3.288 ug/ml
15) N-TETRATRIACONTANE	19.339	76742	0.778 ug/ml
16) N-HEXATRIACONTANE	20.083	36849	0.387 ug/ml
17) N-OCTATRIACONTANE	20.824	294189	3.347 ug/ml
18) N-TETRACONTANE	21.743	1438949	16.427 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002815.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 19:31
Operator : AJ\SJ
Sample : J6083-03
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 29 01:00:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

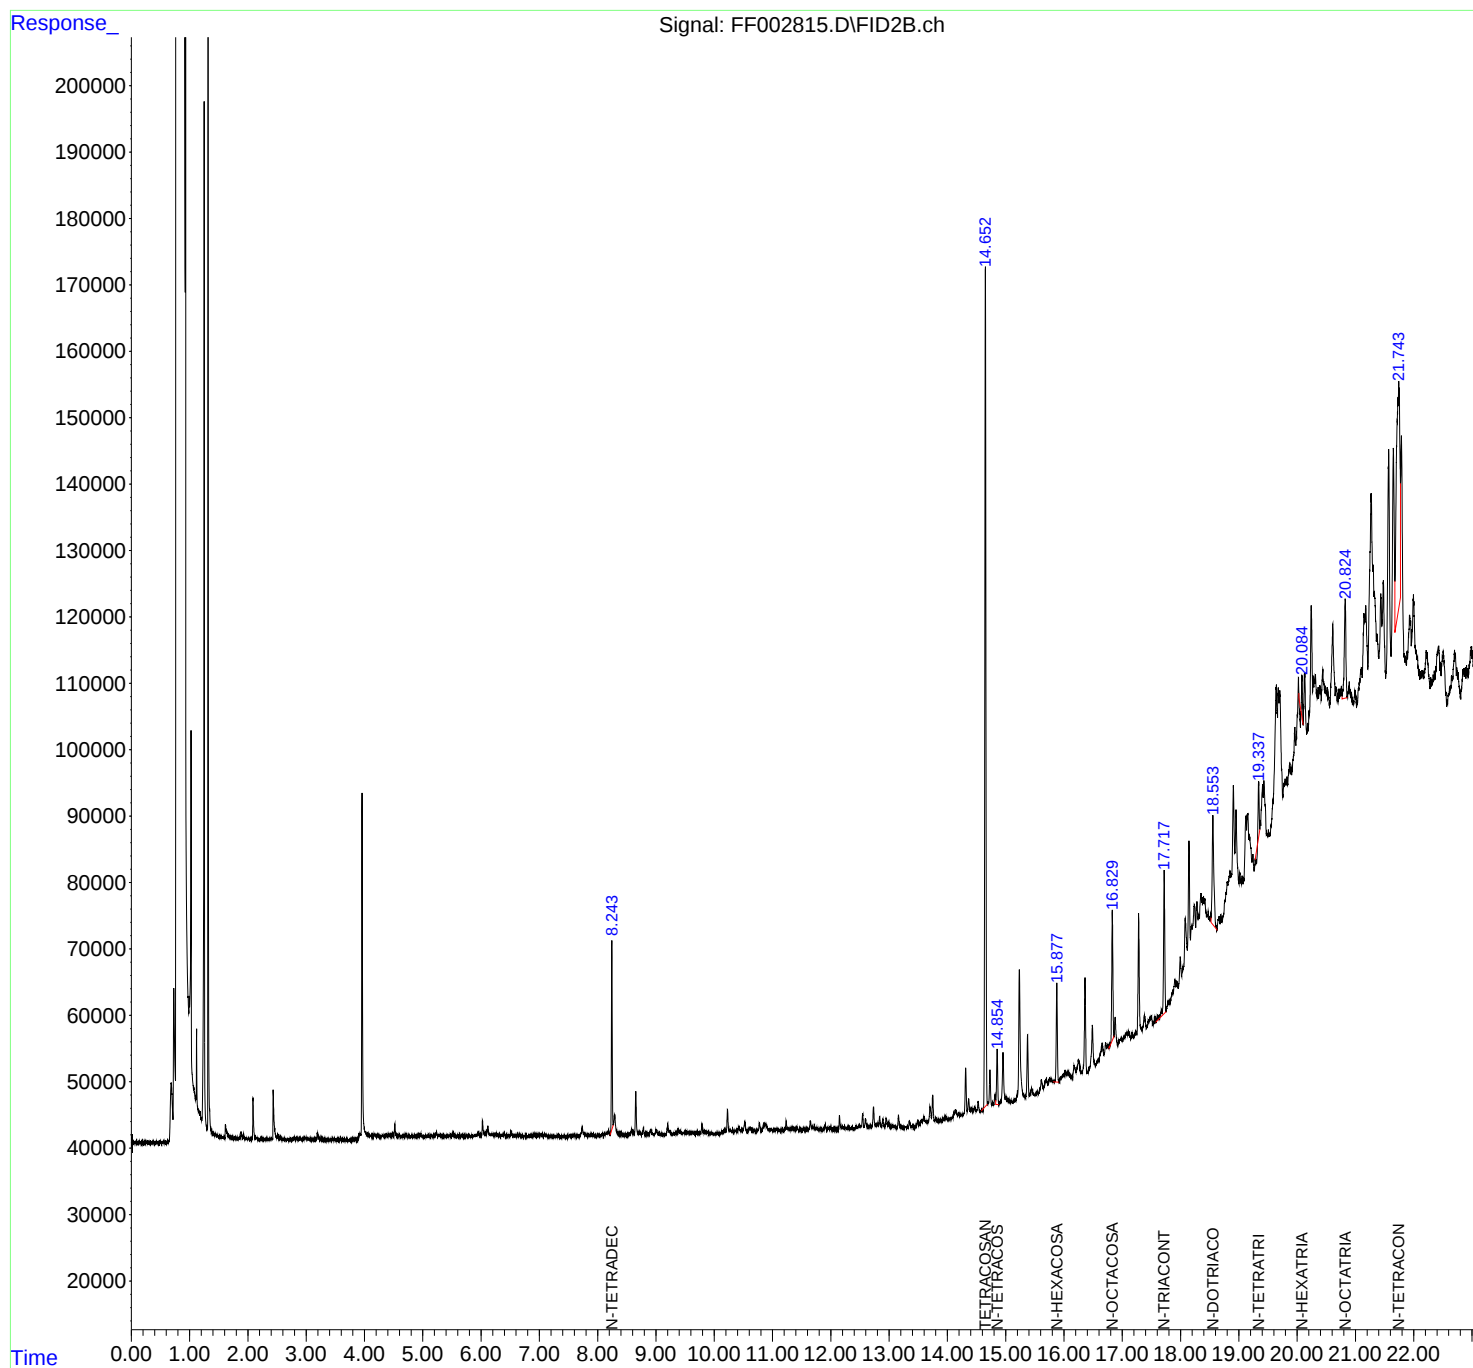


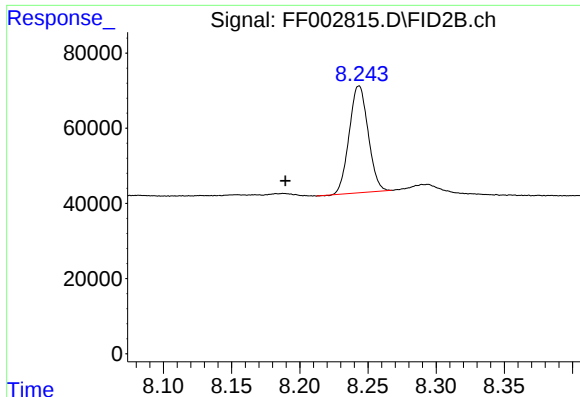

#4 N-TETRADECANE


R.T.: 8.243 min
Delta R.T.: 0.054 min
Response: 275031
Conc: 2.38 ug/ml

Instrument :
FID_F
ClientSampleId :

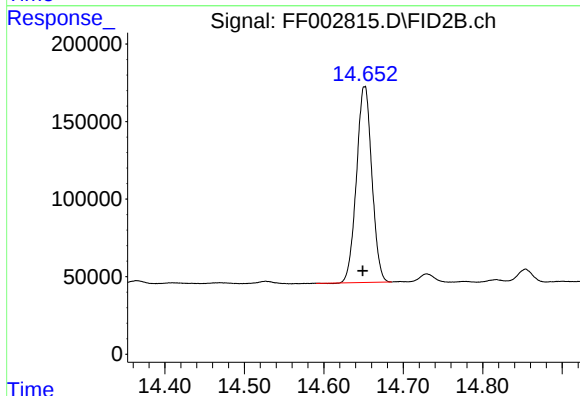


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.651 min
Delta R.T.: 0.003 min
Response: 1696603
Conc: 21.72 ug/ml

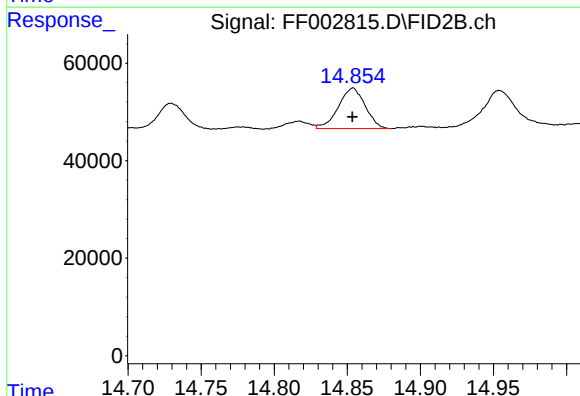


#10 N-TETRACOSANE

R.T.: 14.854 min
Delta R.T.: 0.000 min
Response: 106283
Conc: 1.19 ug/ml

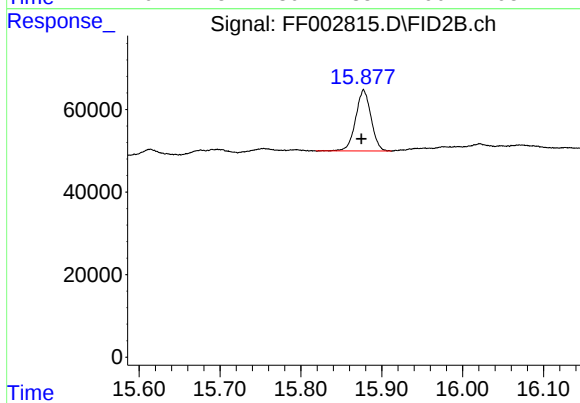

#11 N-HEXACOSANE


R.T.: 15.878 min
Delta R.T.: 0.003 min
Response: 194706
Conc: 2.15 ug/ml

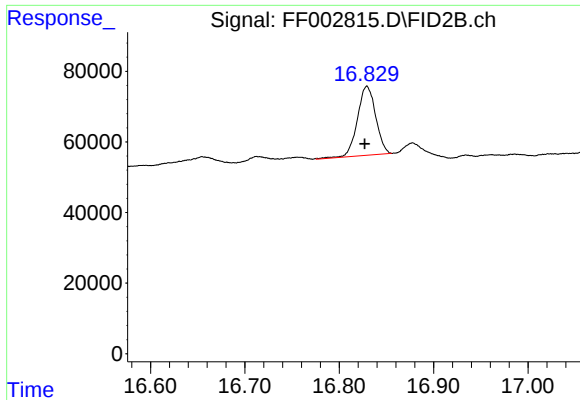

#12 N-OCTACOSANE


R.T.: 16.829 min
Delta R.T.: 0.002 min
Response: 262910
Conc: 2.76 ug/ml

Instrument :
FID_F
ClientSampleId :

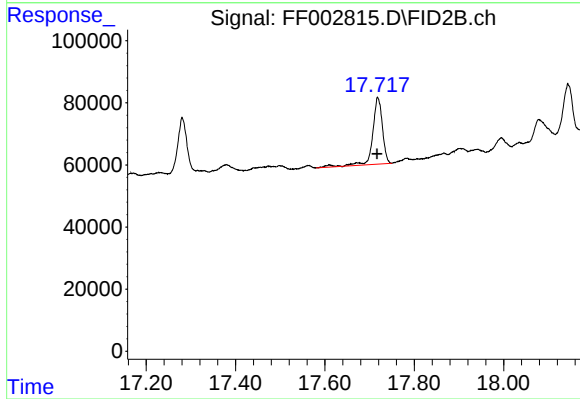


#13 N-TRIACONTANE

R.T.: 17.718 min
Delta R.T.: 0.002 min
Response: 327704
Conc: 3.31 ug/ml

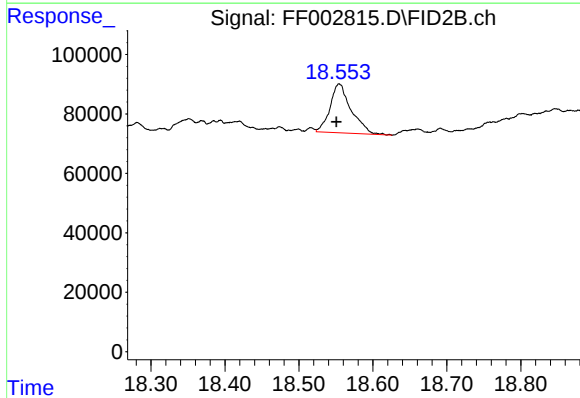


#14 N-DOTRIACONTANE

R.T.: 18.555 min
Delta R.T.: 0.004 min
Response: 325485
Conc: 3.29 ug/ml

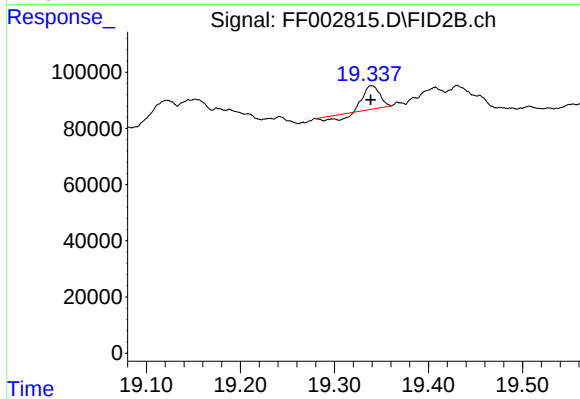

#15 N-TETRATRIACONTANE


R.T.: 19.339 min
Delta R.T.: 0.000 min
Response: 76742
Conc: 0.78 ug/ml

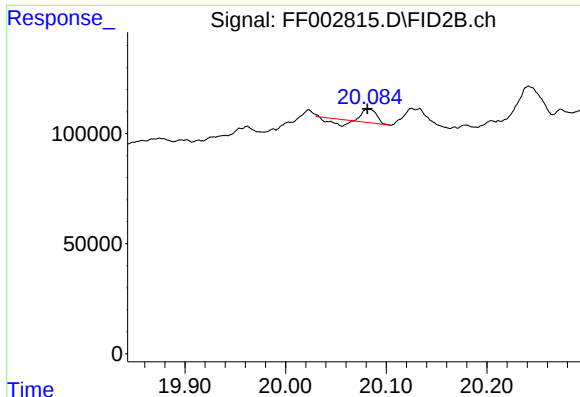

#16 N-HEXATRIACONTANE


R.T.: 20.083 min
Delta R.T.: 0.002 min
Response: 36849
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :

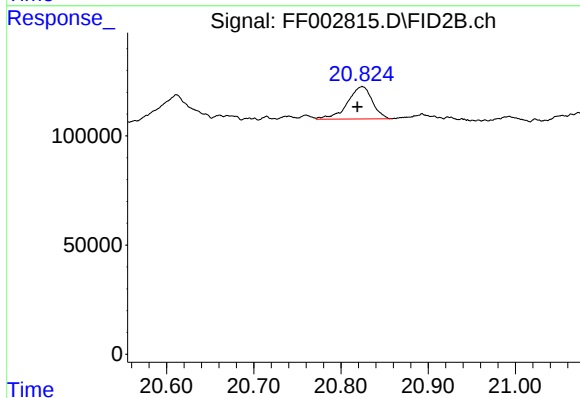

#17 N-OCTATRIACONTANE

R.T.: 20.824 min
Delta R.T.: 0.006 min
Response: 294189
Conc: 3.35 ug/ml

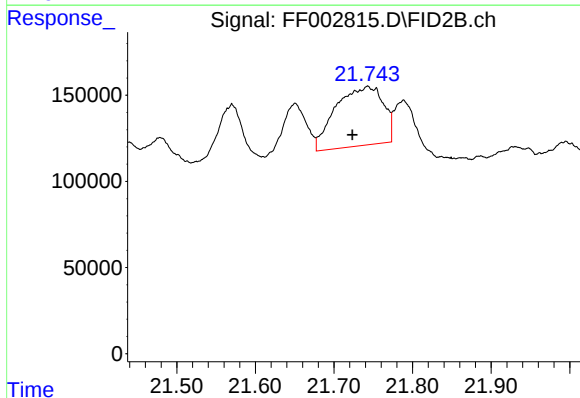

#18 N-TETRACONTANE

R.T.: 21.743 min
Delta R.T.: 0.019 min
Response: 1438949
Conc: 16.43 ug/ml