

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002816.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 20:01
 Operator : AJ\SJ
 Sample : J6083-05
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:01:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.651	820632	10.505 ug/ml
Target Compounds			
4) N-TETRADECANE	8.244f	109281	0.946 ug/ml
12) N-OCTACOSANE	16.830	141770	1.486 ug/ml
13) N-TRIACONTANE	17.720	159490	1.609 ug/ml
14) N-DOTRIACONTANE	18.554	246088	2.486 ug/ml
15) N-TETRATRIACONTANE	19.351	42071	0.426 ug/ml
16) N-HEXATRIACONTANE	20.025f	37675	0.395 ug/ml
18) N-TETRACONTANE	21.751	555358	6.340 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002816.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 20:01
Operator : AJ\SJ
Sample : J6083-05
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:01:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

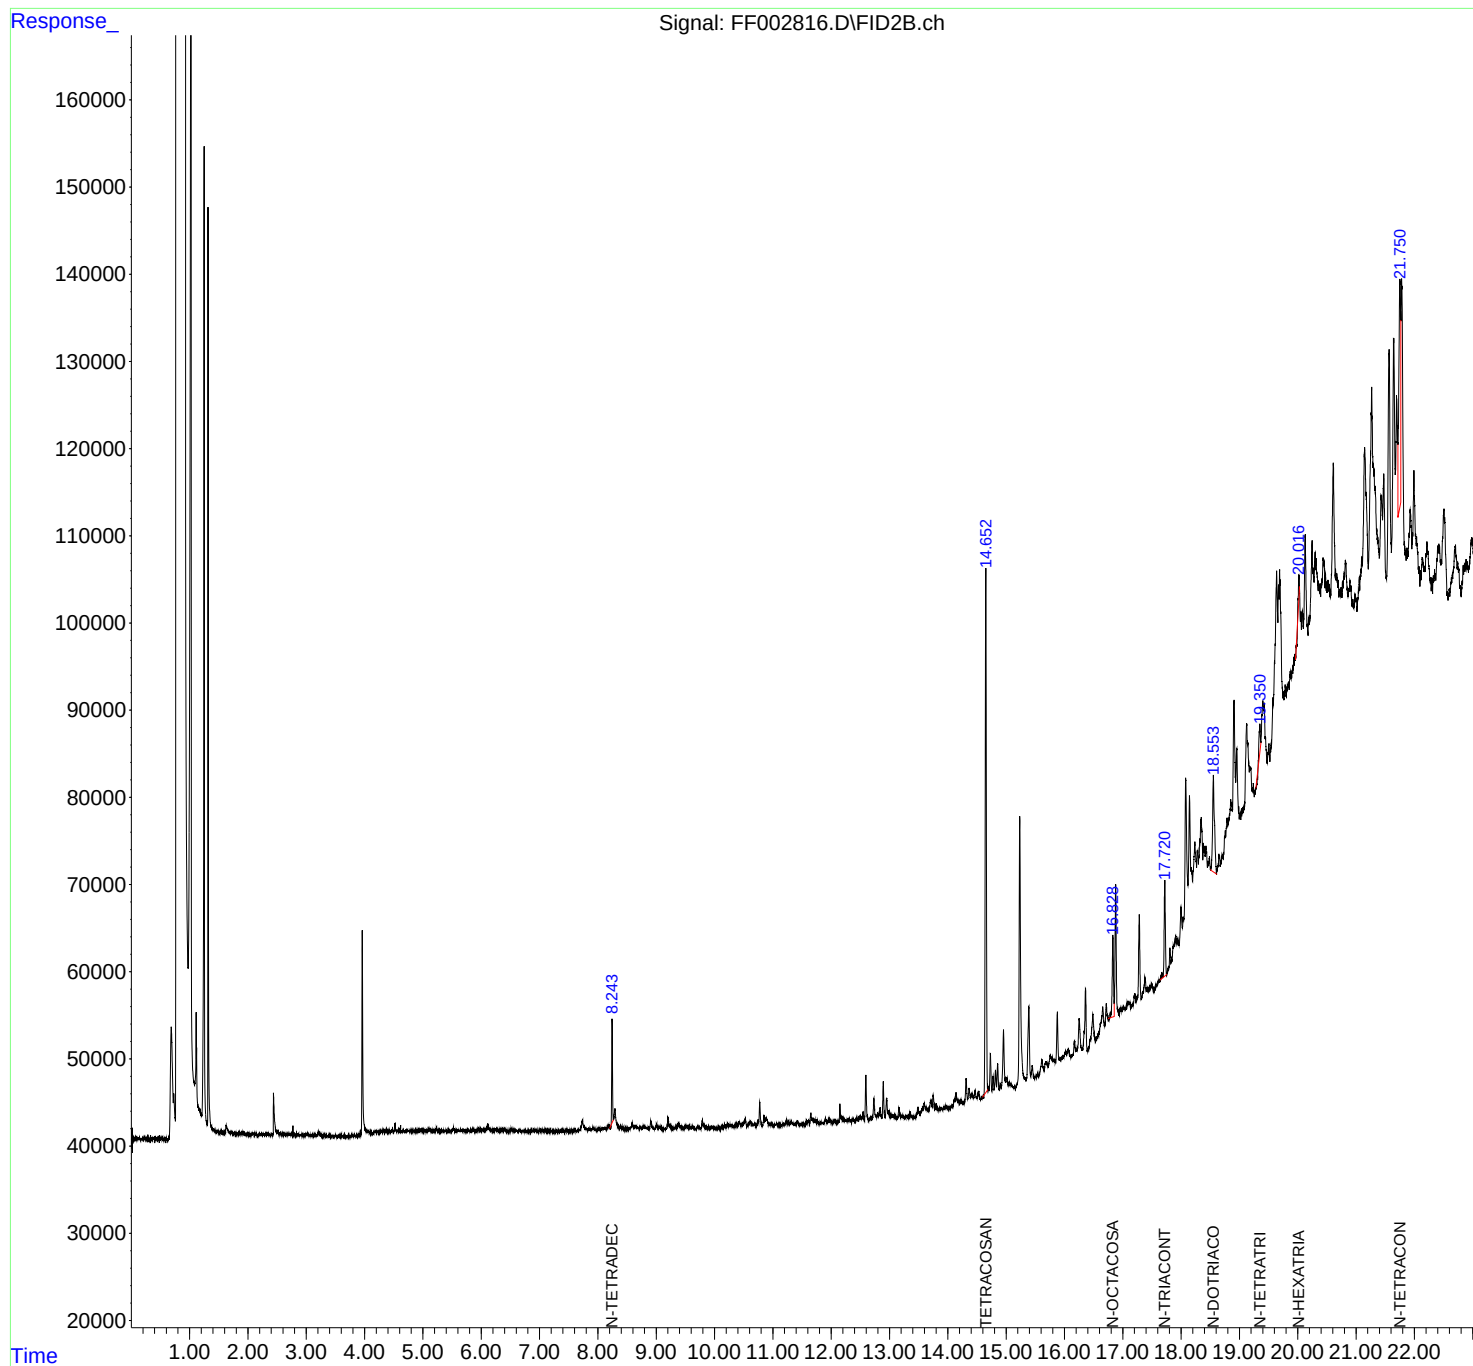


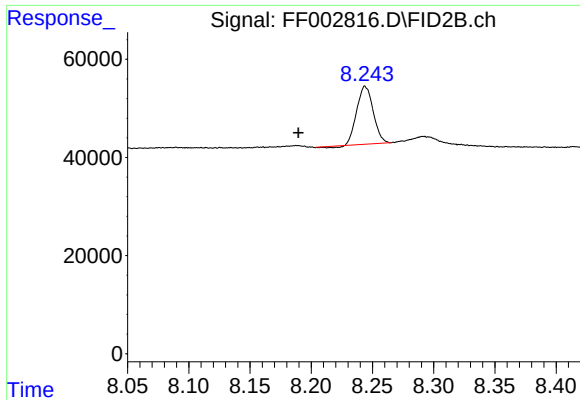

#4 N-TETRADECANE


R.T.: 8.244 min
Delta R.T.: 0.055 min
Response: 109281
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :

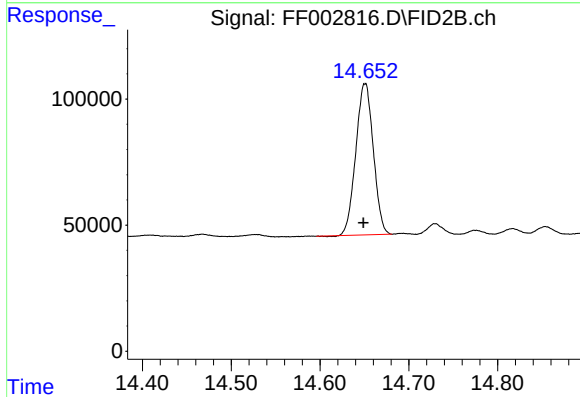


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.651 min
Delta R.T.: 0.002 min
Response: 820632
Conc: 10.51 ug/ml

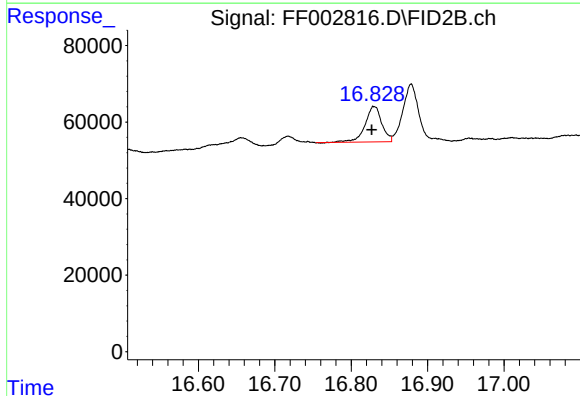


#12 N-OCTACOSANE

R.T.: 16.830 min
Delta R.T.: 0.003 min
Response: 141770
Conc: 1.49 ug/ml

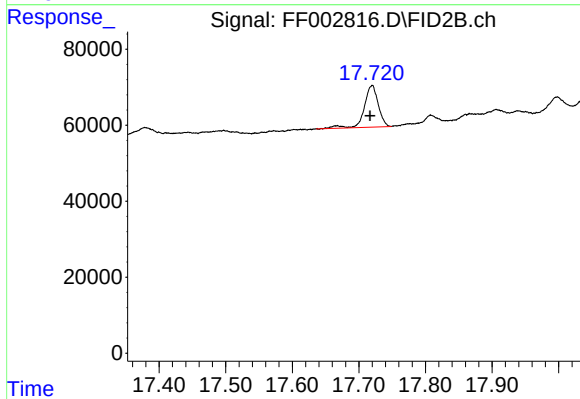

#13 N-TRIACONTANE


R.T.: 17.720 min
Delta R.T.: 0.003 min
Response: 159490
Conc: 1.61 ug/ml

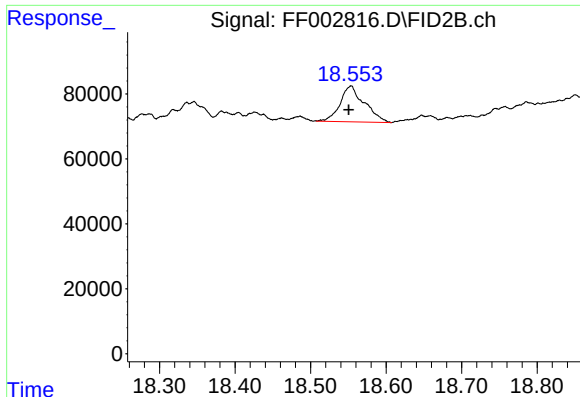

#14 N-DOTRIACONTANE


R.T.: 18.554 min
Delta R.T.: 0.003 min
Response: 246088
Conc: 2.49 ug/ml

Instrument :
FID_F
ClientSampleId :

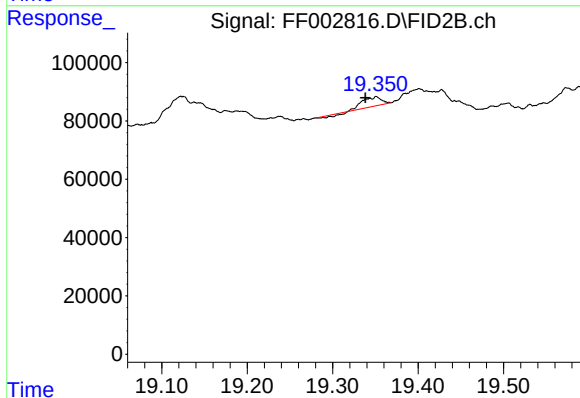


#15 N-TETRATRIACONTANE

R.T.: 19.351 min
Delta R.T.: 0.013 min
Response: 42071
Conc: 0.43 ug/ml

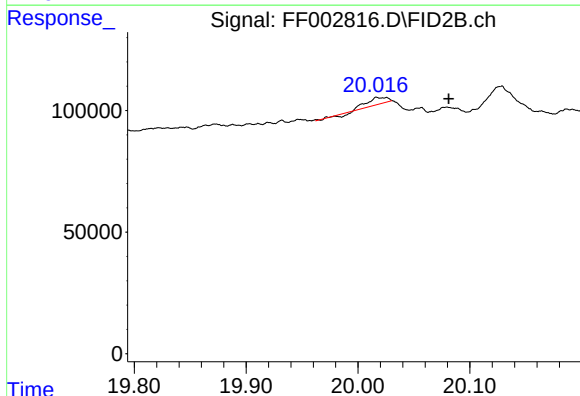

#16 N-HEXATRIACONTANE

R.T.: 20.025 min
Delta R.T.: -0.056 min
Response: 37675
Conc: 0.40 ug/ml

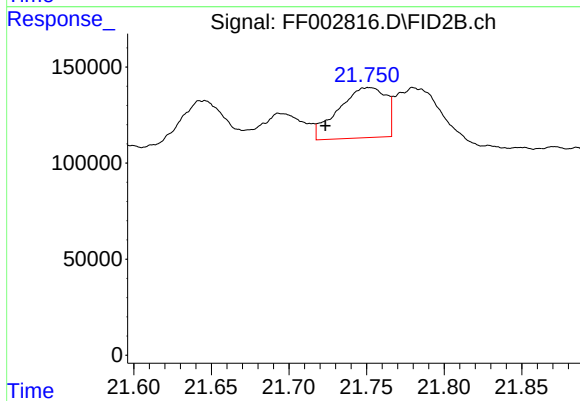

#18 N-TETRACONTANE

R.T.: 21.751 min
Delta R.T.: 0.028 min
Response: 555358
Conc: 6.34 ug/ml