

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002819.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 21:33
 Operator : AJ\SJ
 Sample : J6028-04 10X
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:01:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	140429	1.798 ug/ml
Target Compounds			
7) N-EICOSANE	12.595	235988	2.437 ug/ml
10) N-TETRACOSANE	14.817	96939	1.088 ug/ml
12) N-OCTACOSANE	16.831	151722	1.591 ug/ml
13) N-TRIACONTANE	17.716	164107	1.655 ug/ml
14) N-DOTRIACONTANE	18.545	221147	2.234 ug/ml
15) N-TETRATRIACONTANE	19.335	60628	0.614 ug/ml
16) N-HEXATRIACONTANE	20.026f	26894	0.282 ug/ml
17) N-OCTATRIACONTANE	20.825	136956	1.558 ug/ml
18) N-TETRACONTANE	21.731	441510	5.040 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002819.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 21:33
Operator : AJ\SJ
Sample : J6028-04 10X
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:01:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

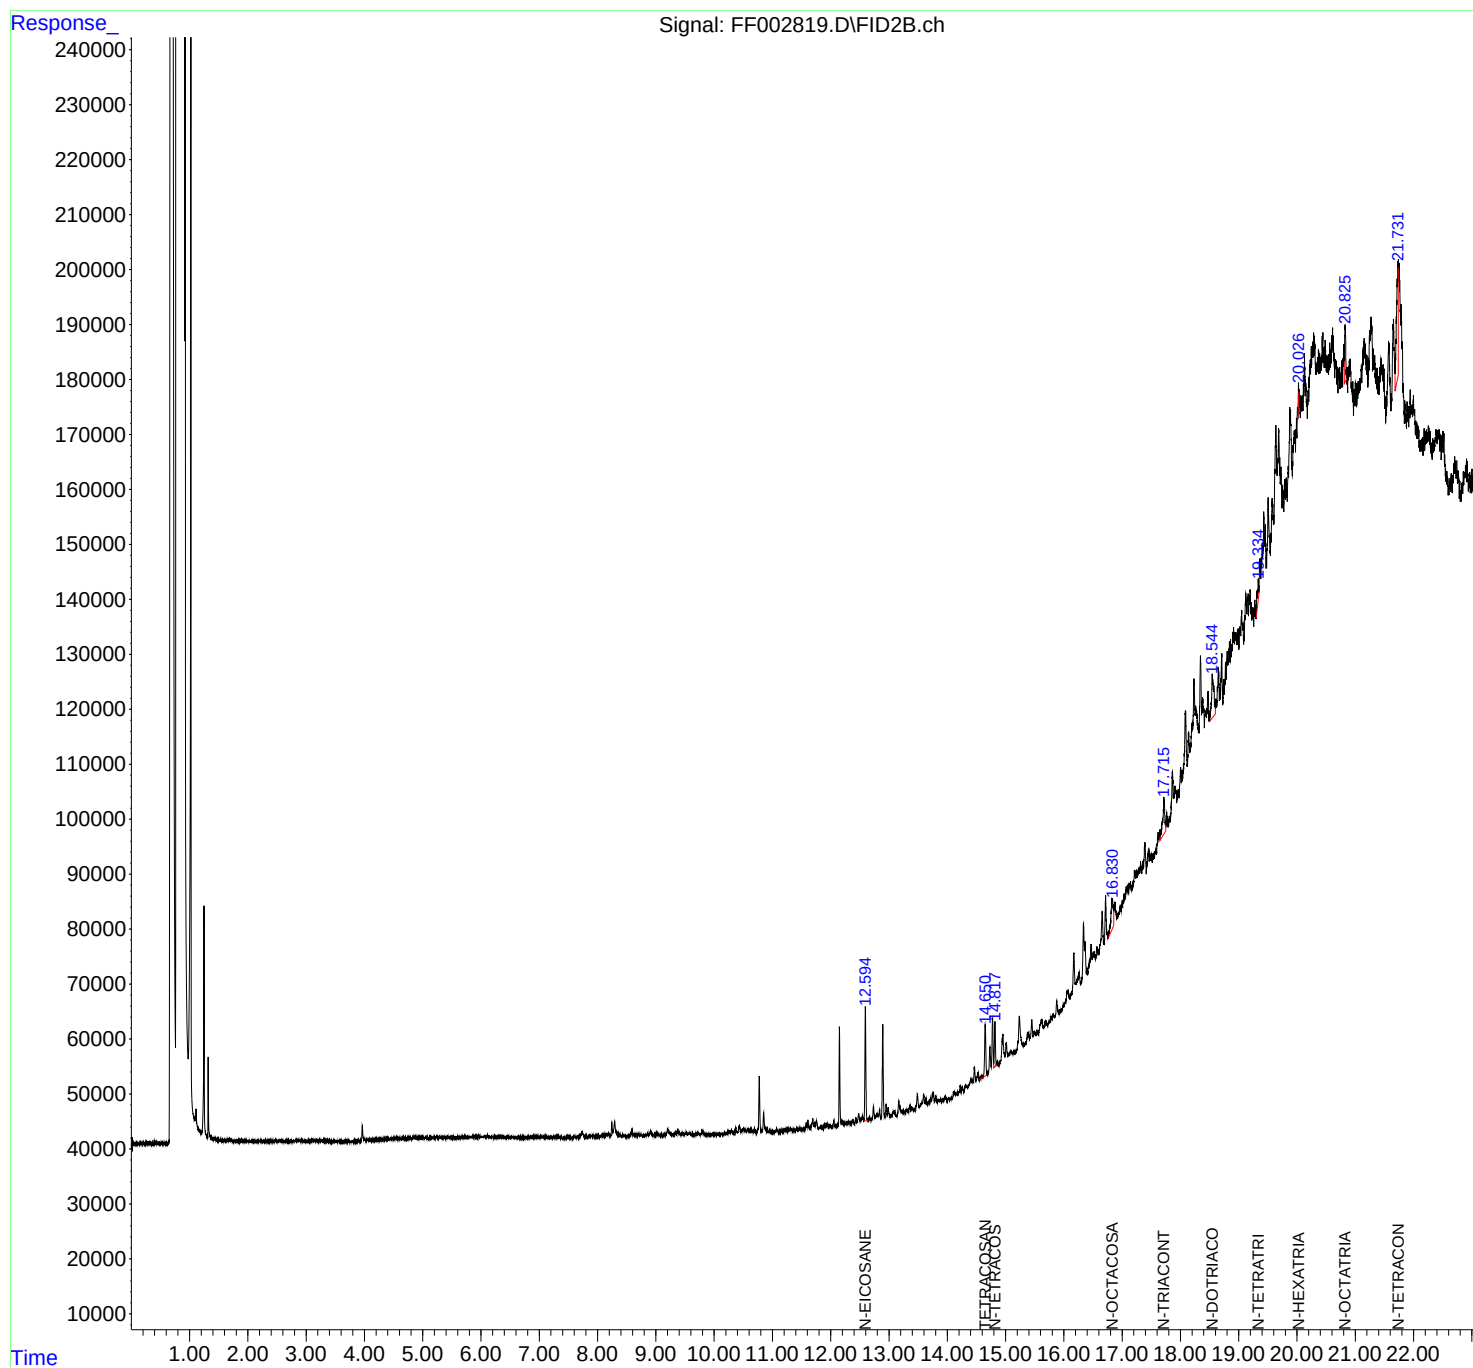


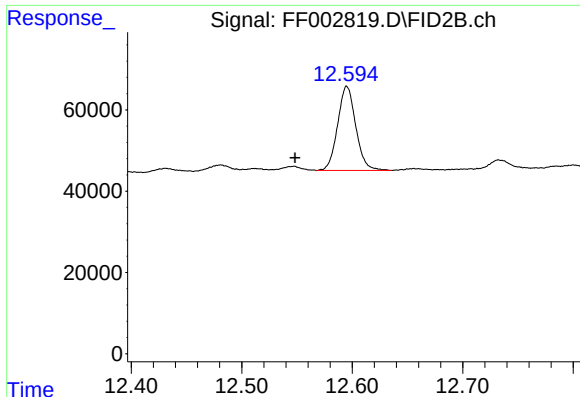

#7 N-EICOSANE


R.T.: 12.595 min
Delta R.T.: 0.047 min
Response: 235988
Conc: 2.44 ug/ml

Instrument :
FID_F
ClientSampleId :

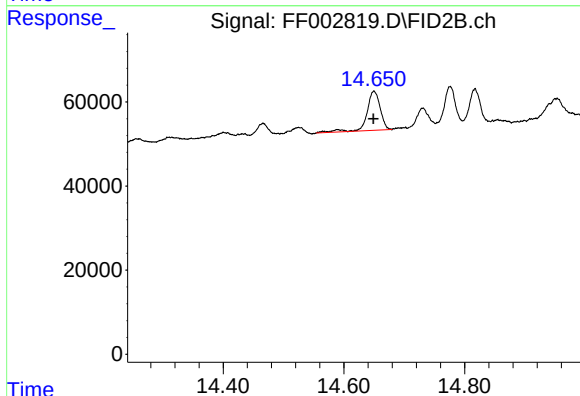


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.000 min
Response: 140429
Conc: 1.80 ug/ml

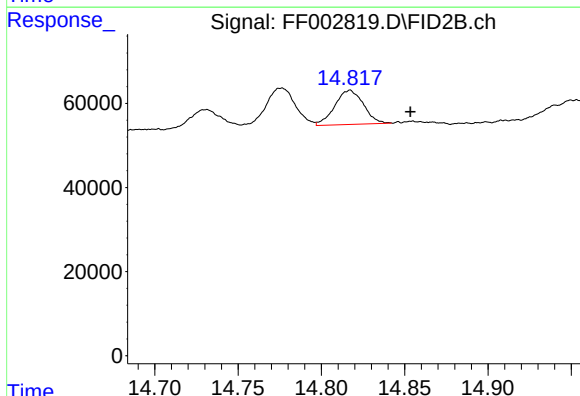


#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: -0.036 min
Response: 96939
Conc: 1.09 ug/ml

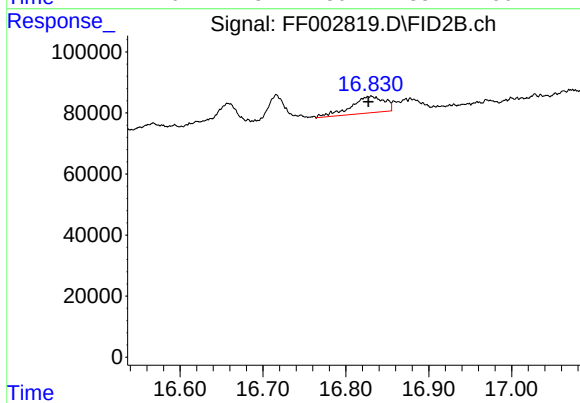

#12 N-OCTACOSANE


R.T.: 16.831 min
Delta R.T.: 0.004 min
Response: 151722
Conc: 1.59 ug/ml

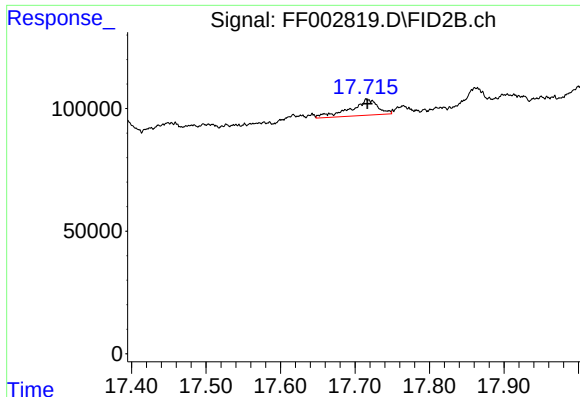

#13 N-TRIACONTANE


R.T.: 17.716 min
Delta R.T.: 0.000 min
Response: 164107
Conc: 1.66 ug/ml

Instrument :
FID_F
ClientSampleId :

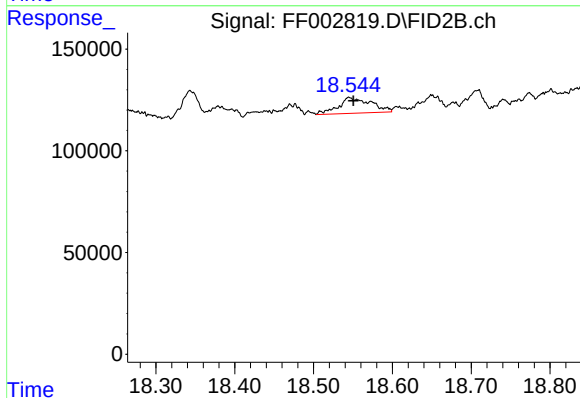


#14 N-DOTRIACONTANE

R.T.: 18.545 min
Delta R.T.: -0.006 min
Response: 221147
Conc: 2.23 ug/ml

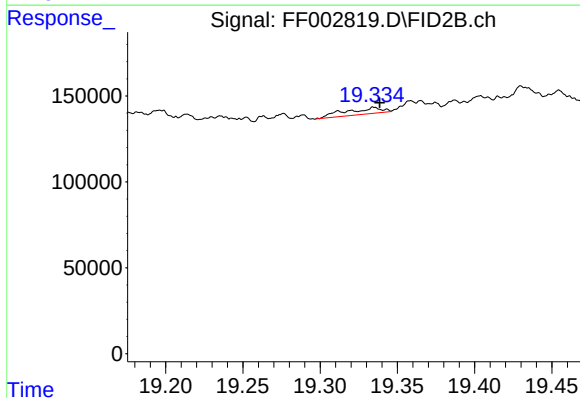


#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: -0.004 min
Response: 60628
Conc: 0.61 ug/ml

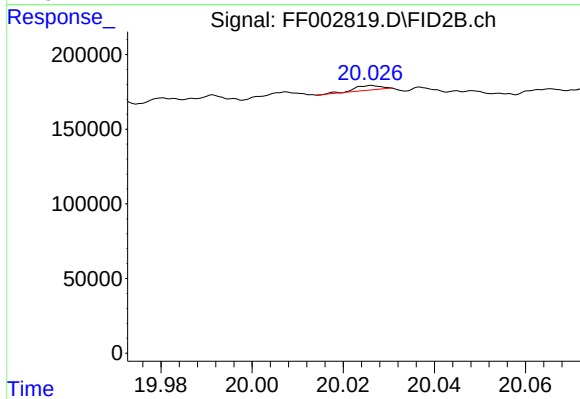

#16 N-HEXATRIACONTANE


R.T.: 20.026 min
Delta R.T.: -0.055 min
Response: 26894
Conc: 0.28 ug/ml

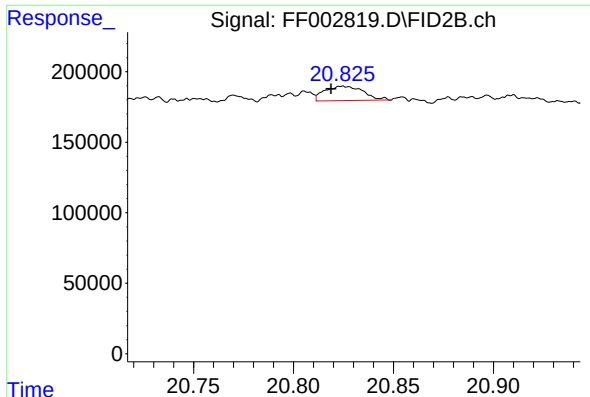

#17 N-OCTATRIACONTANE

R.T.: 20.825 min
Delta R.T.: 0.006 min
Response: 136956
Conc: 1.56 ug/ml

Instrument :
FID_F
ClientSampleId :

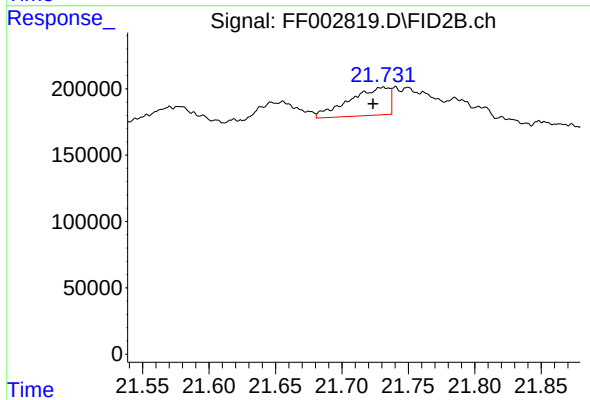

#18 N-TETRACONTANE

R.T.: 21.731 min
Delta R.T.: 0.007 min
Response: 441510
Conc: 5.04 ug/ml