

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002820.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 22:03
 Operator : AJ\SJ
 Sample : J6028-06 5X
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:01:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	392285	5.022 ug/ml
Target Compounds			
7) N-EICOSANE	12.595	428248	4.423 ug/ml
10) N-TETRACOSANE	14.817	209627	2.353 ug/ml
12) N-OCTACOSANE	16.824	203856	2.137 ug/ml
13) N-TRIACONTANE	17.718	225392	2.274 ug/ml
14) N-DOTRIACONTANE	18.551	190347	1.923 ug/ml
15) N-TETRATRIACONTANE	19.337	52050	0.527 ug/ml
16) N-HEXATRIACONTANE	20.025f	51785	0.543 ug/ml
18) N-TETRACONTANE	21.700	201976	2.306 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002820.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 22:03
Operator : AJ\SJ
Sample : J6028-06 5X
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:01:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

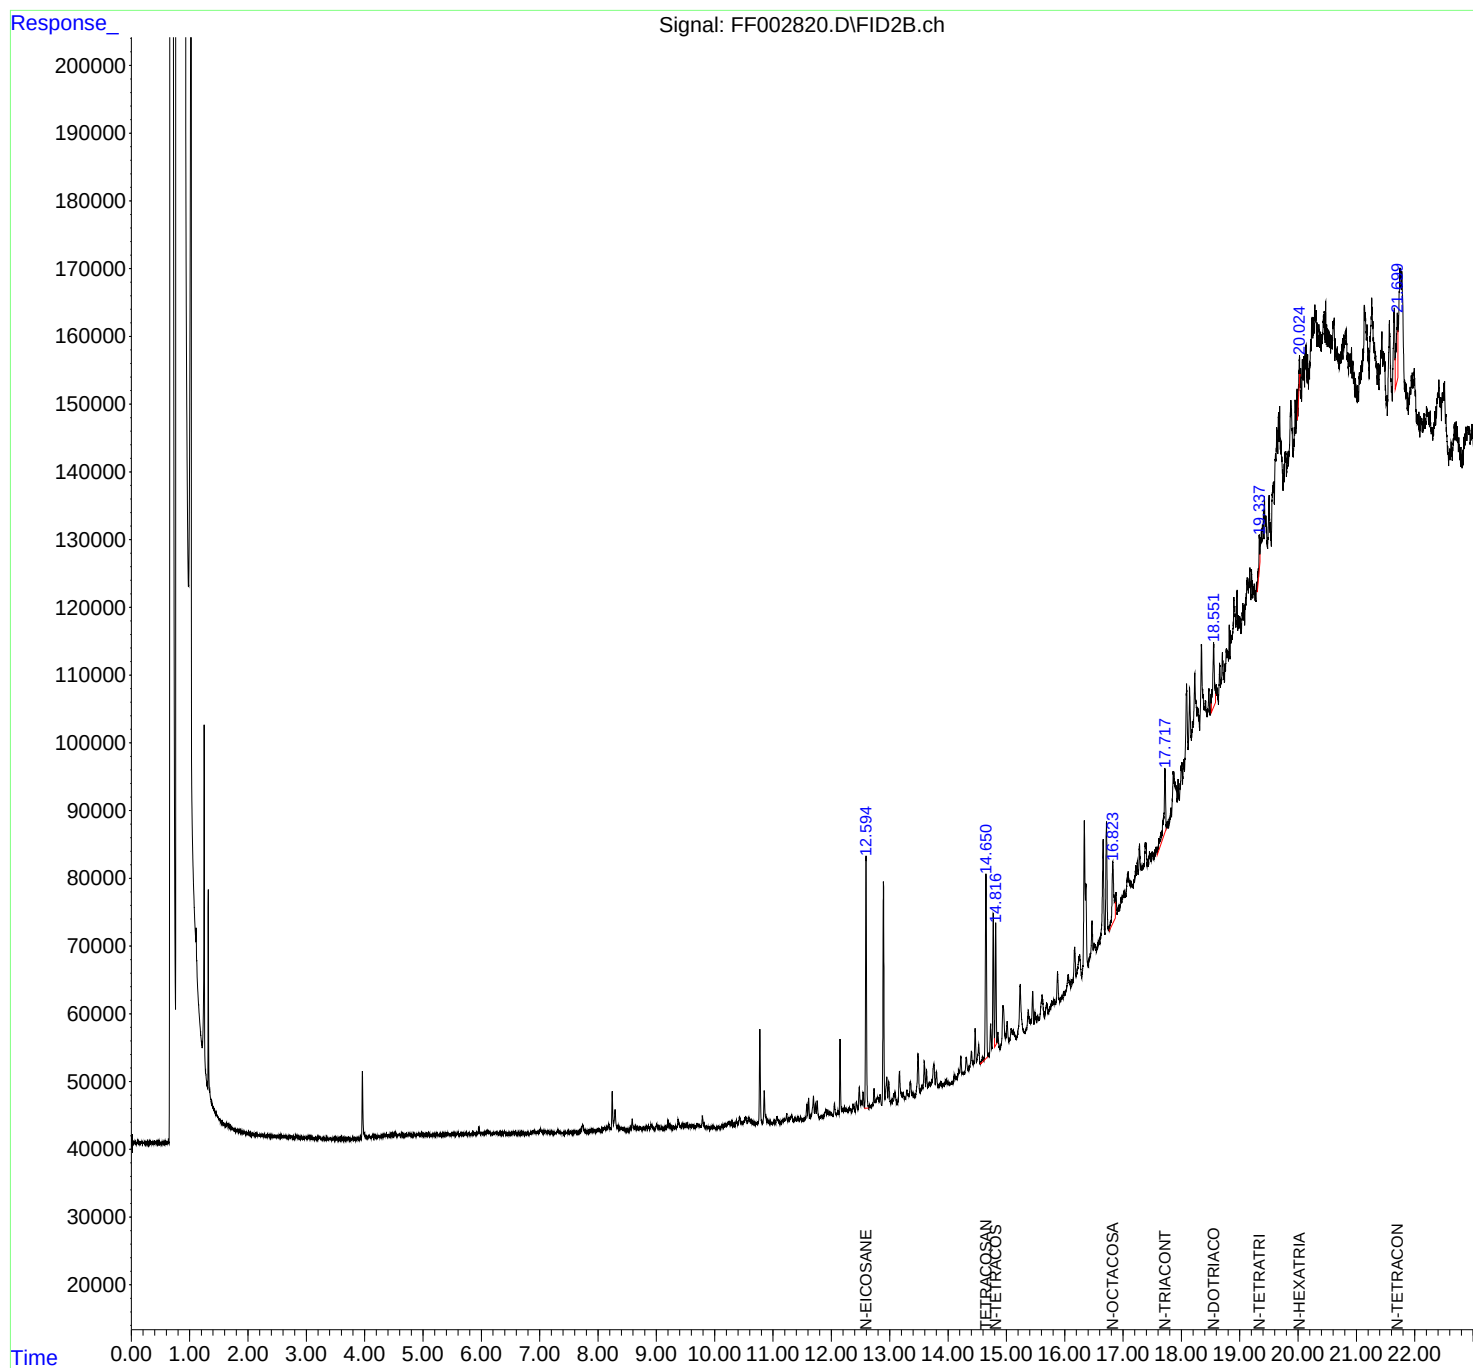


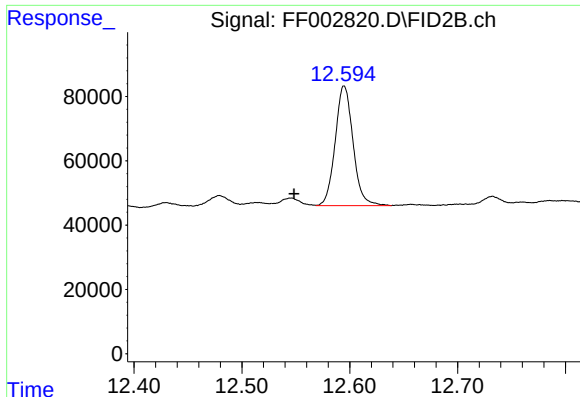

#7 N-EICOSANE


R.T.: 12.595 min
Delta R.T.: 0.046 min
Response: 428248
Conc: 4.42 ug/ml

Instrument :
FID_F
ClientSampleId :

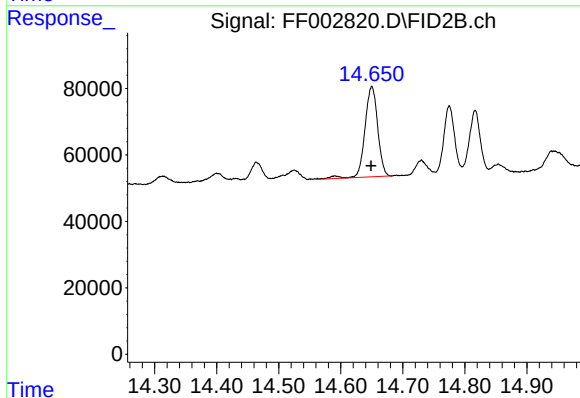


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.001 min
Response: 392285
Conc: 5.02 ug/ml

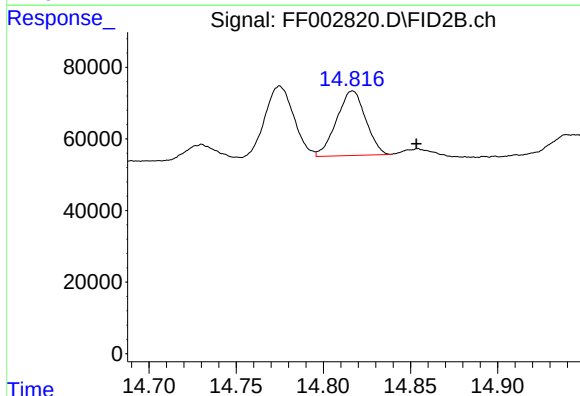


#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: -0.037 min
Response: 209627
Conc: 2.35 ug/ml

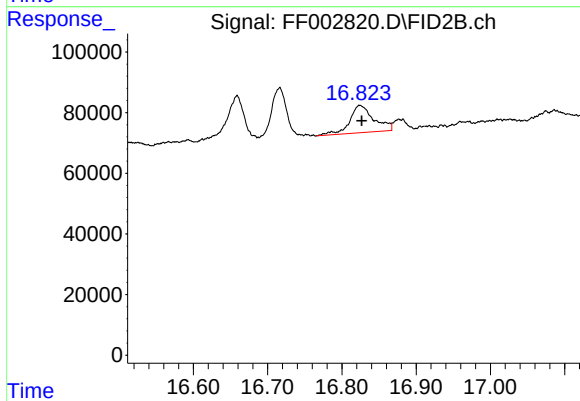

#12 N-OCTACOSANE


R.T.: 16.824 min
Delta R.T.: -0.003 min
Response: 203856
Conc: 2.14 ug/ml

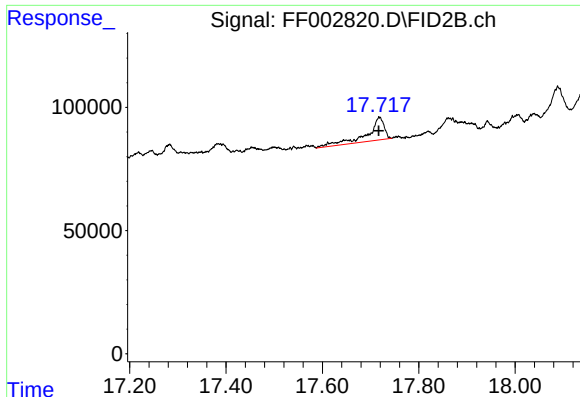

#13 N-TRIACONTANE


R.T.: 17.718 min
Delta R.T.: 0.002 min
Response: 225392
Conc: 2.27 ug/ml

Instrument :
FID_F
ClientSampleId :

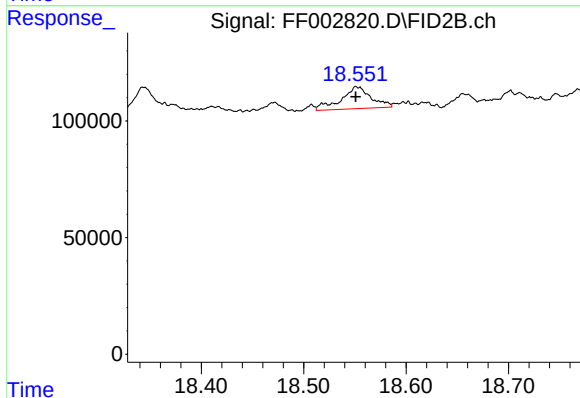


#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: 0.000 min
Response: 190347
Conc: 1.92 ug/ml

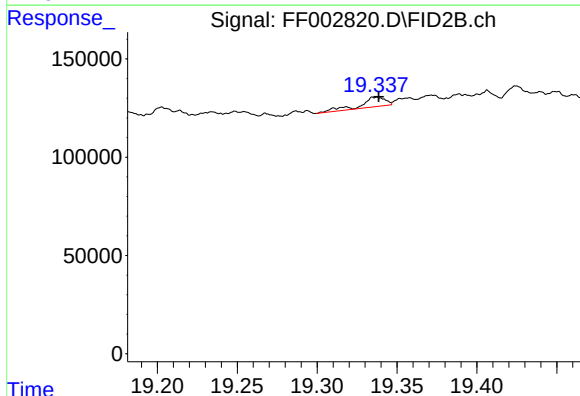


#15 N-TETRATRIACONTANE

R.T.: 19.337 min
Delta R.T.: -0.002 min
Response: 52050
Conc: 0.53 ug/ml

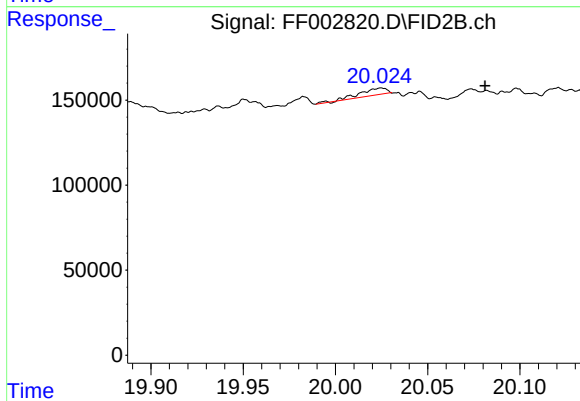

#16 N-HEXATRIACONTANE

R.T.: 20.025 min
Delta R.T.: -0.056 min
Response: 51785
Conc: 0.54 ug/ml

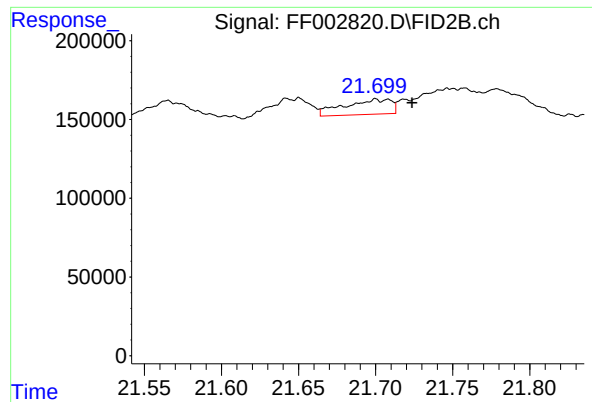

#18 N-TETRACONTANE

R.T.: 21.700 min
Delta R.T.: -0.024 min
Response: 201976
Conc: 2.31 ug/ml

Instrument :
FID_F
ClientSampleId :