

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002821.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 22:34
 Operator : AJ\SJ
 Sample : J6049-01 200X
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:01:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.649	317443	4.064 ug/ml
Target Compounds			
4) N-TETRADECANE	8.162	163253	1.413 ug/ml
5) N-HEXADECANE	9.794	276326	2.527 ug/ml
6) N-OCTADECANE	11.300f	426682	4.110 ug/ml
7) N-EICOSANE	12.546	182557	1.885 ug/ml
8) N-DOCOSANE	13.763	288775	3.154 ug/ml
10) N-TETRACOSANE	14.820	1672495	18.773 ug/ml
11) N-HEXACOSANE	15.876	264371	2.913 ug/ml
12) N-OCTACOSANE	16.820	400749	4.202 ug/ml
13) N-TRIACONTANE	17.717	95046	0.959 ug/ml
15) N-TETRATRIACONTANE	19.367	65314	0.662 ug/ml
18) N-TETRACONTANE	21.749	288151	3.290 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002821.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 22:34
Operator : AJ\SJ
Sample : J6049-01 200X
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:01:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

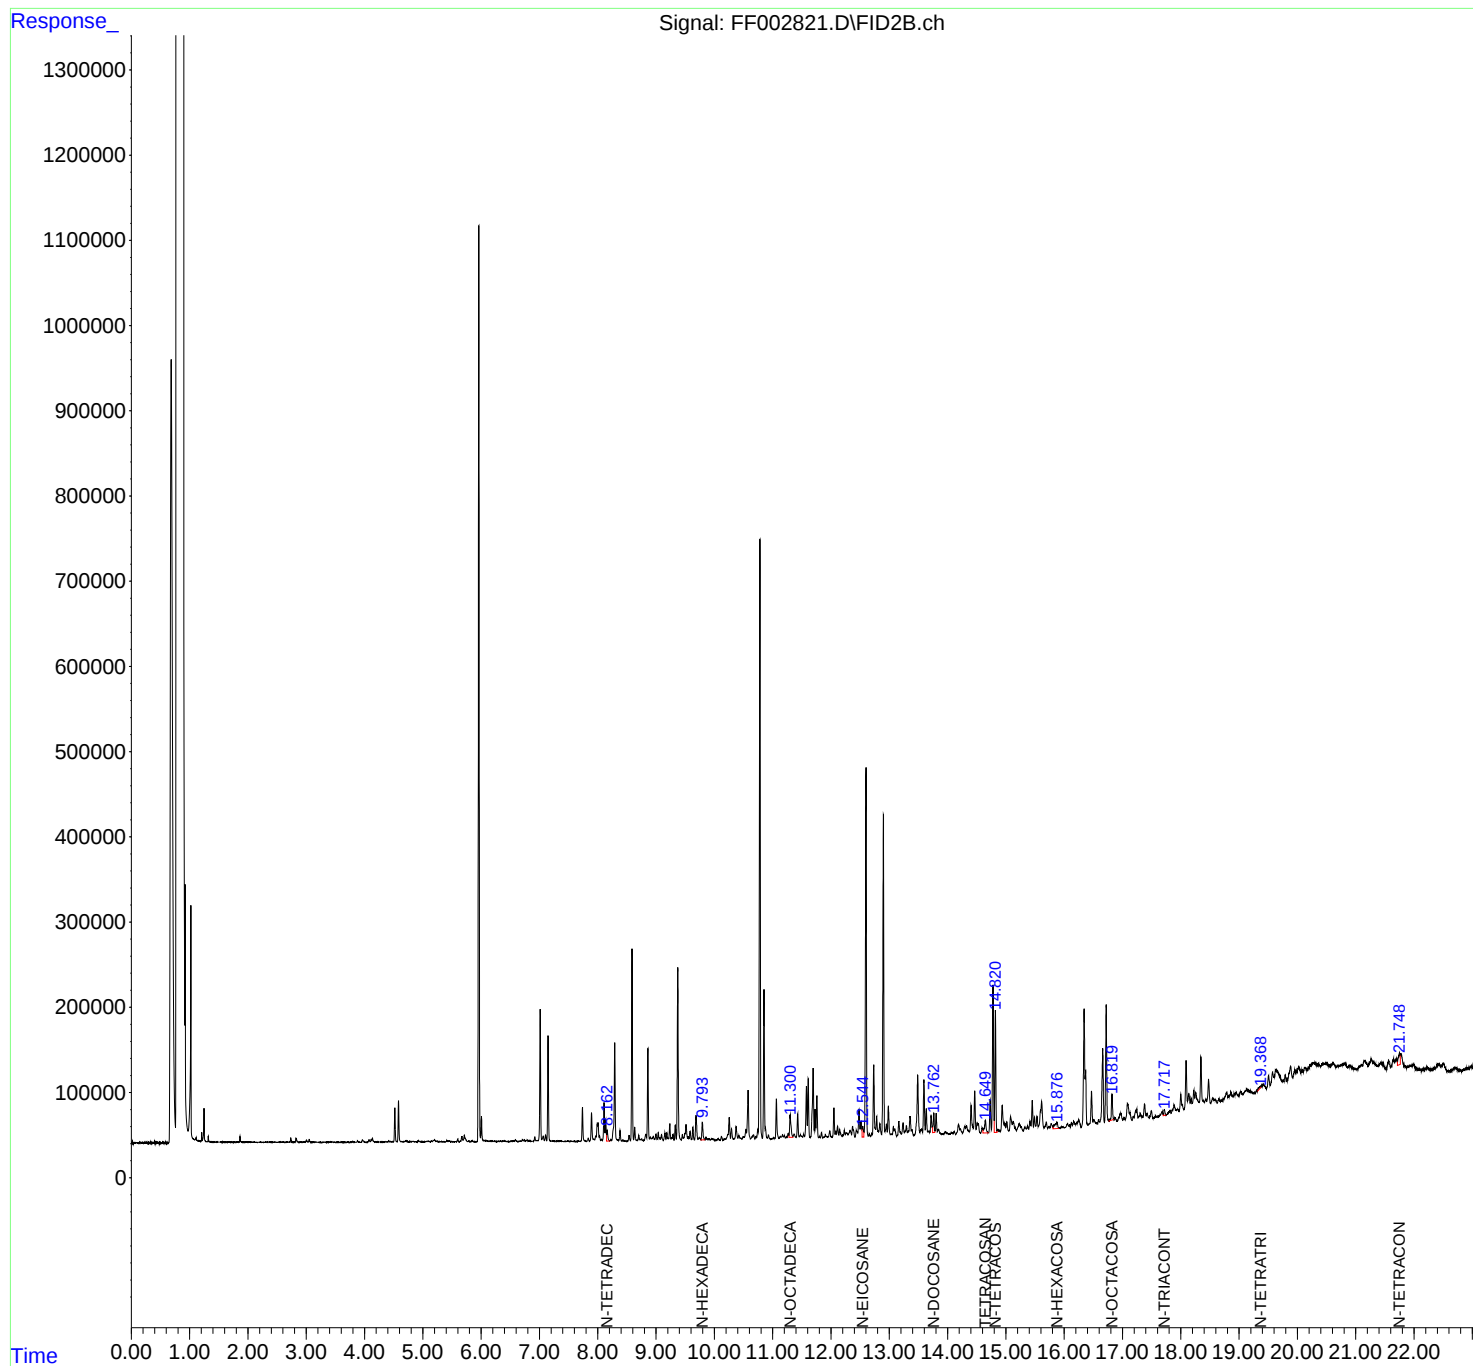


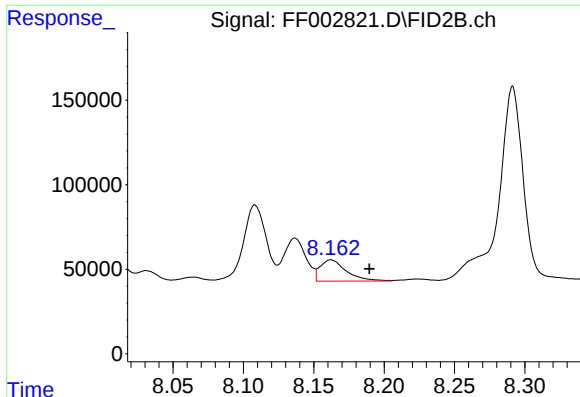

#4 N-TETRADECANE


R.T.: 8.162 min
Delta R.T.: -0.027 min
Response: 163253
Conc: 1.41 ug/ml

Instrument :
FID_F
ClientSampleId :

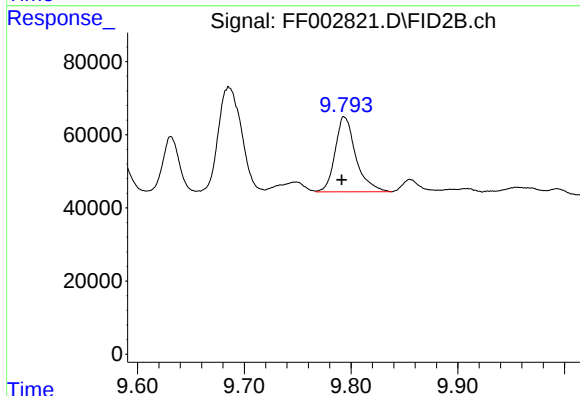


#5 N-HEXADECANE

R.T.: 9.794 min
Delta R.T.: 0.002 min
Response: 276326
Conc: 2.53 ug/ml

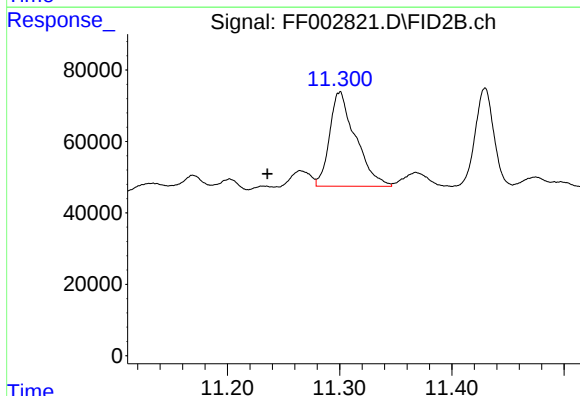


#6 N-OCTADECANE

R.T.: 11.300 min
Delta R.T.: 0.065 min
Response: 426682
Conc: 4.11 ug/ml

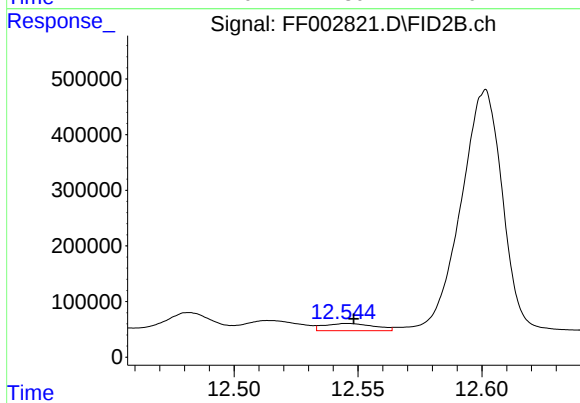

#7 N-EICOSANE


R.T.: 12.546 min
Delta R.T.: -0.003 min
Response: 182557
Conc: 1.89 ug/ml

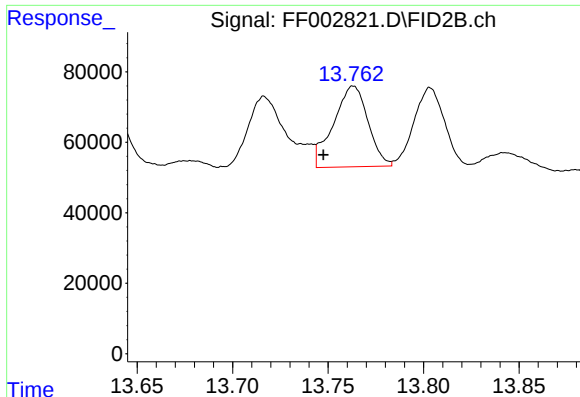

#8 N-DOCOSANE


R.T.: 13.763 min
Delta R.T.: 0.016 min
Response: 288775
Conc: 3.15 ug/ml

Instrument :
FID_F
ClientSampleId :

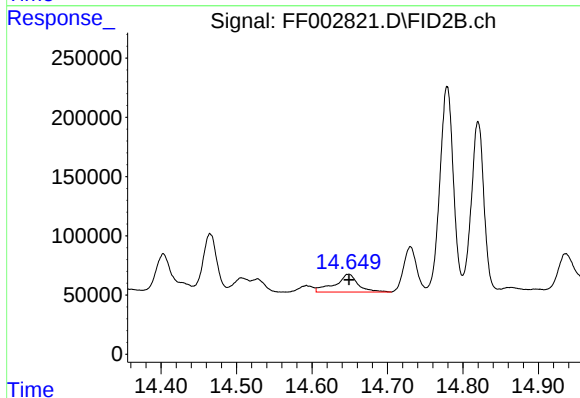


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.649 min
Delta R.T.: 0.000 min
Response: 317443
Conc: 4.06 ug/ml

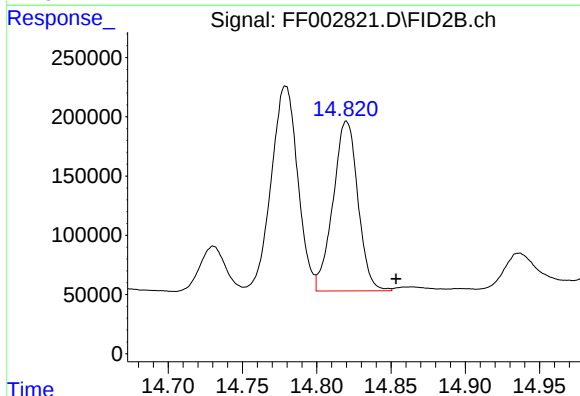


#10 N-TETRACOSANE

R.T.: 14.820 min
Delta R.T.: -0.033 min
Response: 1672495
Conc: 18.77 ug/ml

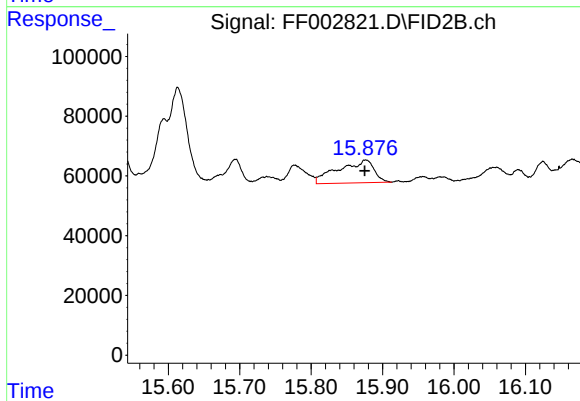

#11 N-HEXACOSANE


R.T.: 15.876 min
Delta R.T.: 0.001 min
Response: 264371
Conc: 2.91 ug/ml

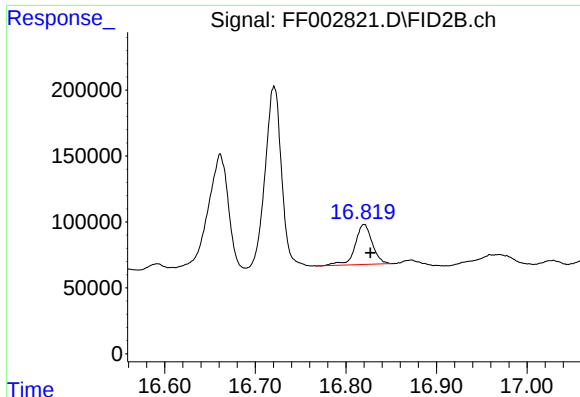

#12 N-OCTACOSANE


R.T.: 16.820 min
Delta R.T.: -0.007 min
Response: 400749
Conc: 4.20 ug/ml

Instrument :
FID_F
ClientSampleId :

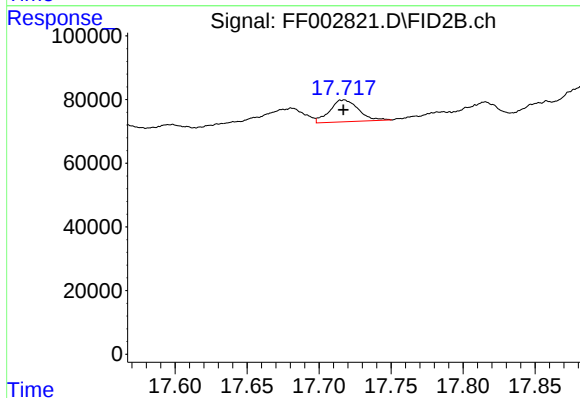


#13 N-TRIACONTANE

R.T.: 17.717 min
Delta R.T.: 0.000 min
Response: 95046
Conc: 0.96 ug/ml

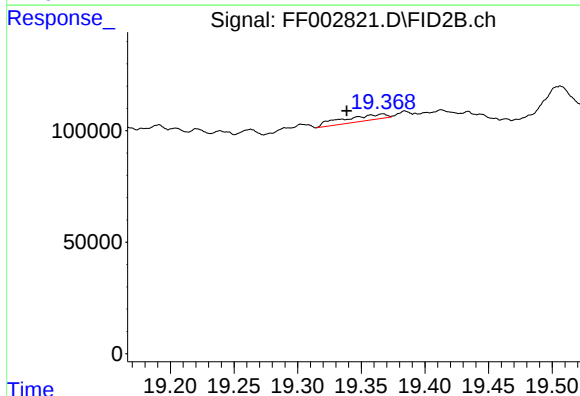

#15 N-TETRATRIACONTANE

R.T.: 19.367 min
Delta R.T.: 0.028 min
Response: 65314
Conc: 0.66 ug/ml

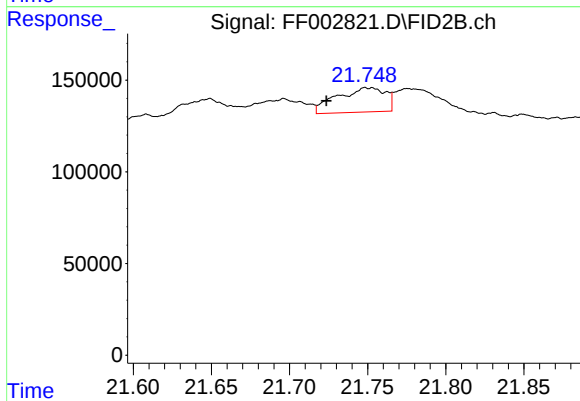

#18 N-TETRACONTANE

R.T.: 21.749 min
Delta R.T.: 0.025 min
Response: 288151
Conc: 3.29 ug/ml