

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002822.D
 Signal(s) : FID2B.ch
 Acq On : 28 Nov 2018 23:04
 Operator : AJ\SJ
 Sample : J6028-08 10X
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:01:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	197769	2.532 ug/ml
Target Compounds			
7) N-EICOSANE	12.595	423919	4.378 ug/ml
10) N-TETRACOSANE	14.817	189374	2.126 ug/ml
15) N-TETRATRIACONTANE	19.347	24809	0.251 ug/ml
16) N-HEXATRIACONTANE	20.022f	70459	0.739 ug/ml
18) N-TETRACONTANE	21.740	283008	3.231 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002822.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 23:04
Operator : AJ\SJ
Sample : J6028-08 10X
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:01:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

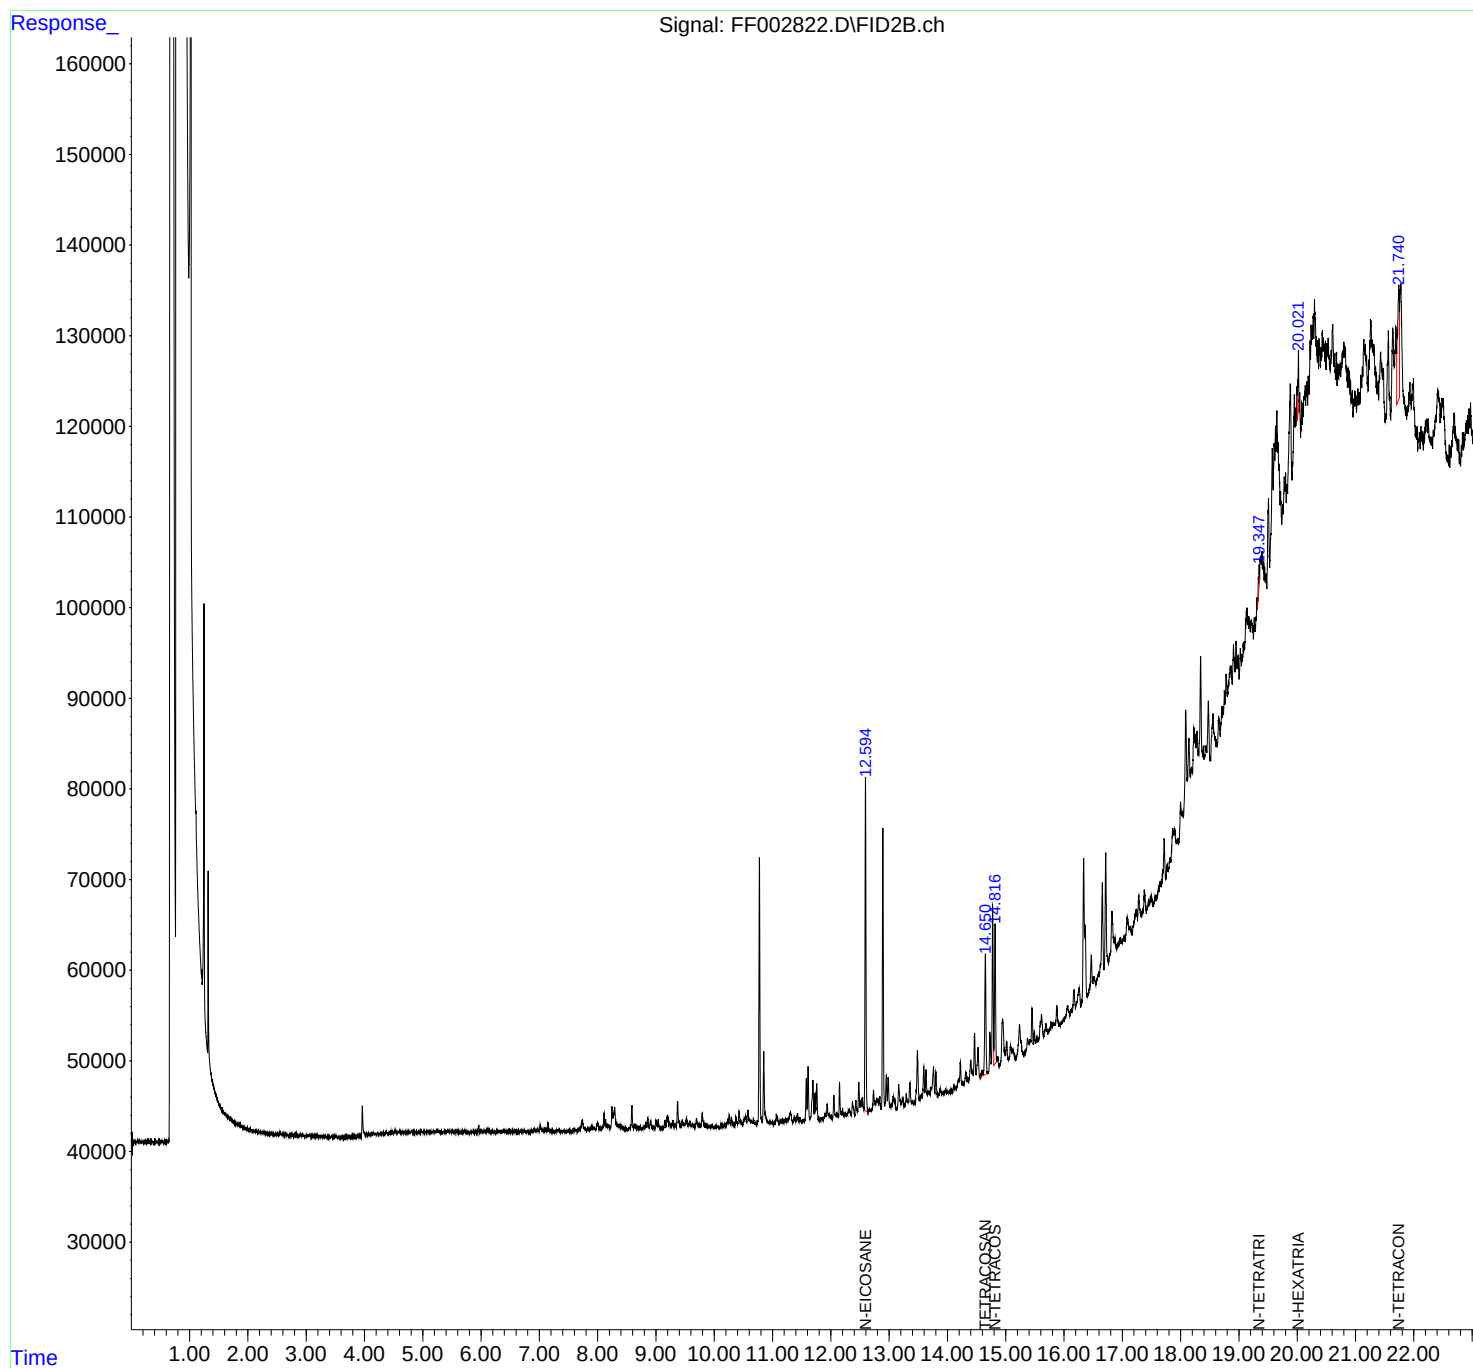


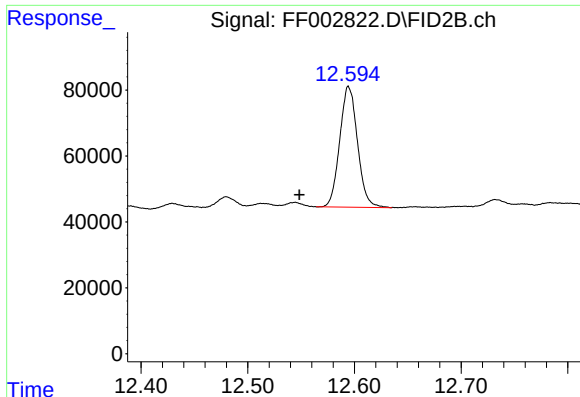

#7 N-EICOSANE


R.T.: 12.595 min
Delta R.T.: 0.046 min
Response: 423919
Conc: 4.38 ug/ml

Instrument :
FID_F
ClientSampleId :

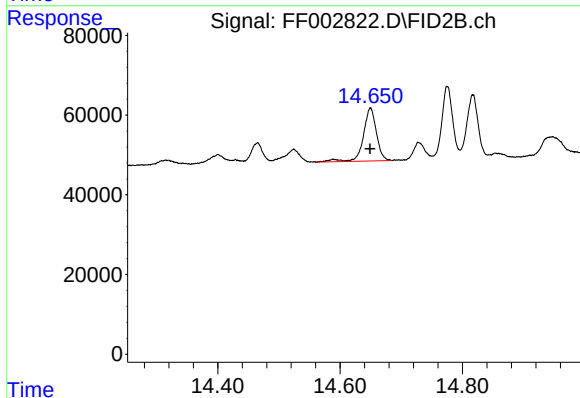


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.000 min
Response: 197769
Conc: 2.53 ug/ml

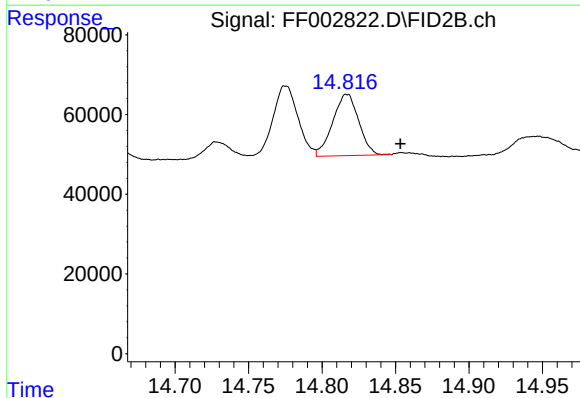


#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: -0.036 min
Response: 189374
Conc: 2.13 ug/ml

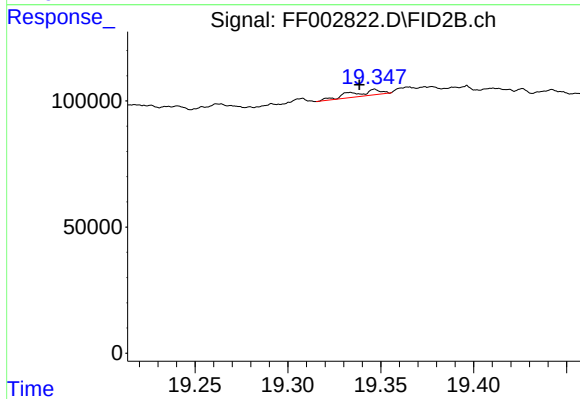

#15 N-TETRATRIACONTANE


R.T.: 19.347 min
Delta R.T.: 0.008 min
Response: 24809
Conc: 0.25 ug/ml

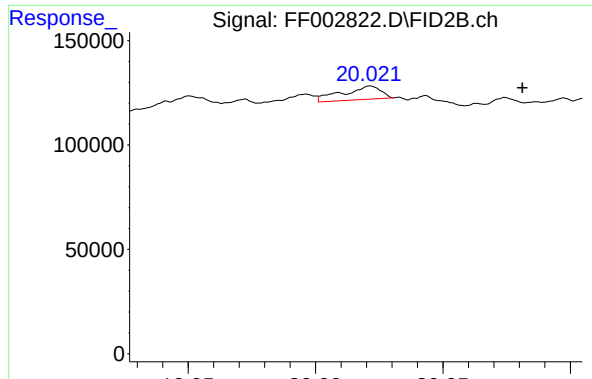

#16 N-HEXATRIACONTANE

R.T.: 20.022 min
Delta R.T.: -0.059 min
Response: 70459
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :

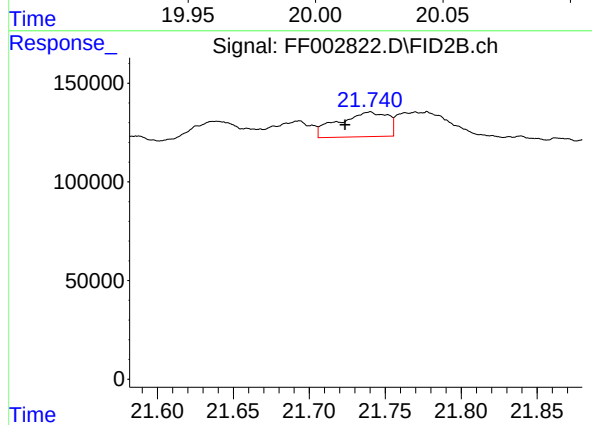

#18 N-TETRACONTANE

R.T.: 21.740 min
Delta R.T.: 0.016 min
Response: 283008
Conc: 3.23 ug/ml