

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002823.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 23:34
Operator : AJ\SJ
Sample : J6080-04 10X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:01:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.650	139328	1.784 ug/ml
Target Compounds				
7)	N-EICOSANE	12.595	98185	1.014 ug/ml
16)	N-HEXATRIACONTANE	20.013f	146883	1.541 ug/ml
18)	N-TETRACONTANE	21.738	251285	2.869 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002823.D
Signal(s) : FID2B.ch
Acq On : 28 Nov 2018 23:34
Operator : AJ\SJ
Sample : J6080-04 10X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Nov 29 01:01:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

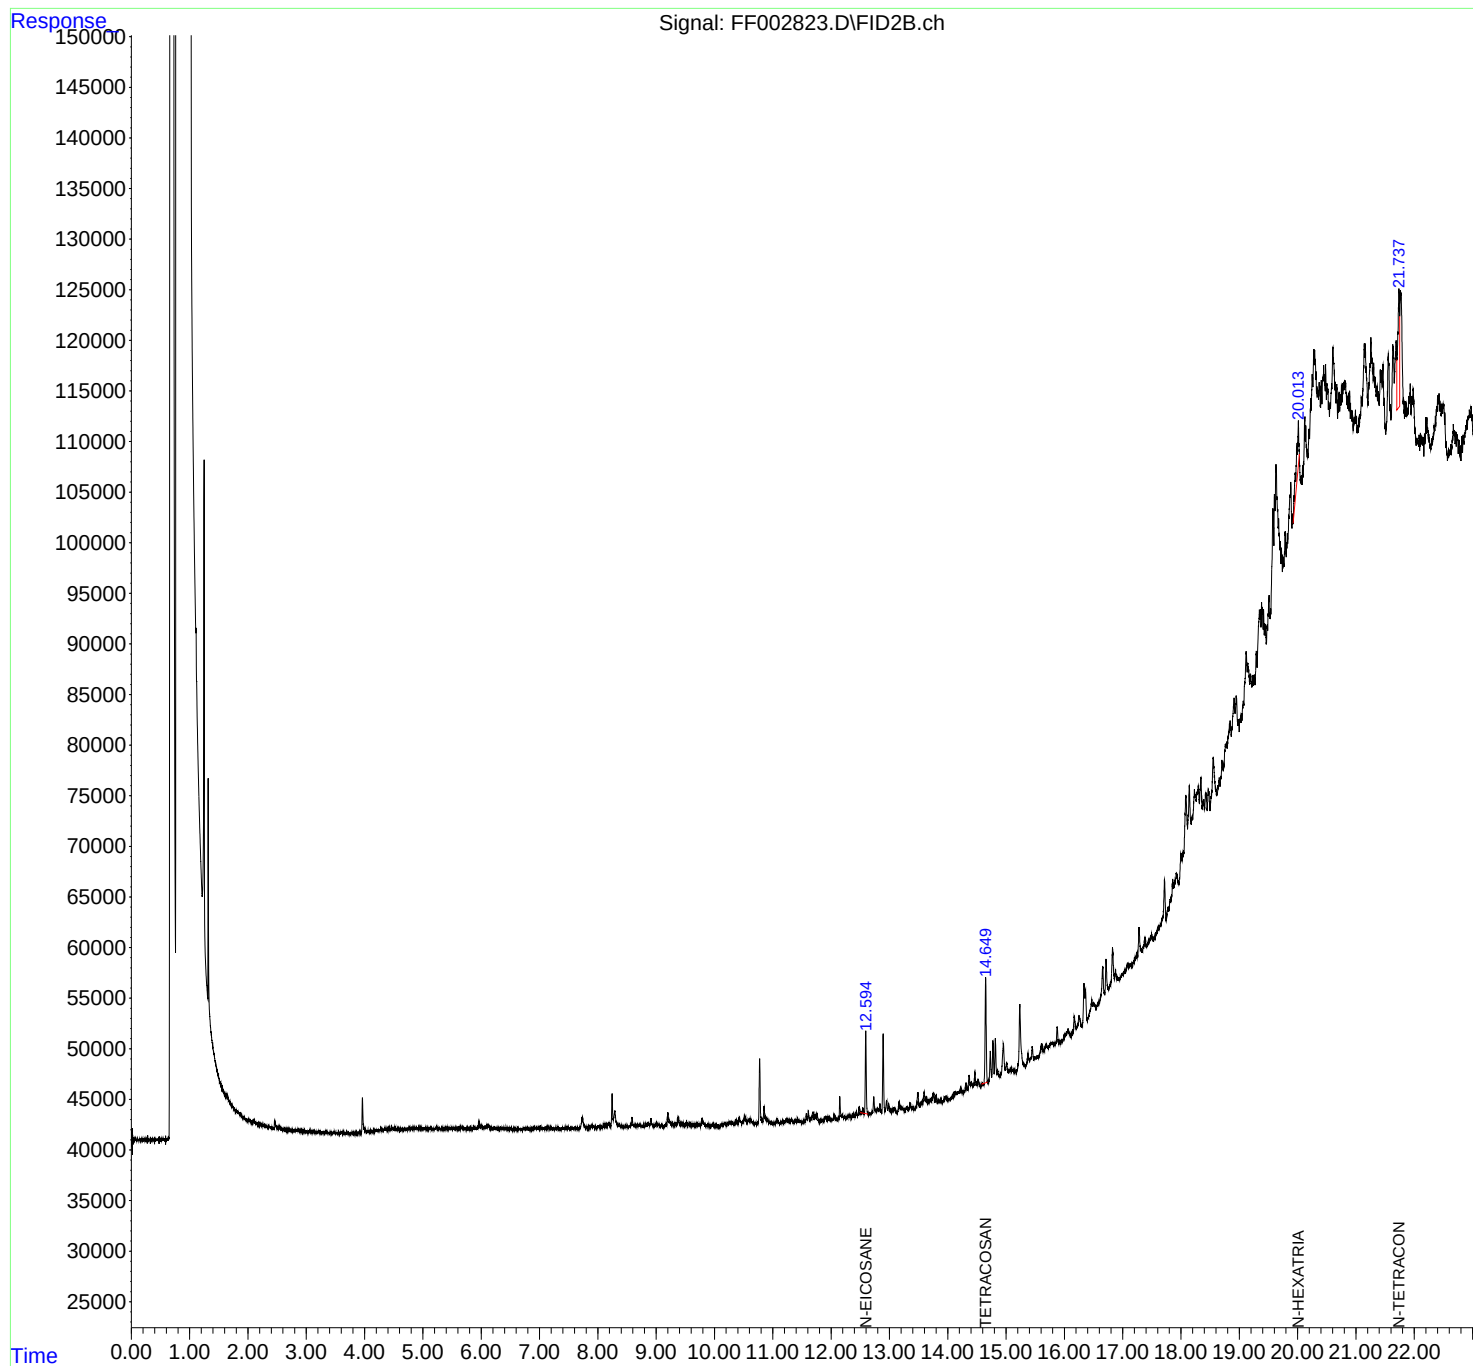


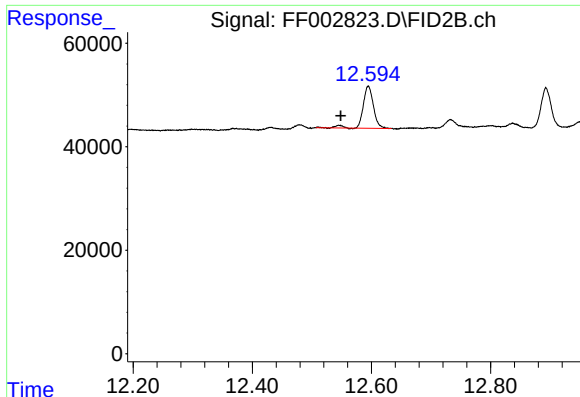

#7 N-EICOSANE


R.T.: 12.595 min
Delta R.T.: 0.046 min
Response: 98185
Conc: 1.01 ug/ml

Instrument :
FID_F
ClientSampleId :

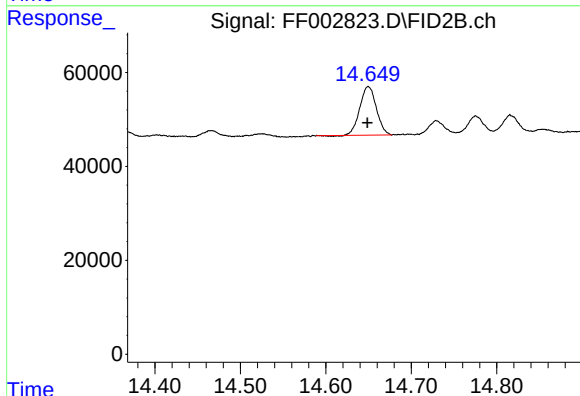


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.000 min
Response: 139328
Conc: 1.78 ug/ml

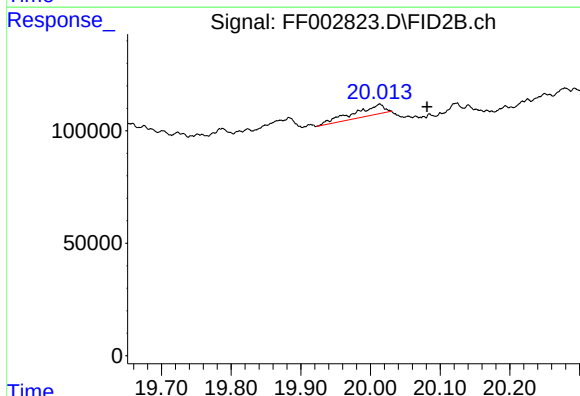

#16 N-HEXATRIACONTANE

R.T.: 20.013 min
Delta R.T.: -0.068 min
Response: 146883
Conc: 1.54 ug/ml

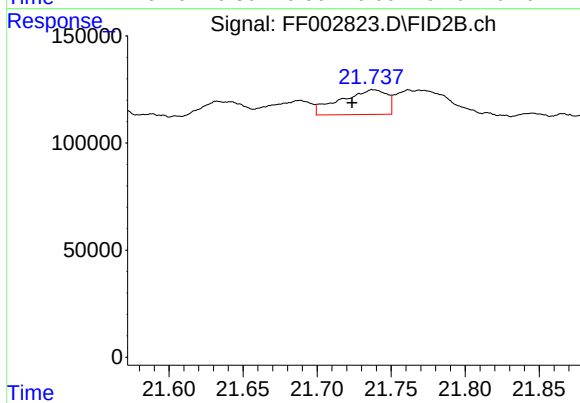

#18 N-TETRACONTANE

R.T.: 21.738 min
Delta R.T.: 0.014 min
Response: 251285
Conc: 2.87 ug/ml