

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002824.D
 Signal(s) : FID2B.ch
 Acq On : 29 Nov 2018 00:05
 Operator : AJ\SJ
 Sample : J6080-02 5X
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:02:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.650	265215	3.395 ug/ml
Target Compounds			
7) N-EICOSANE	12.594	224415	2.318 ug/ml
10) N-TETRACOSANE	14.816	88887	0.998 ug/ml
13) N-TRIACONTANE	17.716	106532	1.075 ug/ml
15) N-TETRATRIACONTANE	19.334	38240	0.387 ug/ml
18) N-TETRACONTANE	21.746	63102	0.720 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002824.D
Signal(s) : FID2B.ch
Acq On : 29 Nov 2018 00:05
Operator : AJ\SJ
Sample : J6080-02 5X
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:02:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

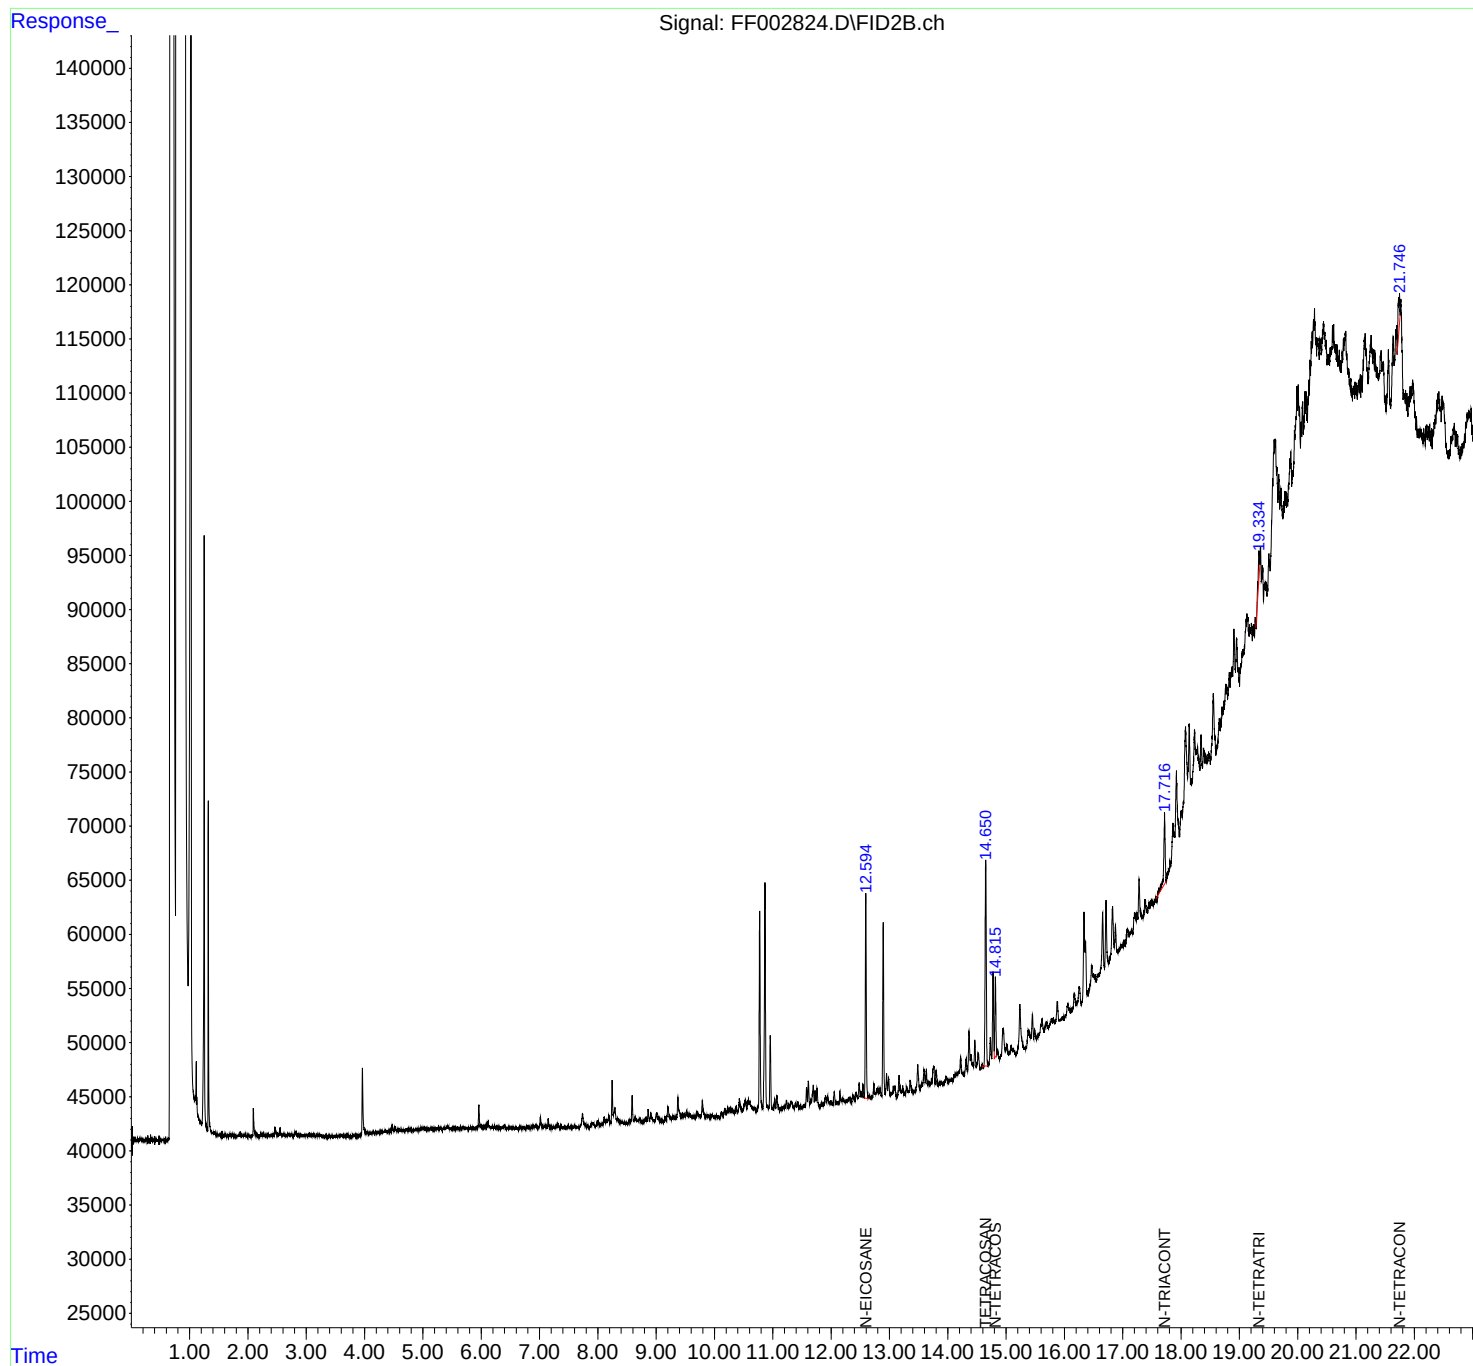


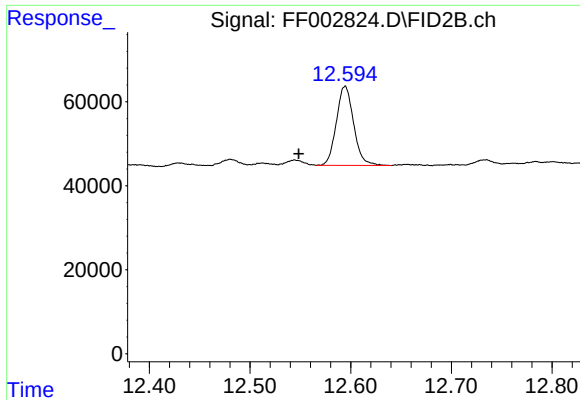

#7 N-EICOSANE


R.T.: 12.594 min
Delta R.T.: 0.046 min
Response: 224415
Conc: 2.32 ug/ml

Instrument :
FID_F
ClientSampleId :

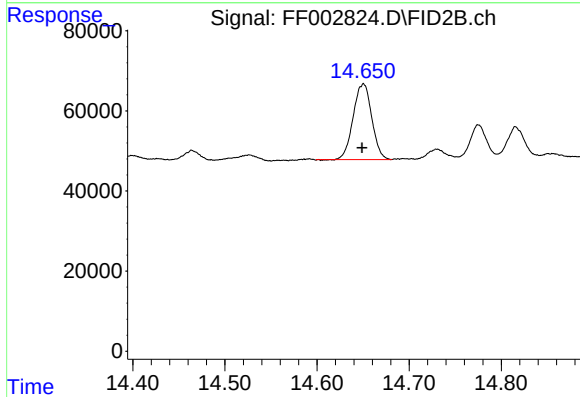


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.650 min
Delta R.T.: 0.002 min
Response: 265215
Conc: 3.40 ug/ml

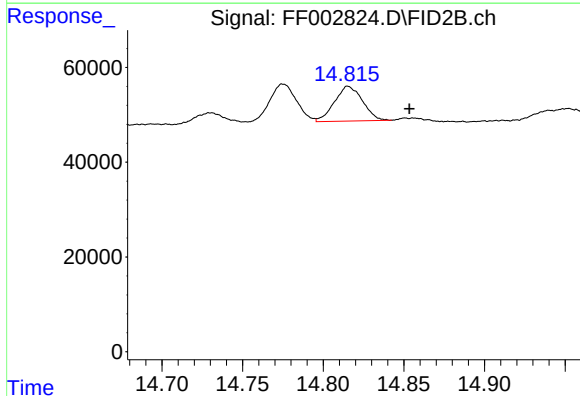


#10 N-TETRACOSANE

R.T.: 14.816 min
Delta R.T.: -0.038 min
Response: 88887
Conc: 1.00 ug/ml

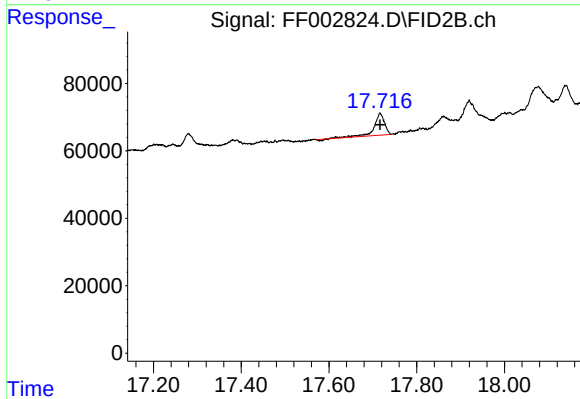

#13 N-TRIACONTANE


R.T.: 17.716 min
Delta R.T.: 0.000 min
Response: 106532
Conc: 1.07 ug/ml

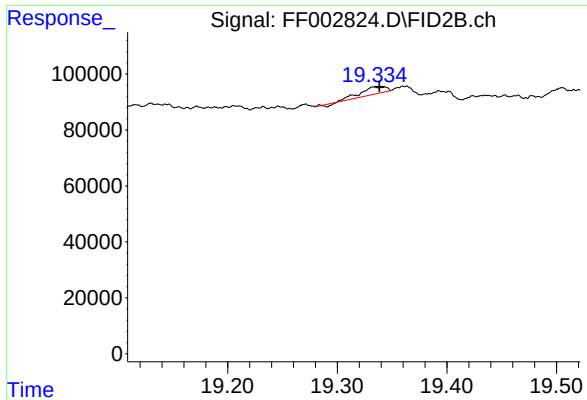

#15 N-TETRATRIACONTANE

R.T.: 19.334 min
Delta R.T.: -0.005 min
Response: 38240
Conc: 0.39 ug/ml

Instrument :
FID_F
ClientSampleId :

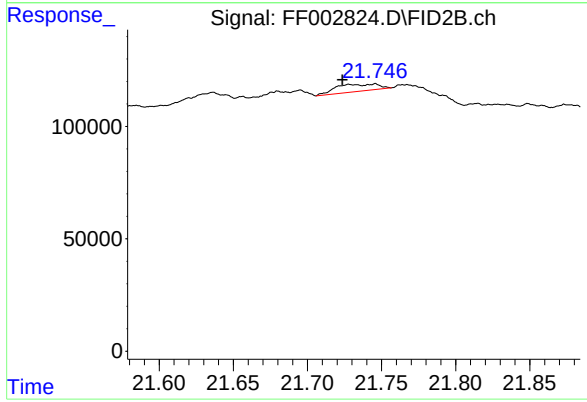

#18 N-TETRACONTANE

R.T.: 21.746 min
Delta R.T.: 0.022 min
Response: 63102
Conc: 0.72 ug/ml