

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
 Data File : FF002825.D
 Signal(s) : FID2B.ch
 Acq On : 29 Nov 2018 00:35
 Operator : AJ\SJ
 Sample : J6080-03 5X
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 29 01:02:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.649	246844	3.160 ug/ml
Target Compounds			
7) N-EICOSANE	12.594	198031	2.045 ug/ml
13) N-TRIACONTANE	17.718	96431	0.973 ug/ml
14) N-DOTRIACONTANE	18.553	152471	1.540 ug/ml
18) N-TETRACONTANE	21.736	121015	1.382 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112818\
Data File : FF002825.D
Signal(s) : FID2B.ch
Acq On : 29 Nov 2018 00:35
Operator : AJ\SJ
Sample : J6080-03 5X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 29 01:02:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

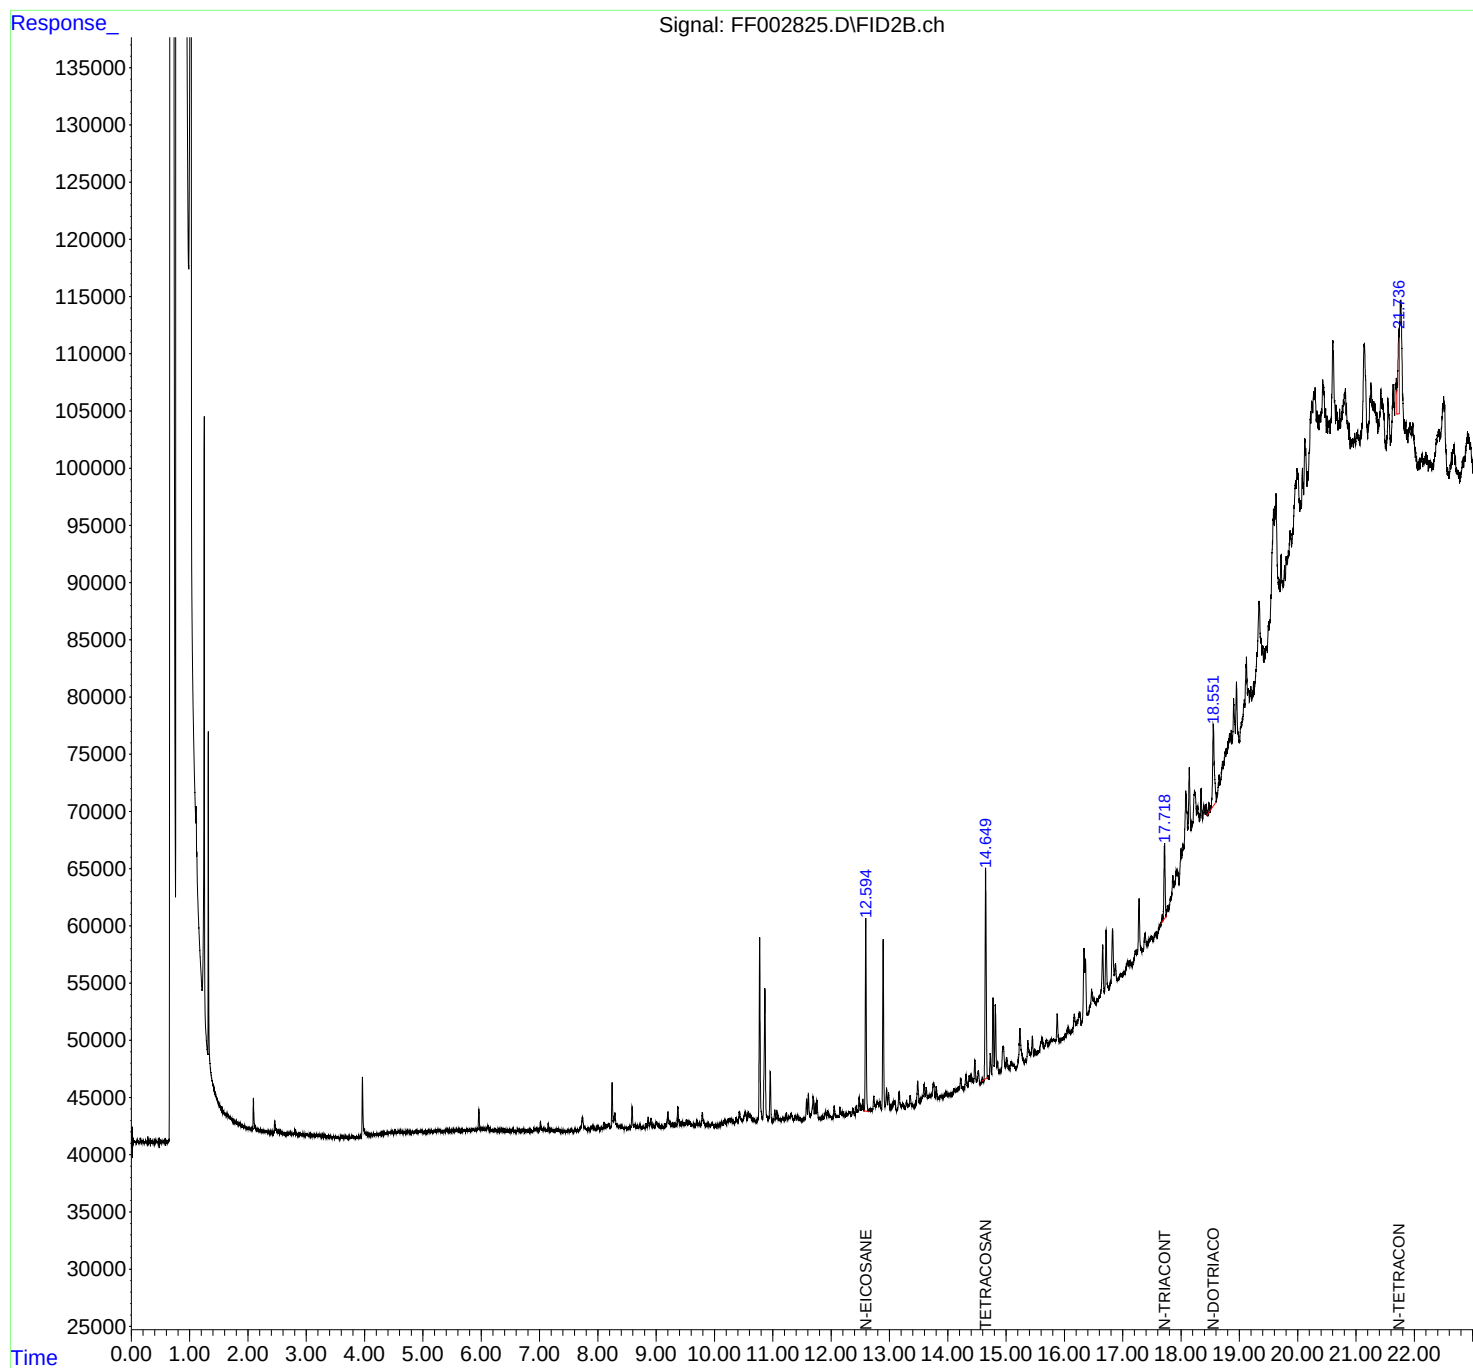


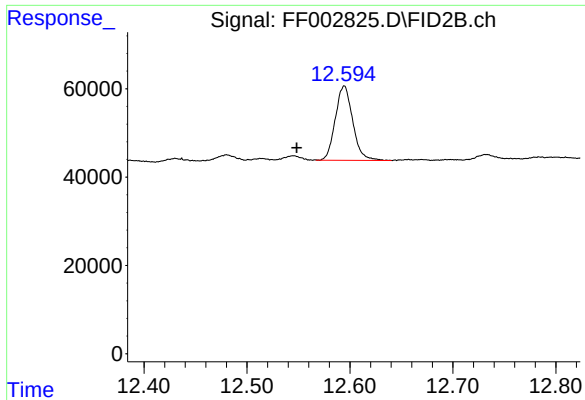

#7 N-EICOSANE


R.T.: 12.594 min
Delta R.T.: 0.046 min
Response: 198031
Conc: 2.05 ug/ml

Instrument :
FID_F
ClientSampleId :

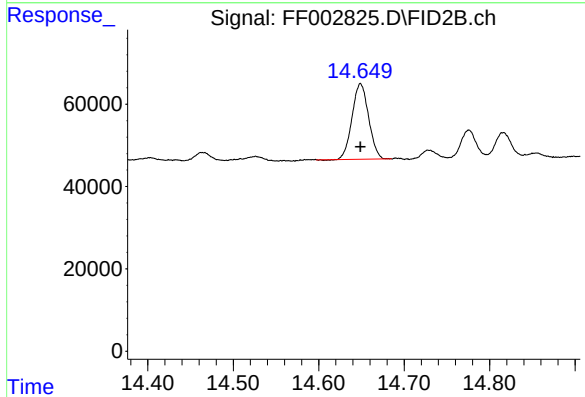


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.649 min
Delta R.T.: 0.000 min
Response: 246844
Conc: 3.16 ug/ml

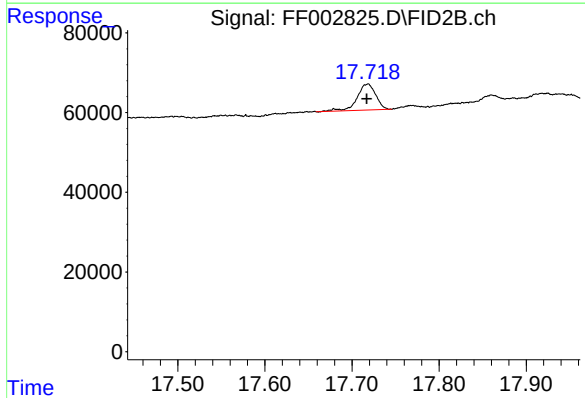


#13 N-TRIACONTANE

R.T.: 17.718 min
Delta R.T.: 0.001 min
Response: 96431
Conc: 0.97 ug/ml

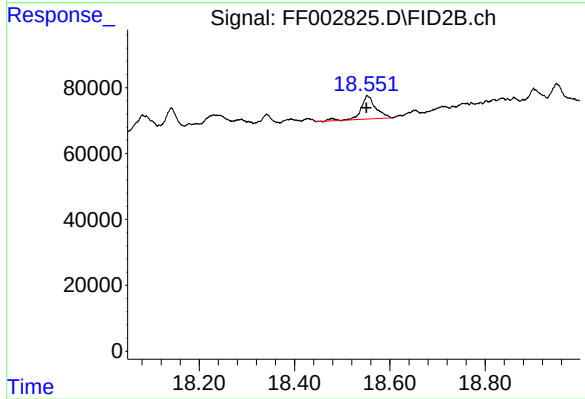

#14 N-DOTRIACONTANE

R.T.: 18.553 min
Delta R.T.: 0.002 min
Response: 152471
Conc: 1.54 ug/ml

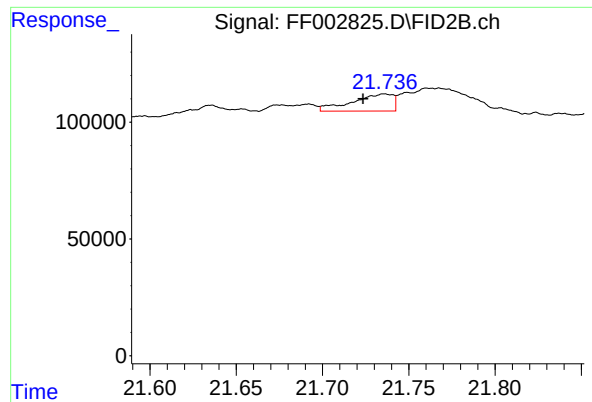

#18 N-TETRACONTANE

R.T.: 21.736 min
Delta R.T.: 0.012 min
Response: 121015
Conc: 1.38 ug/ml

Instrument :
FID_F
ClientSampleId :