

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF112818\  
 Data File : FF002826.D  
 Signal(s) : FID2B.ch  
 Acq On : 29 Nov 2018 01:05  
 Operator : AJ\SJ  
 Sample : J6080-01 5X  
 Misc :  
 ALS Vial : 78 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Nov 29 03:27:16 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF111418.M  
 Quant Title :  
 QLast Update : Wed Nov 14 13:46:00 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units  |
|-------------------------------|--------|----------|-------------|
| -----                         |        |          |             |
| System Monitoring Compounds   |        |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 14.648 | 301066   | 3.854 ug/ml |
| Target Compounds              |        |          |             |
| 7) N-EICOSANE                 | 12.594 | 141753   | 1.464 ug/ml |
| 12) N-OCTACOSANE              | 16.828 | 92821    | 0.973 ug/ml |
| 13) N-TRIACONTANE             | 17.717 | 142313   | 1.436 ug/ml |
| 14) N-DOTRIACONTANE           | 18.554 | 212422   | 2.146 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.337 | 126902   | 1.286 ug/ml |
| 18) N-TETRACONTANE            | 21.731 | 50002    | 0.571 ug/ml |
| -----                         |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF112818\  
Data File : FF002826.D  
Signal(s) : FID2B.ch  
Acq On : 29 Nov 2018 01:05  
Operator : AJ\SJ  
Sample : J6080-01 5X  
Misc :  
ALS Vial : 78 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampled :

Integration File: autoint1.e  
Quant Time: Nov 29 03:27:16 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF111418.M  
Quant Title :  
QLast Update : Wed Nov 14 13:46:00 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

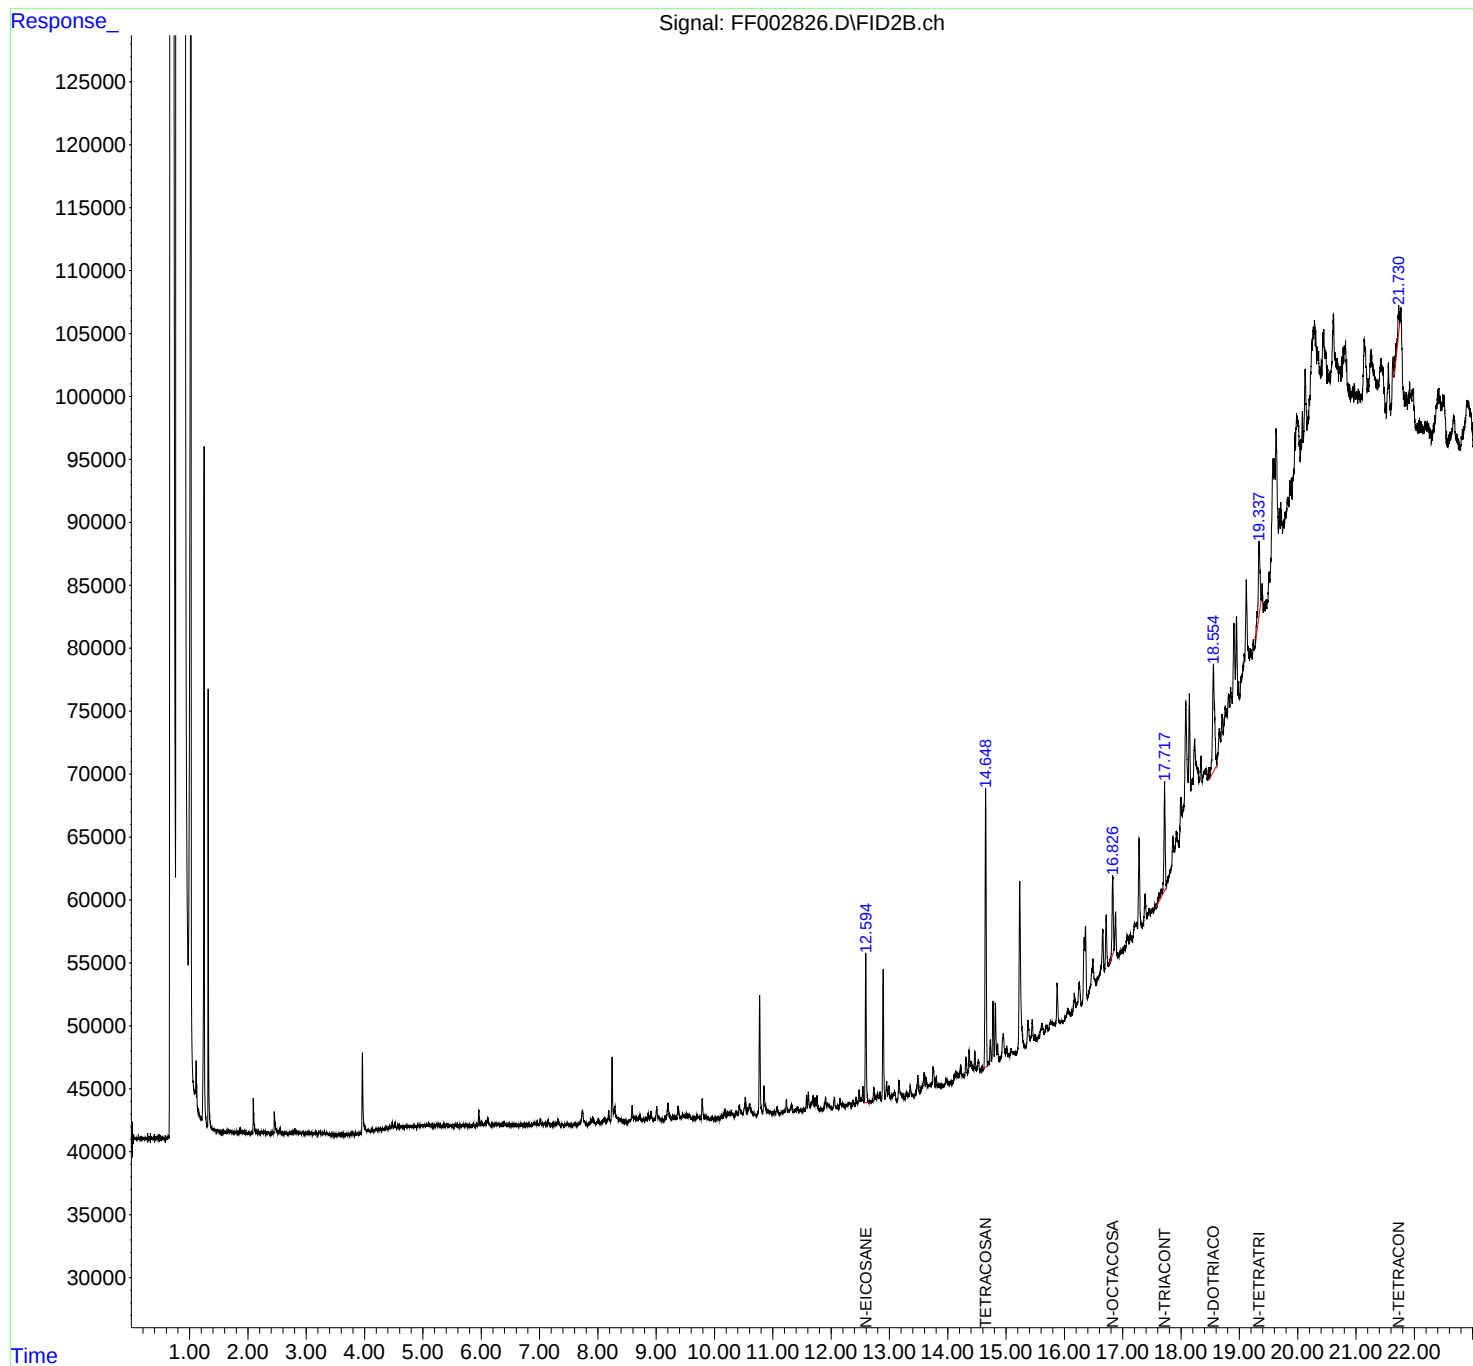


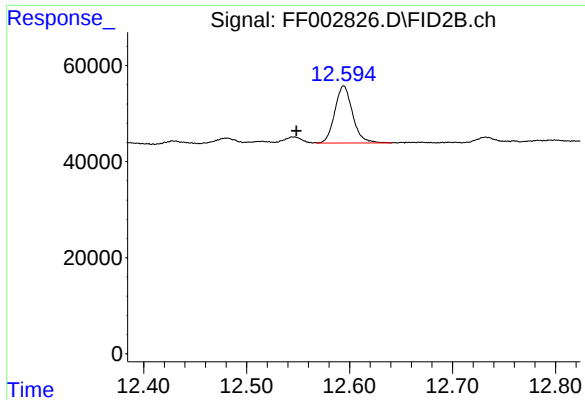

#7 N-EICOSANE


R.T.: 12.594 min  
Delta R.T.: 0.046 min  
Response: 141753  
Conc: 1.46 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

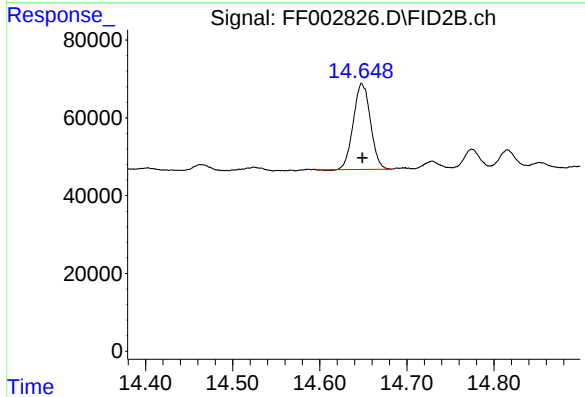


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min  
Delta R.T.: 0.000 min  
Response: 301066  
Conc: 3.85 ug/ml

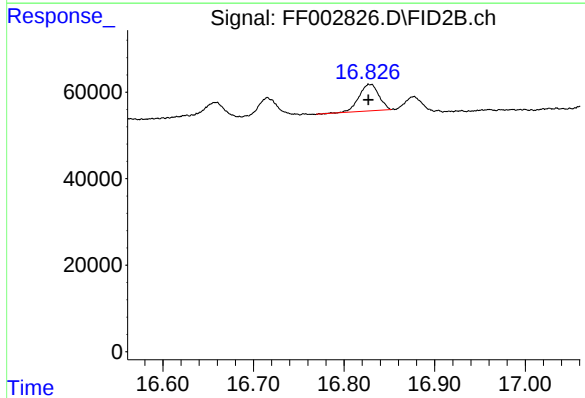


#12 N-OCTACOSANE

R.T.: 16.828 min  
Delta R.T.: 0.001 min  
Response: 92821  
Conc: 0.97 ug/ml

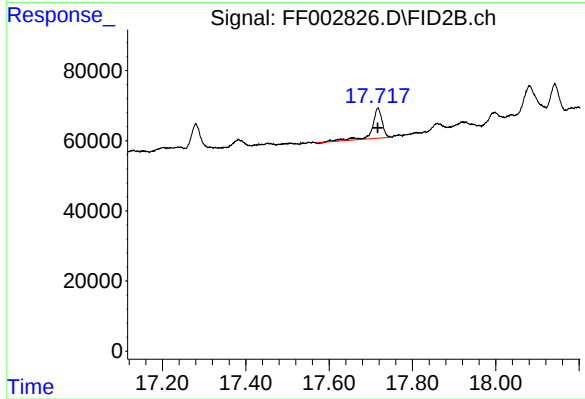

#13 N-TRIACONTANE


R.T.: 17.717 min  
Delta R.T.: 0.000 min  
Response: 142313  
Conc: 1.44 ug/ml

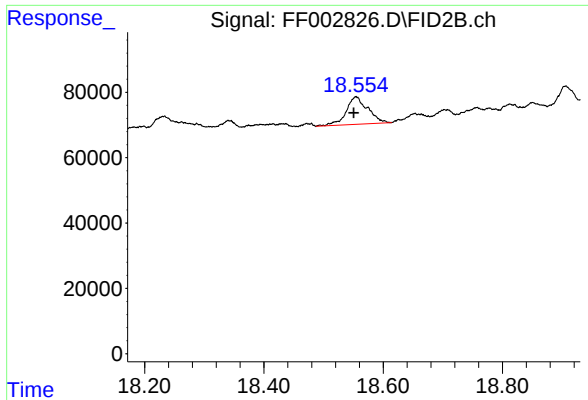

#14 N-DOTRIACONTANE


R.T.: 18.554 min  
Delta R.T.: 0.004 min  
Response: 212422  
Conc: 2.15 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

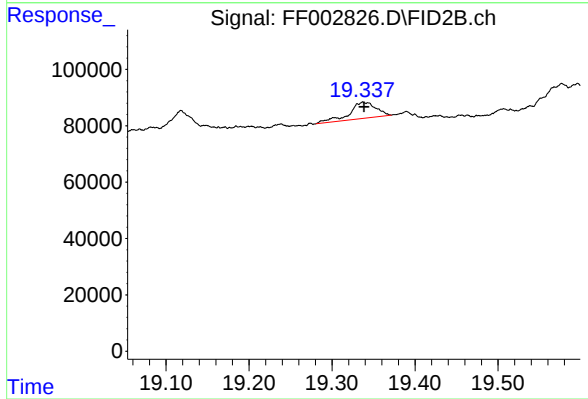

#15 N-TETRATRIACONTANE

R.T.: 19.337 min  
Delta R.T.: -0.001 min  
Response: 126902  
Conc: 1.29 ug/ml

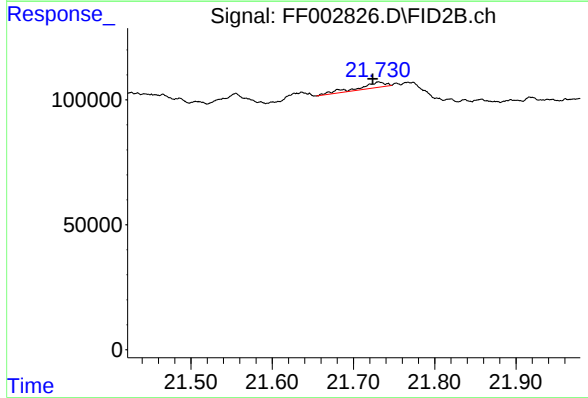

#18 N-TETRACONTANE

R.T.: 21.731 min  
Delta R.T.: 0.007 min  
Response: 50002  
Conc: 0.57 ug/ml