

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF112818\  
 Data File : FF002830.D  
 Signal(s) : FID2B.ch  
 Acq On : 29 Nov 2018 03:07  
 Operator : AJ\SJ  
 Sample : J6083-01 2X  
 Misc :  
 ALS Vial : 82 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Nov 29 03:28:14 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF111418.M  
 Quant Title :  
 QLast Update : Wed Nov 14 13:46:00 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.648	1022149	13.085 ug/ml
Target Compounds			
4) N-TETRADECANE	8.243f	156476	1.355 ug/ml
12) N-OCTACOSANE	16.828	114756	1.203 ug/ml
13) N-TRIACONTANE	17.717	141128	1.424 ug/ml
14) N-DOTRIACONTANE	18.549	192706	1.947 ug/ml
15) N-TETRATRIACONTANE	19.335	131335	1.331 ug/ml
17) N-OCTATRIACONTANE	20.818	298691	3.398 ug/ml
18) N-TETRACONTANE	21.723	770502	8.796 ug/ml
-----			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF112818\  
 Data File : FF002830.D  
 Signal(s) : FID2B.ch  
 Acq On : 29 Nov 2018 03:07  
 Operator : AJ\SJ  
 Sample : J6083-01 2X  
 Misc :  
 ALS Vial : 82 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampled :

Integration File: autoint1.e  
 Quant Time: Nov 29 03:28:14 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF111418.M  
 Quant Title :  
 QLast Update : Wed Nov 14 13:46:00 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

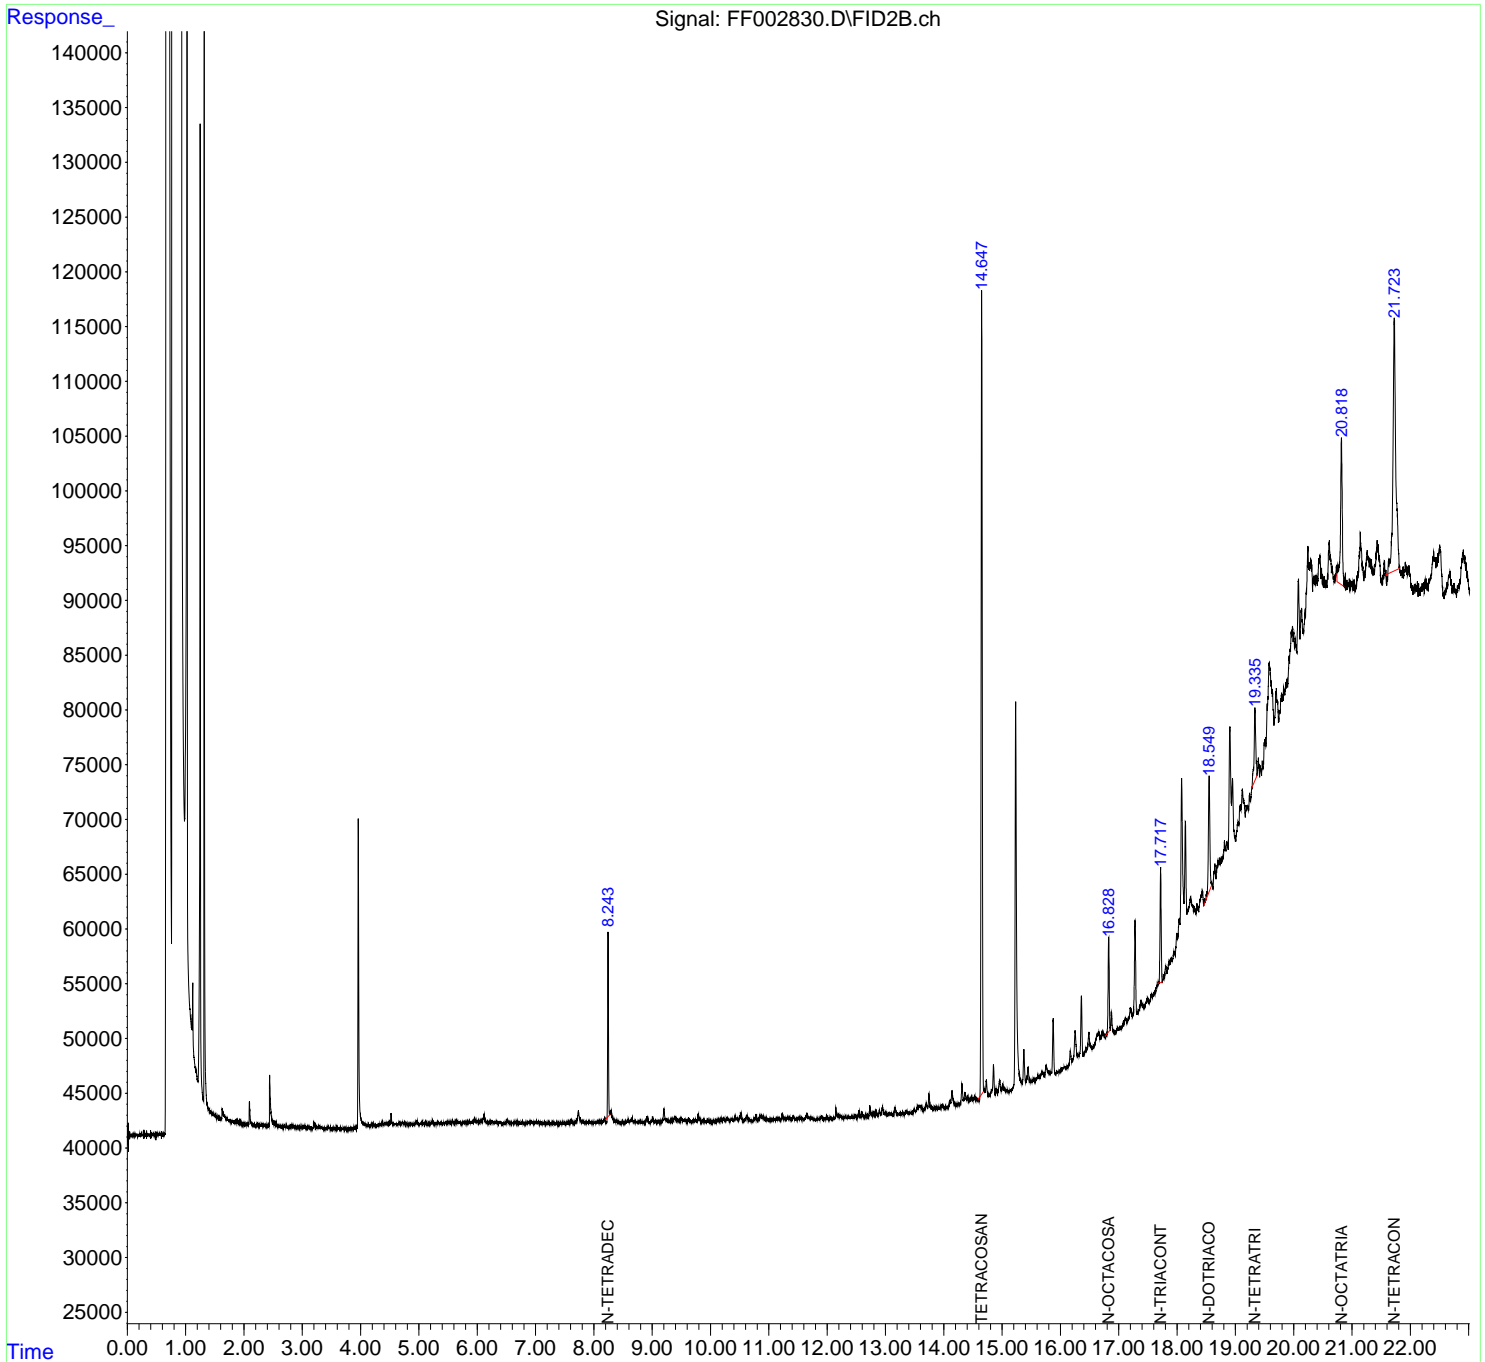


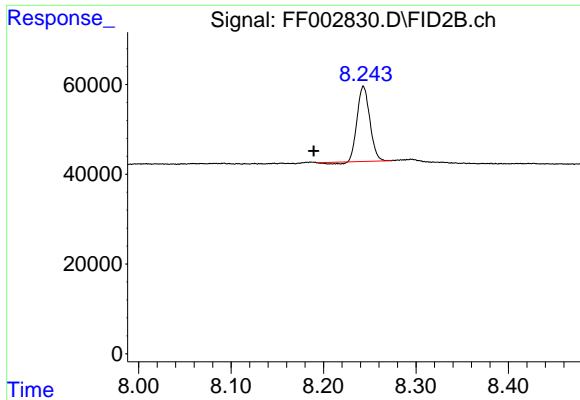

#4 N-TETRADECANE


R.T.: 8.243 min  
Delta R.T.: 0.054 min  
Response: 156476  
Conc: 1.35 ug/ml

Instrument :  
FID\_F  
ClientSampleId :

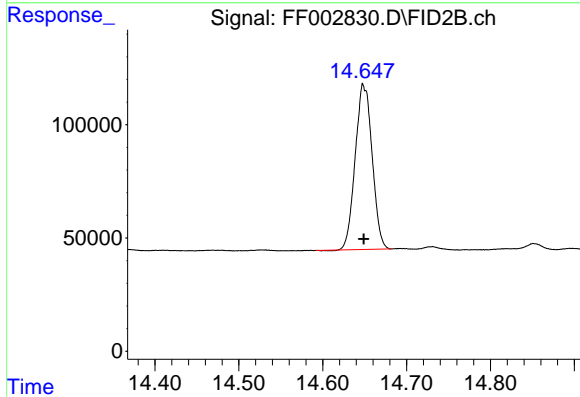


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.648 min  
Delta R.T.: 0.000 min  
Response: 1022149  
Conc: 13.08 ug/ml

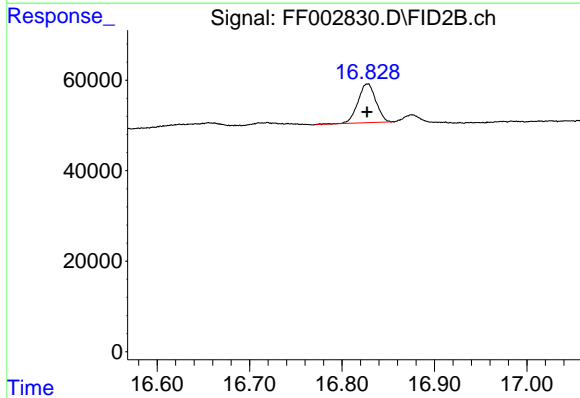


#12 N-OCTACOSANE

R.T.: 16.828 min  
Delta R.T.: 0.000 min  
Response: 114756  
Conc: 1.20 ug/ml

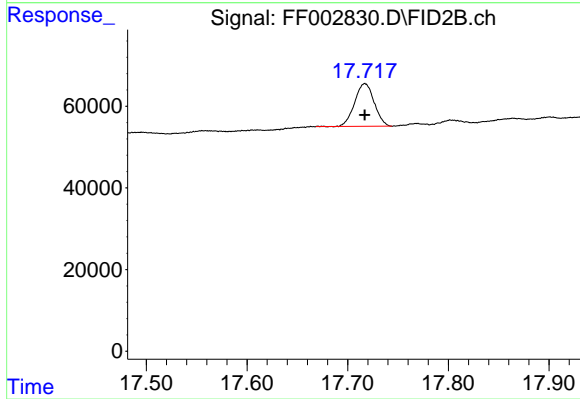


#13 N-TRIACONTANE

R.T.: 17.717 min  
Delta R.T.: 0.000 min  
Response: 141128  
Conc: 1.42 ug/ml

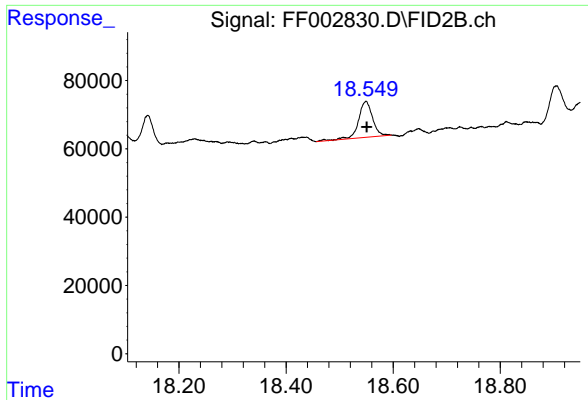


#14 N-DOTRIACONTANE  
 R.T.: 18.549 min  
 Delta R.T.: -0.001 min  
 Response: 192706  
 Conc: 1.95 ug/ml


Instrument :  
 FID\_F  
 ClientSampleId :

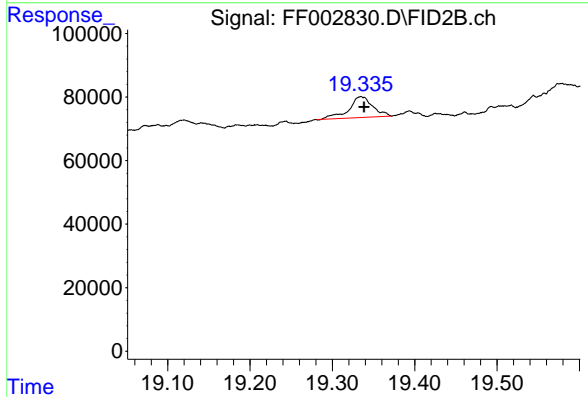

#15 N-TETRATRIACONTANE  
 R.T.: 19.335 min  
 Delta R.T.: -0.004 min  
 Response: 131335  
 Conc: 1.33 ug/ml

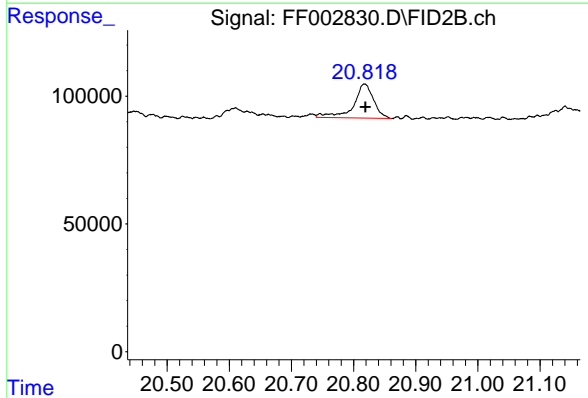

#17 N-OCTATRIACONTANE  
 R.T.: 20.818 min  
 Delta R.T.: 0.000 min  
 Response: 298691  
 Conc: 3.40 ug/ml

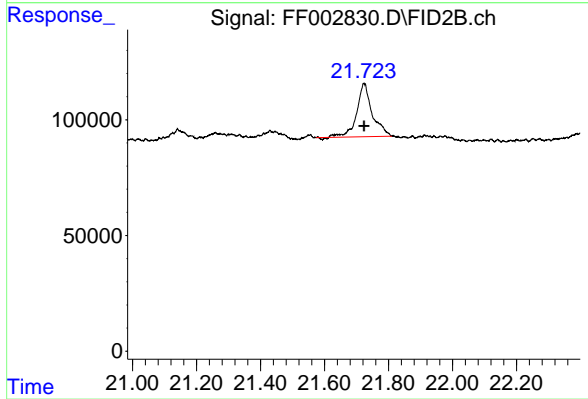

#18 N-TETRACONTANE  
 R.T.: 21.723 min  
 Delta R.T.: -0.001 min  
 Response: 770502  
 Conc: 8.80 ug/ml