

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002845.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 08:29
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Nov 30 11:03:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.648	1735024	22.211 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.716	124371	1.255 ug/ml
14) N-DOTRIACONTANE	18.551	178120	1.799 ug/ml
15) N-TETRATRIACONTANE	19.338	130312	1.320 ug/ml
16) N-HEXATRIACONTANE	20.016f	125338	1.315 ug/ml
18) N-TETRACONTANE	21.716	1033277	11.796 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002845.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 08:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 30 11:03:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

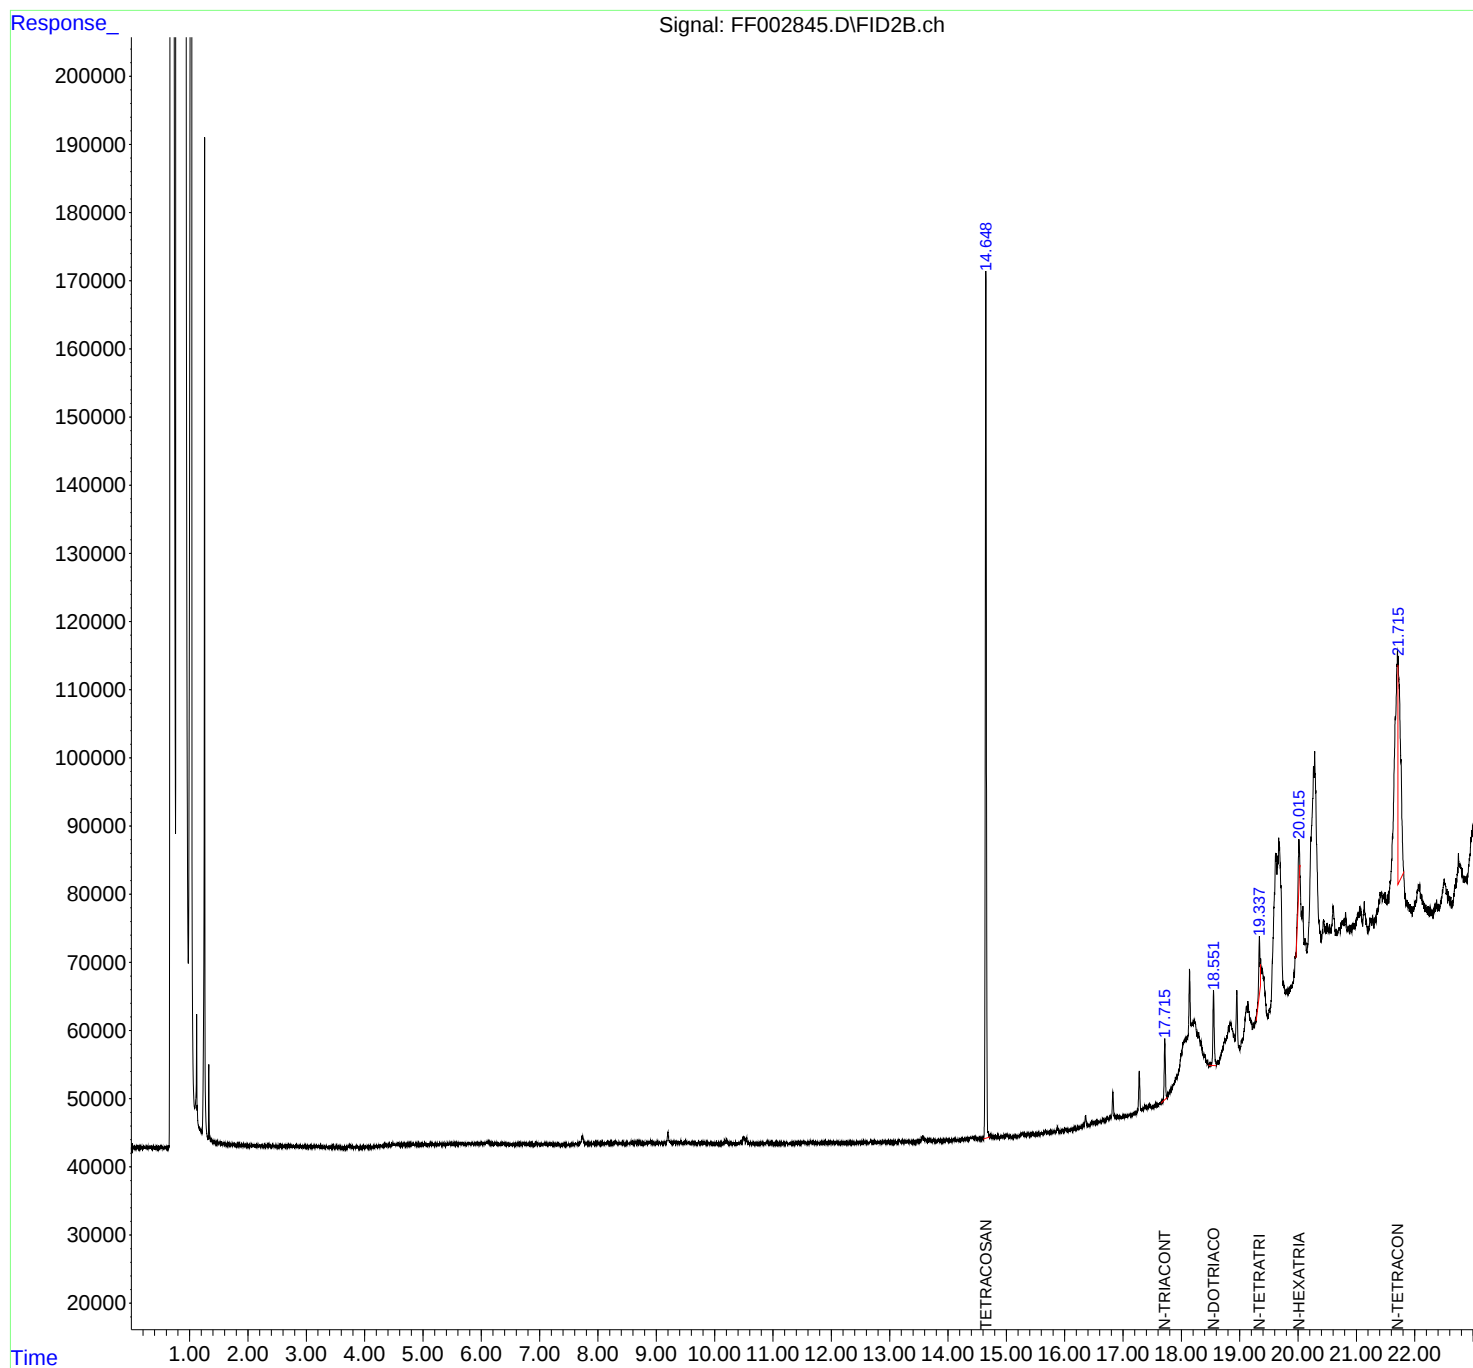


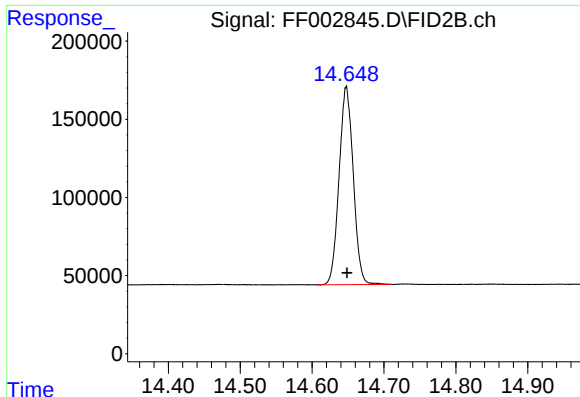

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.648 min
Delta R.T.: -0.001 min
Response: 1735024
Conc: 22.21 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

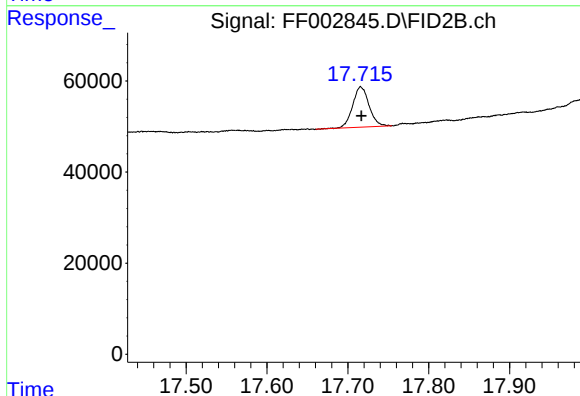


#13 N-TRIACONTANE

R.T.: 17.716 min
Delta R.T.: 0.000 min
Response: 124371
Conc: 1.25 ug/ml

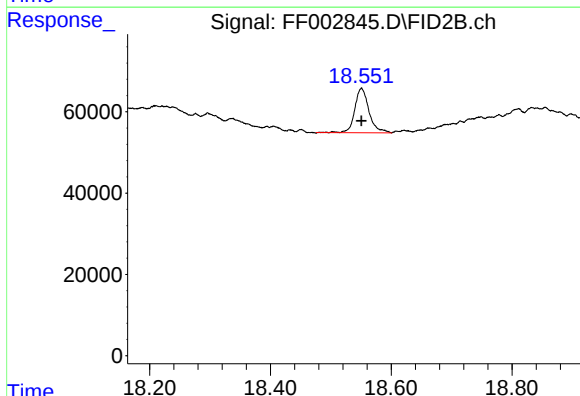


#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: 0.000 min
Response: 178120
Conc: 1.80 ug/ml

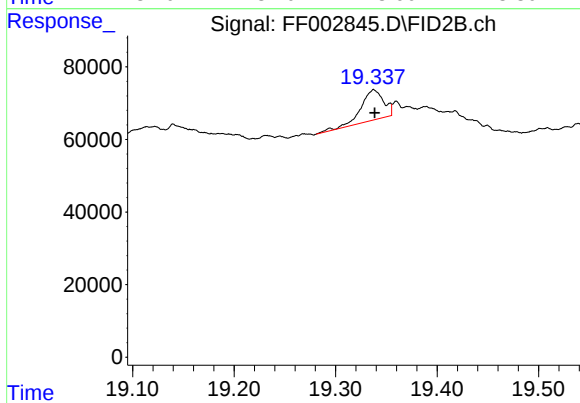

#15 N-TETRATRIACONTANE


R.T.: 19.338 min
Delta R.T.: 0.000 min
Response: 130312
Conc: 1.32 ug/ml

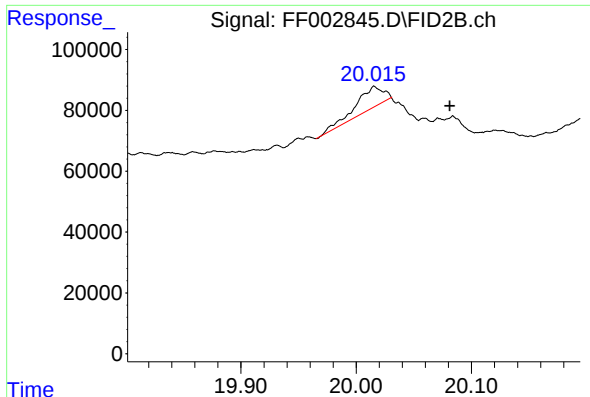

#16 N-HEXATRIACONTANE

R.T.: 20.016 min
Delta R.T.: -0.065 min
Response: 125338
Conc: 1.32 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

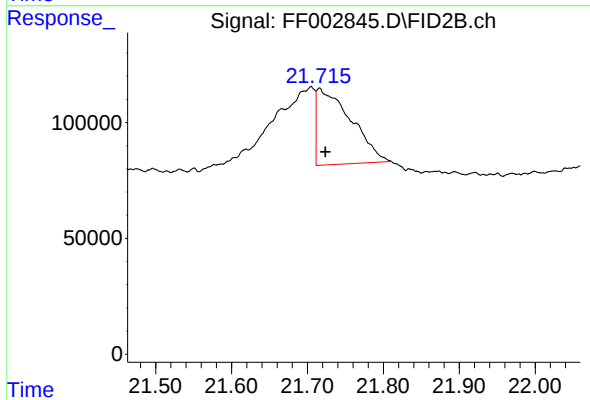

#18 N-TETRACONTANE

R.T.: 21.716 min
Delta R.T.: -0.008 min
Response: 1033277
Conc: 11.80 ug/ml