

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002847.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 09:29
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Nov 30 11:04:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.393	2494535	20.581	ug/ml
12) N-OCTACOSANE	16.827	2502598	26.238	ug/ml
13) N-TRIACONTANE	17.714	126591	1.277	ug/ml
14) N-DOTRIACONTANE	18.549	185673	1.876	ug/ml
15) N-TETRATRIACONTANE	19.336	158697	1.608	ug/ml
16) N-HEXATRIACONTANE	20.078	202822	2.128	ug/ml
17) N-OCTATRIACONTANE	20.817	581580	6.617	ug/ml
18) N-TETRACONTANE	21.718	1296708	14.803	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002847.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 09:29
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Nov 30 11:04:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

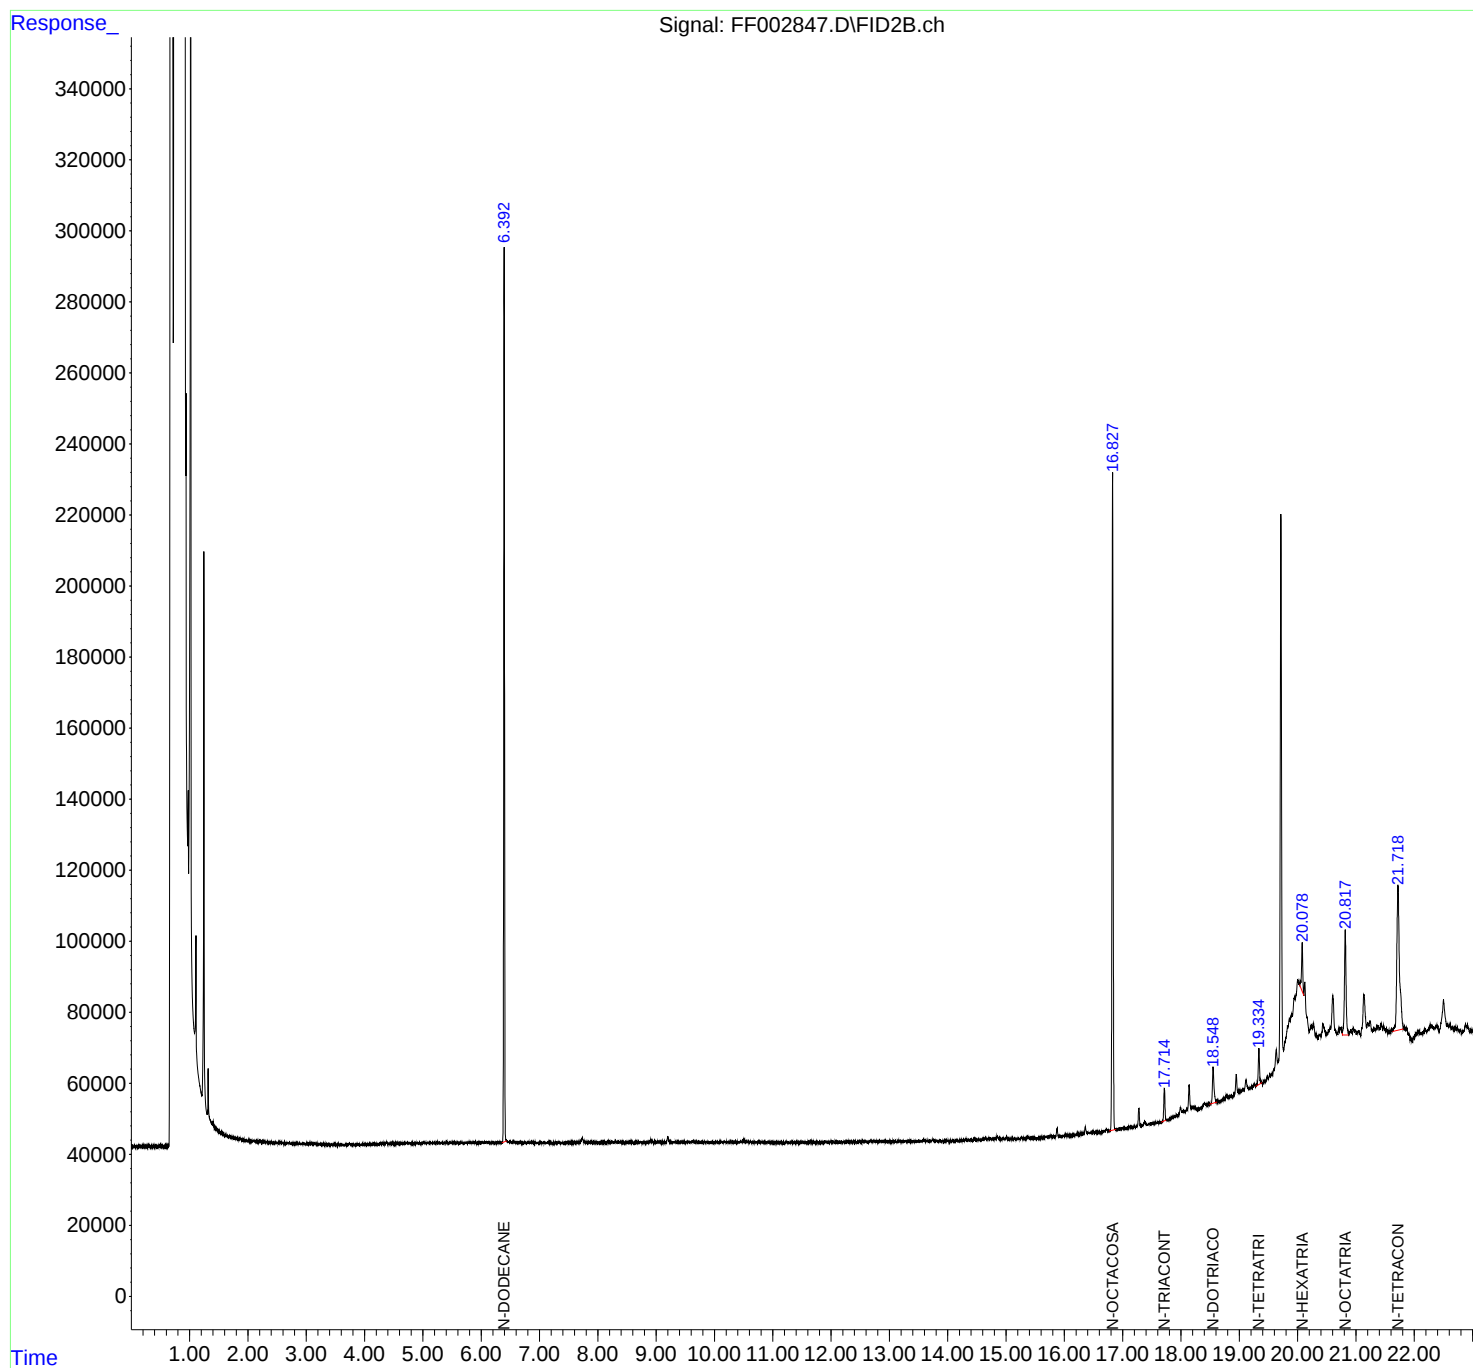


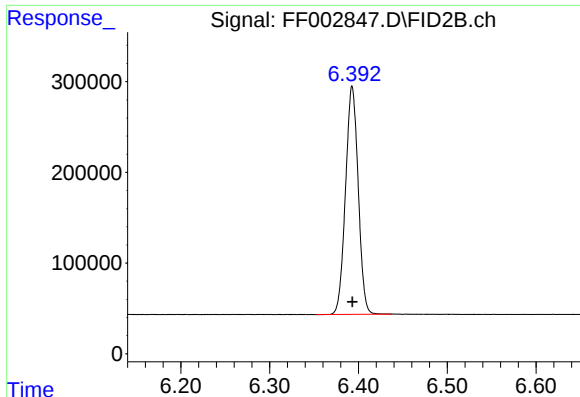

#3 N-DODECANE


R.T.: 6.393 min
Delta R.T.: 0.000 min
Response: 2494535
Conc: 20.58 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

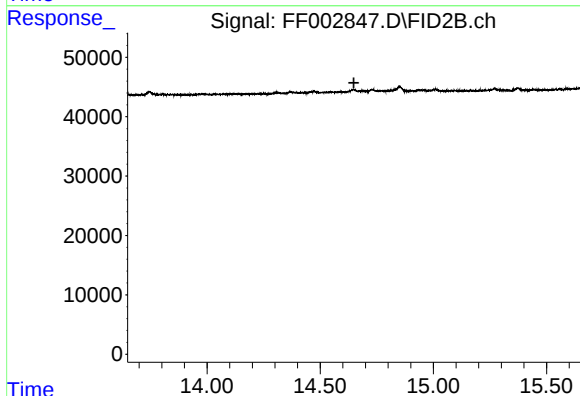


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.649 min
Response: 0
Conc: N.D.

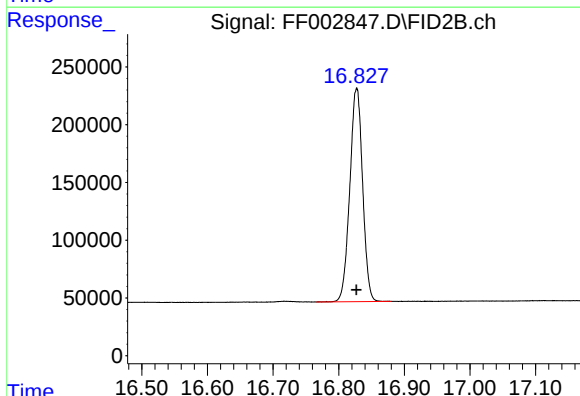


#12 N-OCTACOSANE

R.T.: 16.827 min
Delta R.T.: 0.000 min
Response: 2502598
Conc: 26.24 ug/ml

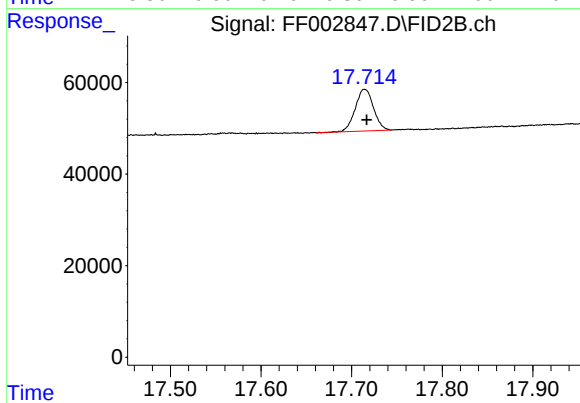

#13 N-TRIACONTANE


R.T.: 17.714 min
Delta R.T.: -0.002 min
Response: 126591
Conc: 1.28 ug/ml

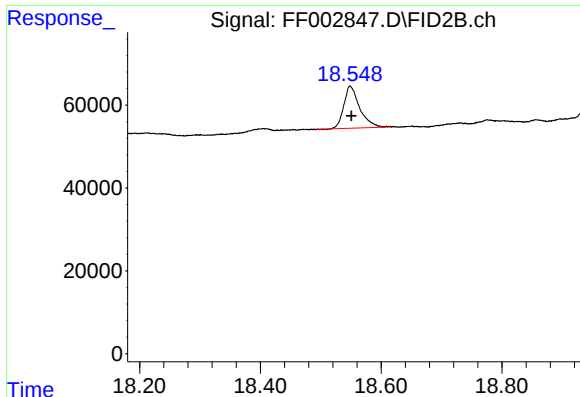

#14 N-DOTRIACONTANE


R.T.: 18.549 min
Delta R.T.: -0.002 min
Response: 185673
Conc: 1.88 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

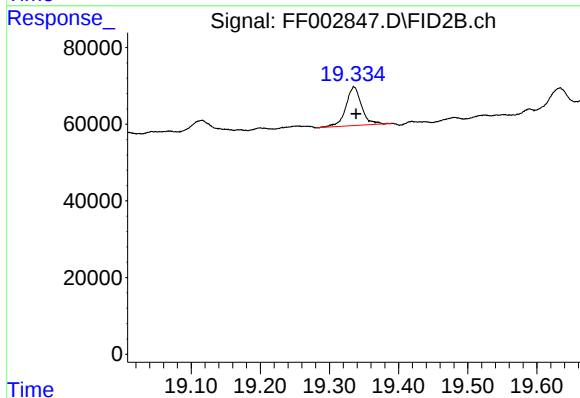


#15 N-TETRATRIACONTANE

R.T.: 19.336 min
Delta R.T.: -0.003 min
Response: 158697
Conc: 1.61 ug/ml

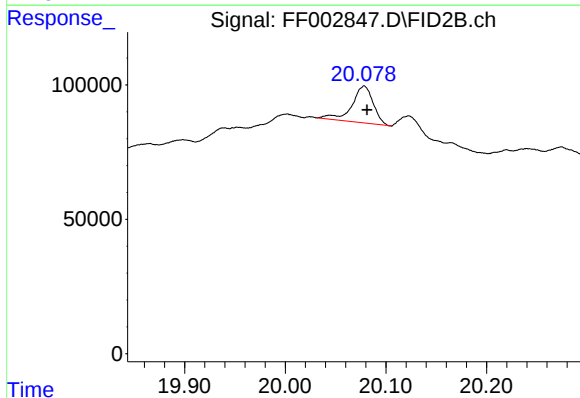


#16 N-HEXATRIACONTANE

R.T.: 20.078 min
Delta R.T.: -0.003 min
Response: 202822
Conc: 2.13 ug/ml

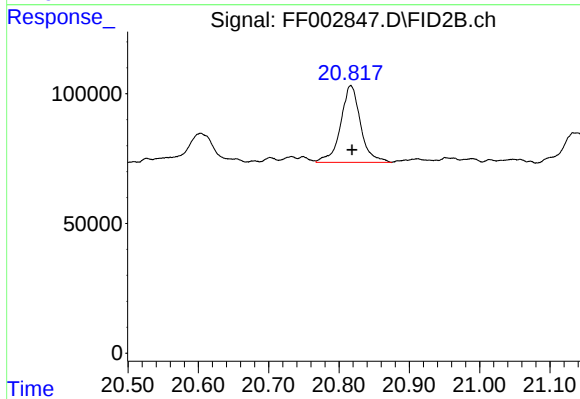

#17 N-OCTATRIACONTANE

R.T.: 20.817 min
Delta R.T.: -0.002 min
Response: 581580
Conc: 6.62 ug/ml

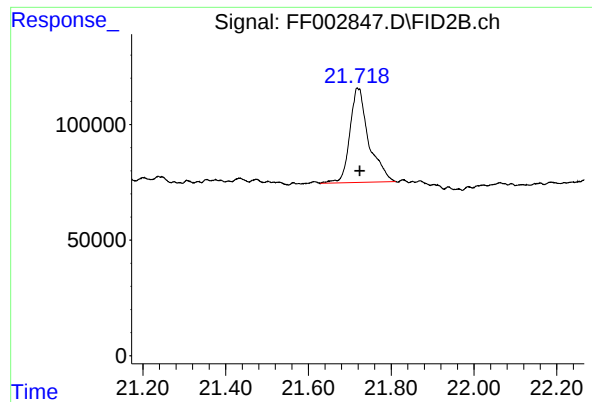

#18 N-TETRACONTANE

R.T.: 21.718 min
Delta R.T.: -0.006 min
Response: 1296708
Conc: 14.80 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER