

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002848.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 09:59
 Operator : AJ\SJ
 Sample : J6028-08 20X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 COMP-3

Integration File: autoint1.e
 Quant Time: Nov 30 11:04:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	83157	1.065 ug/ml
Target Compounds			
7) N-EICOSANE	12.592	231915	2.395 ug/ml
10) N-TETRACOSANE	14.814	97857	1.098 ug/ml
12) N-OCTACOSANE	16.823	92269	0.967 ug/ml
13) N-TRIACONTANE	17.714	127728	1.288 ug/ml
14) N-DOTRIACONTANE	18.552	251945	2.545 ug/ml
16) N-HEXATRIACONTANE	20.124	66882	0.702 ug/ml
18) N-TETRACONTANE	21.723	323455	3.693 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002848.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 09:59
Operator : AJ\SJ
Sample : J6028-08 20X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
COMP-3

Integration File: autoint1.e
Quant Time: Nov 30 11:04:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

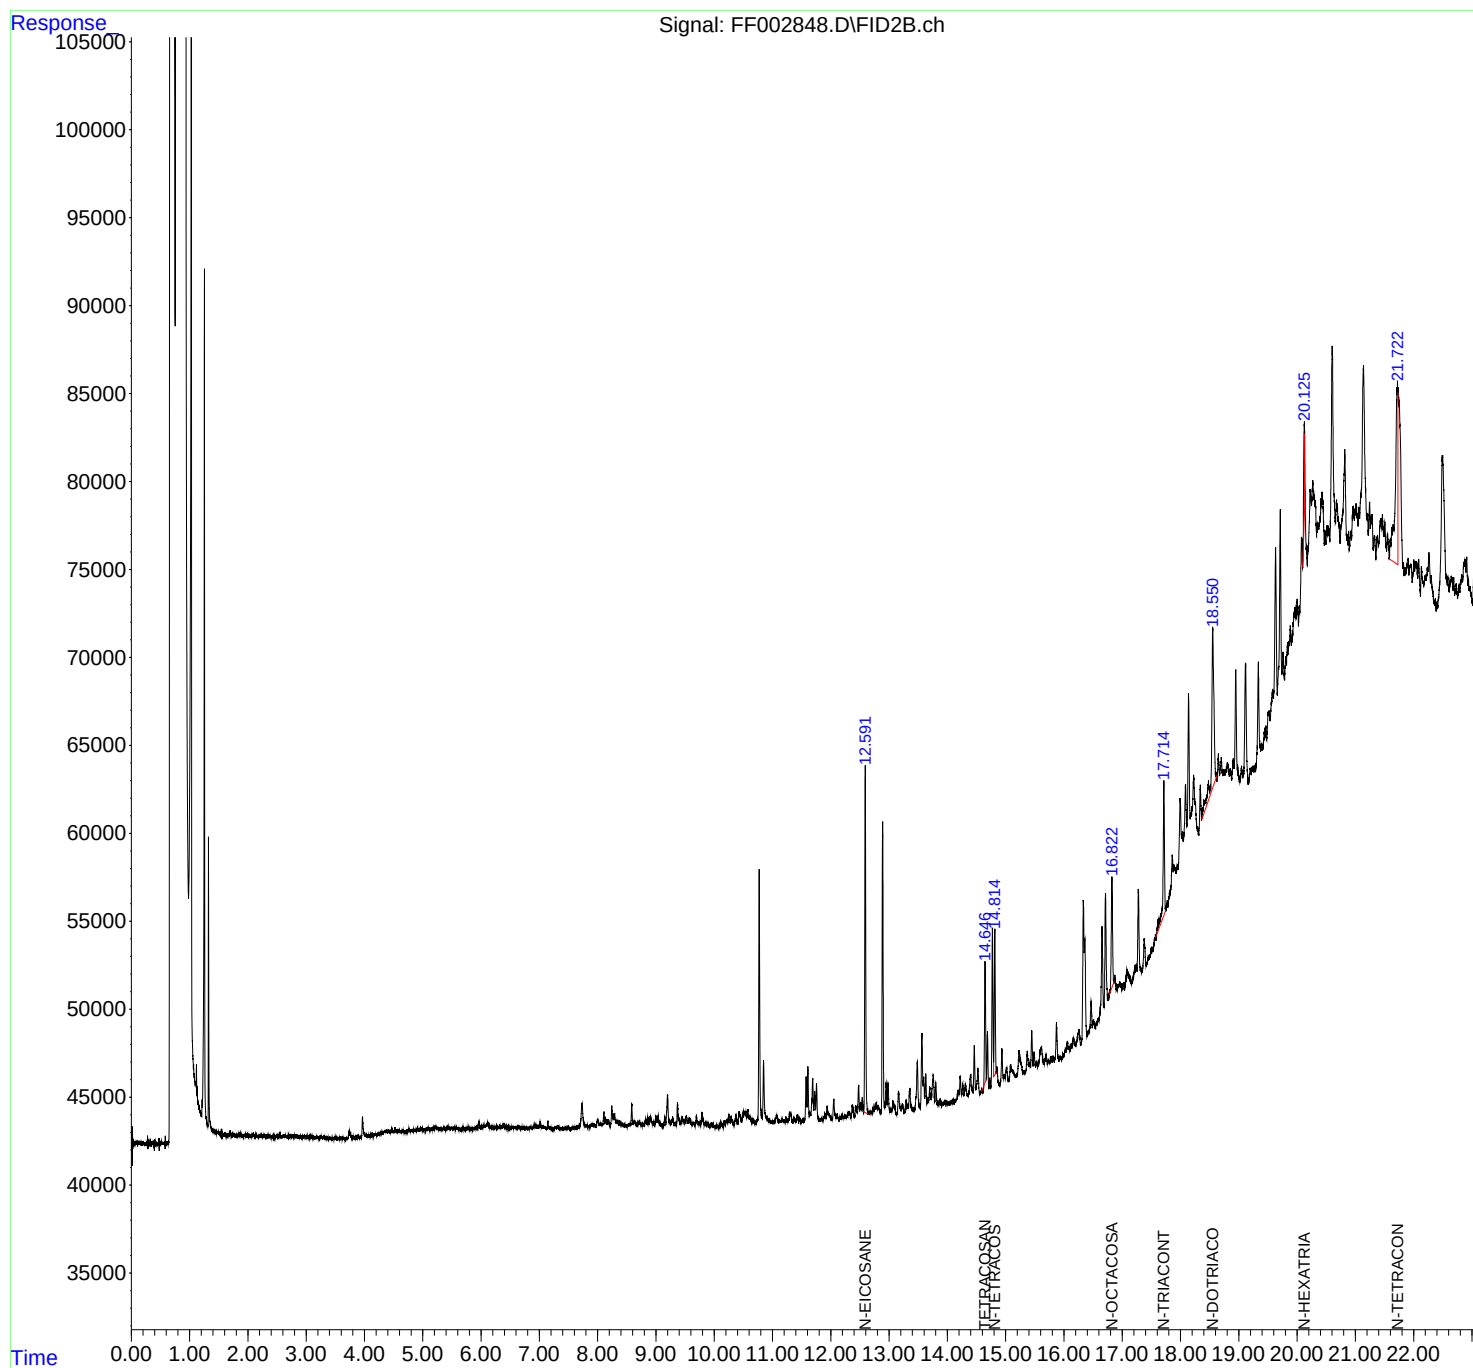


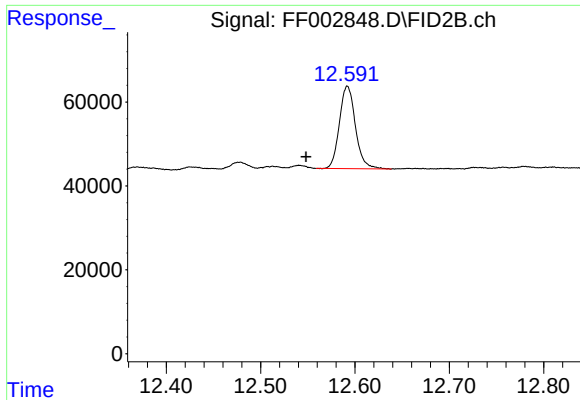

#7 N-EICOSANE


R.T.: 12.592 min
Delta R.T.: 0.044 min
Response: 231915
Conc: 2.40 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-3

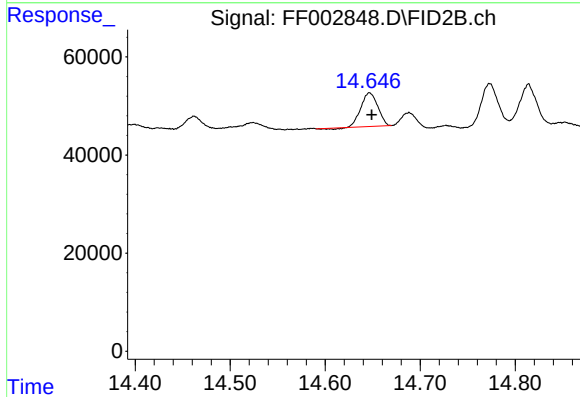


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.002 min
Response: 83157
Conc: 1.06 ug/ml

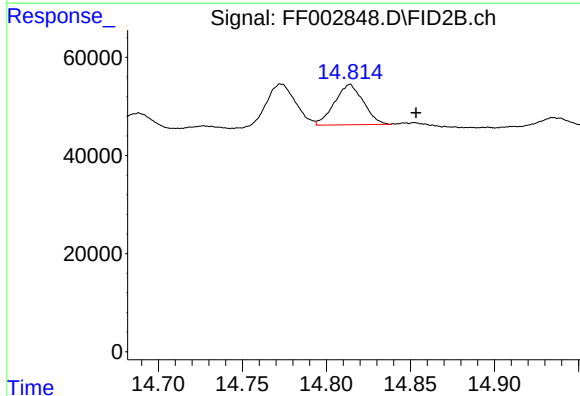


#10 N-TETRACOSANE

R.T.: 14.814 min
Delta R.T.: -0.039 min
Response: 97857
Conc: 1.10 ug/ml

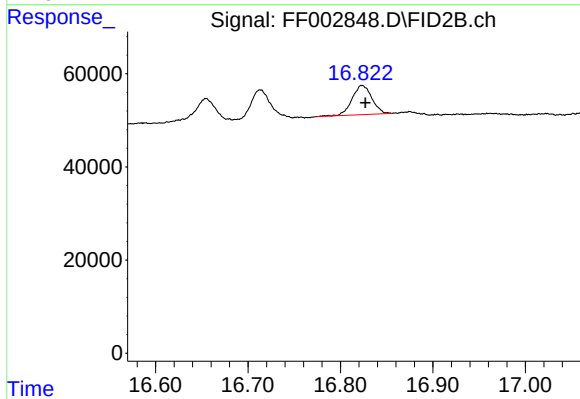

#12 N-OCTACOSANE


R.T.: 16.823 min
Delta R.T.: -0.004 min
Response: 92269
Conc: 0.97 ug/ml

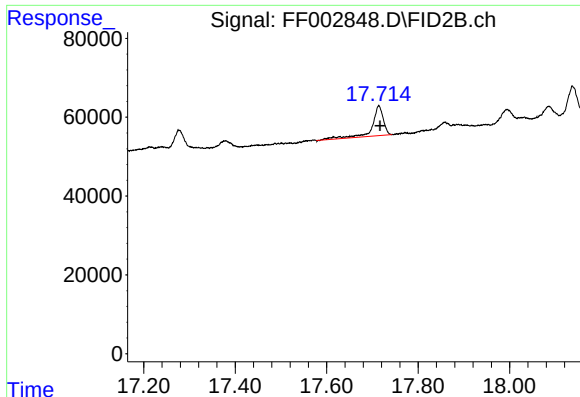

#13 N-TRIACONTANE


R.T.: 17.714 min
Delta R.T.: -0.003 min
Response: 127728
Conc: 1.29 ug/ml

Instrument :
FID_F
ClientSampleId :
COMP-3

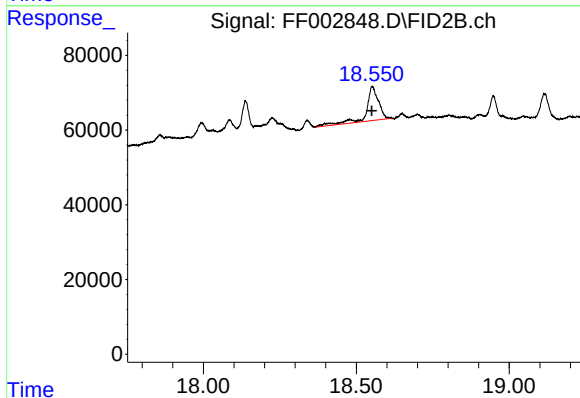


#14 N-DOTRIACONTANE

R.T.: 18.552 min
Delta R.T.: 0.000 min
Response: 251945
Conc: 2.55 ug/ml

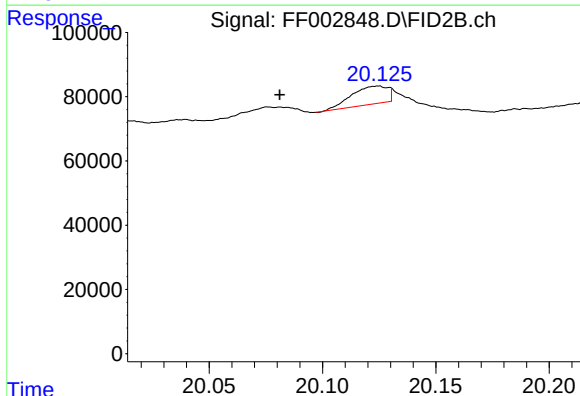

#16 N-HEXATRIACONTANE

R.T.: 20.124 min
Delta R.T.: 0.043 min
Response: 66882
Conc: 0.70 ug/ml

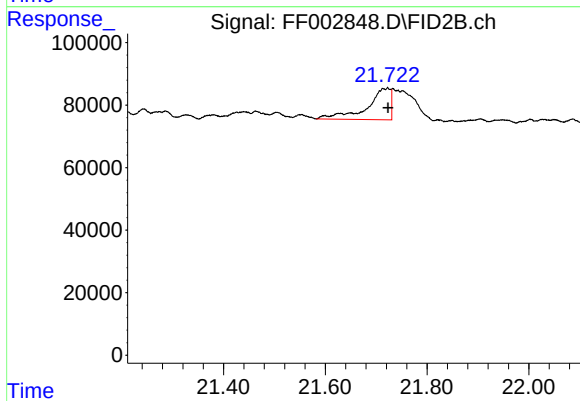

#18 N-TETRACONTANE

R.T.: 21.723 min
Delta R.T.: -0.001 min
Response: 323455
Conc: 3.69 ug/ml