

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002849.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 10:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 30 11:04:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	1663387	21.294 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.714	147322	1.486 ug/ml
14) N-DOTRIACONTANE	18.548	215756	2.179 ug/ml
15) N-TETRATRIACONTANE	19.334	135564	1.373 ug/ml
16) N-HEXATRIACONTANE	20.125	78919	0.828 ug/ml
18) N-TETRACONTANE	21.757	491660	5.613 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002849.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 10:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Nov 30 11:04:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

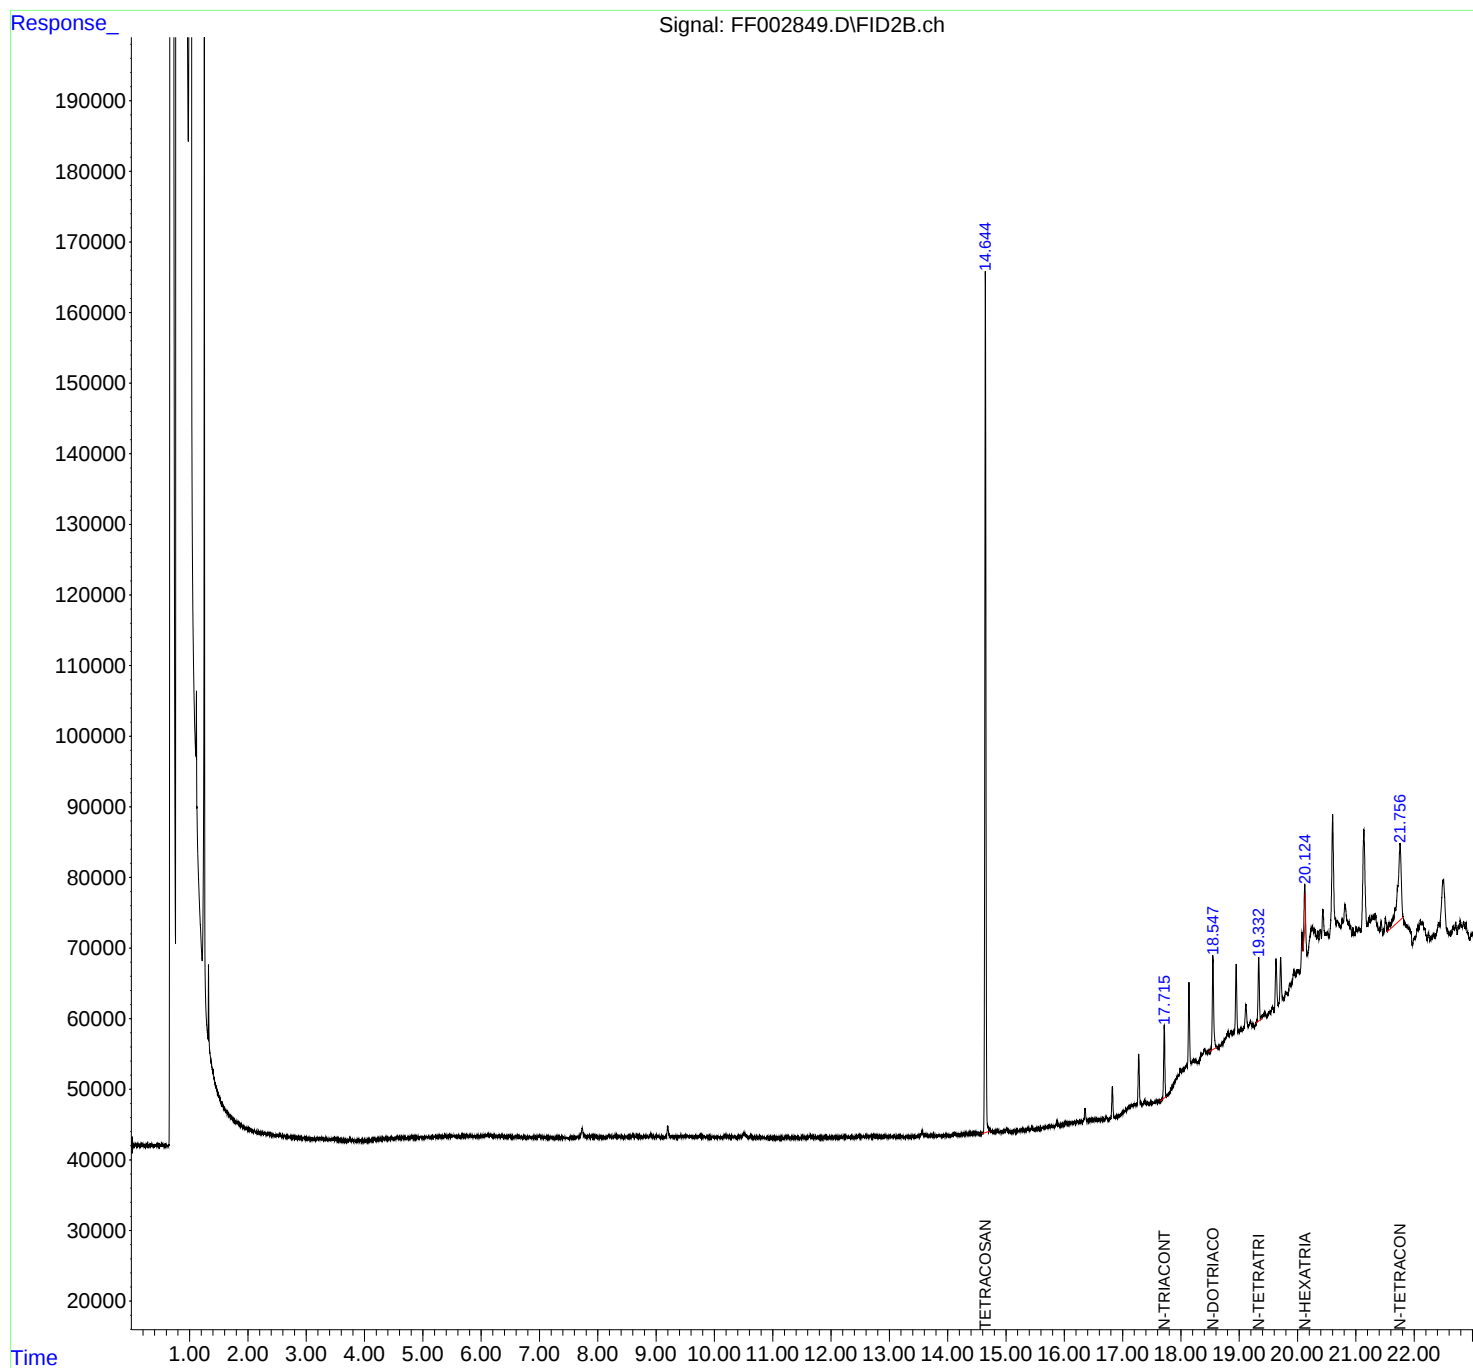


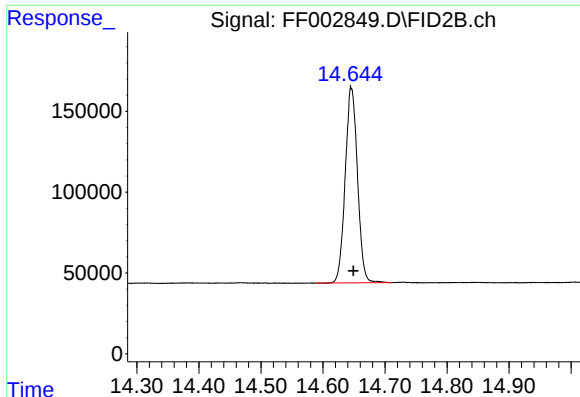

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.646 min
Delta R.T.: -0.003 min
Response: 1663387
Conc: 21.29 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

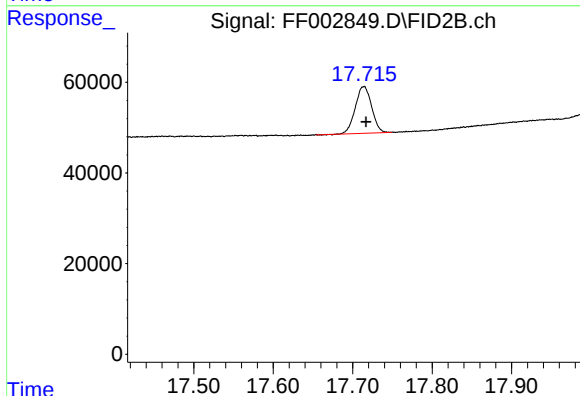


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.003 min
Response: 147322
Conc: 1.49 ug/ml

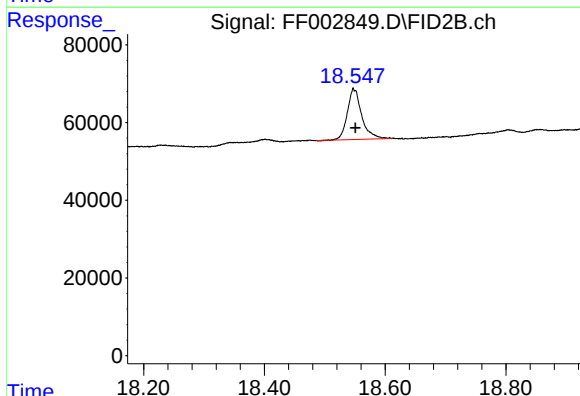


#14 N-DOTRIACONTANE

R.T.: 18.548 min
Delta R.T.: -0.003 min
Response: 215756
Conc: 2.18 ug/ml

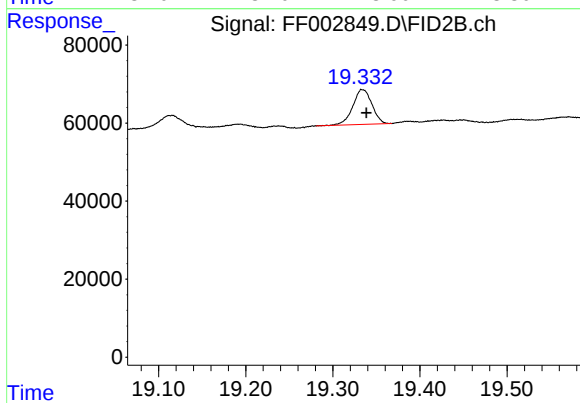

#15 N-TETRATRIACONTANE


R.T.: 19.334 min
Delta R.T.: -0.005 min
Response: 135564
Conc: 1.37 ug/ml

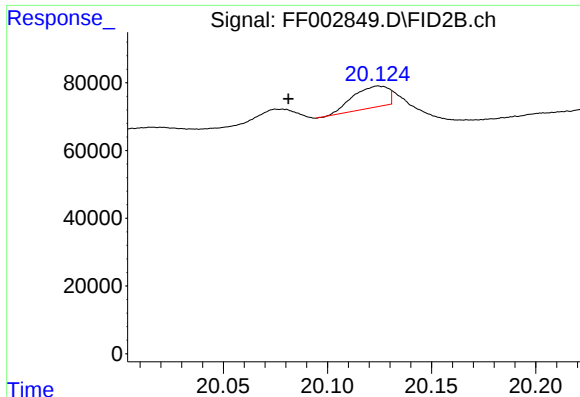

#16 N-HEXATRIACONTANE

R.T.: 20.125 min
Delta R.T.: 0.044 min
Response: 78919
Conc: 0.83 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

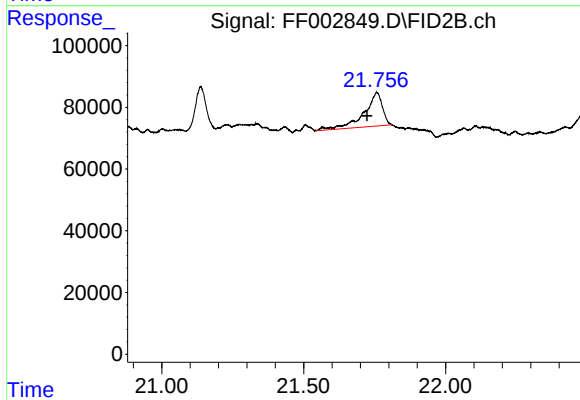

#18 N-TETRACONTANE

R.T.: 21.757 min
Delta R.T.: 0.034 min
Response: 491660
Conc: 5.61 ug/ml