

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002851.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 11:29
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Dec 01 01:25:39 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	1824591	23.357 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.826	87676	0.919 ug/ml
13) N-TRIACONTANE	17.714	207904	2.097 ug/ml
14) N-DOTRIACONTANE	18.549	302673	3.057 ug/ml
15) N-TETRATRIACONTANE	19.335	247649	2.509 ug/ml
16) N-HEXATRIACONTANE	20.078	256789	2.695 ug/ml
17) N-OCTATRIACONTANE	20.816	571363	6.501 ug/ml
18) N-TETRACONTANE	21.716	1624633	18.547 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002851.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 11:29
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Dec 01 01:25:39 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

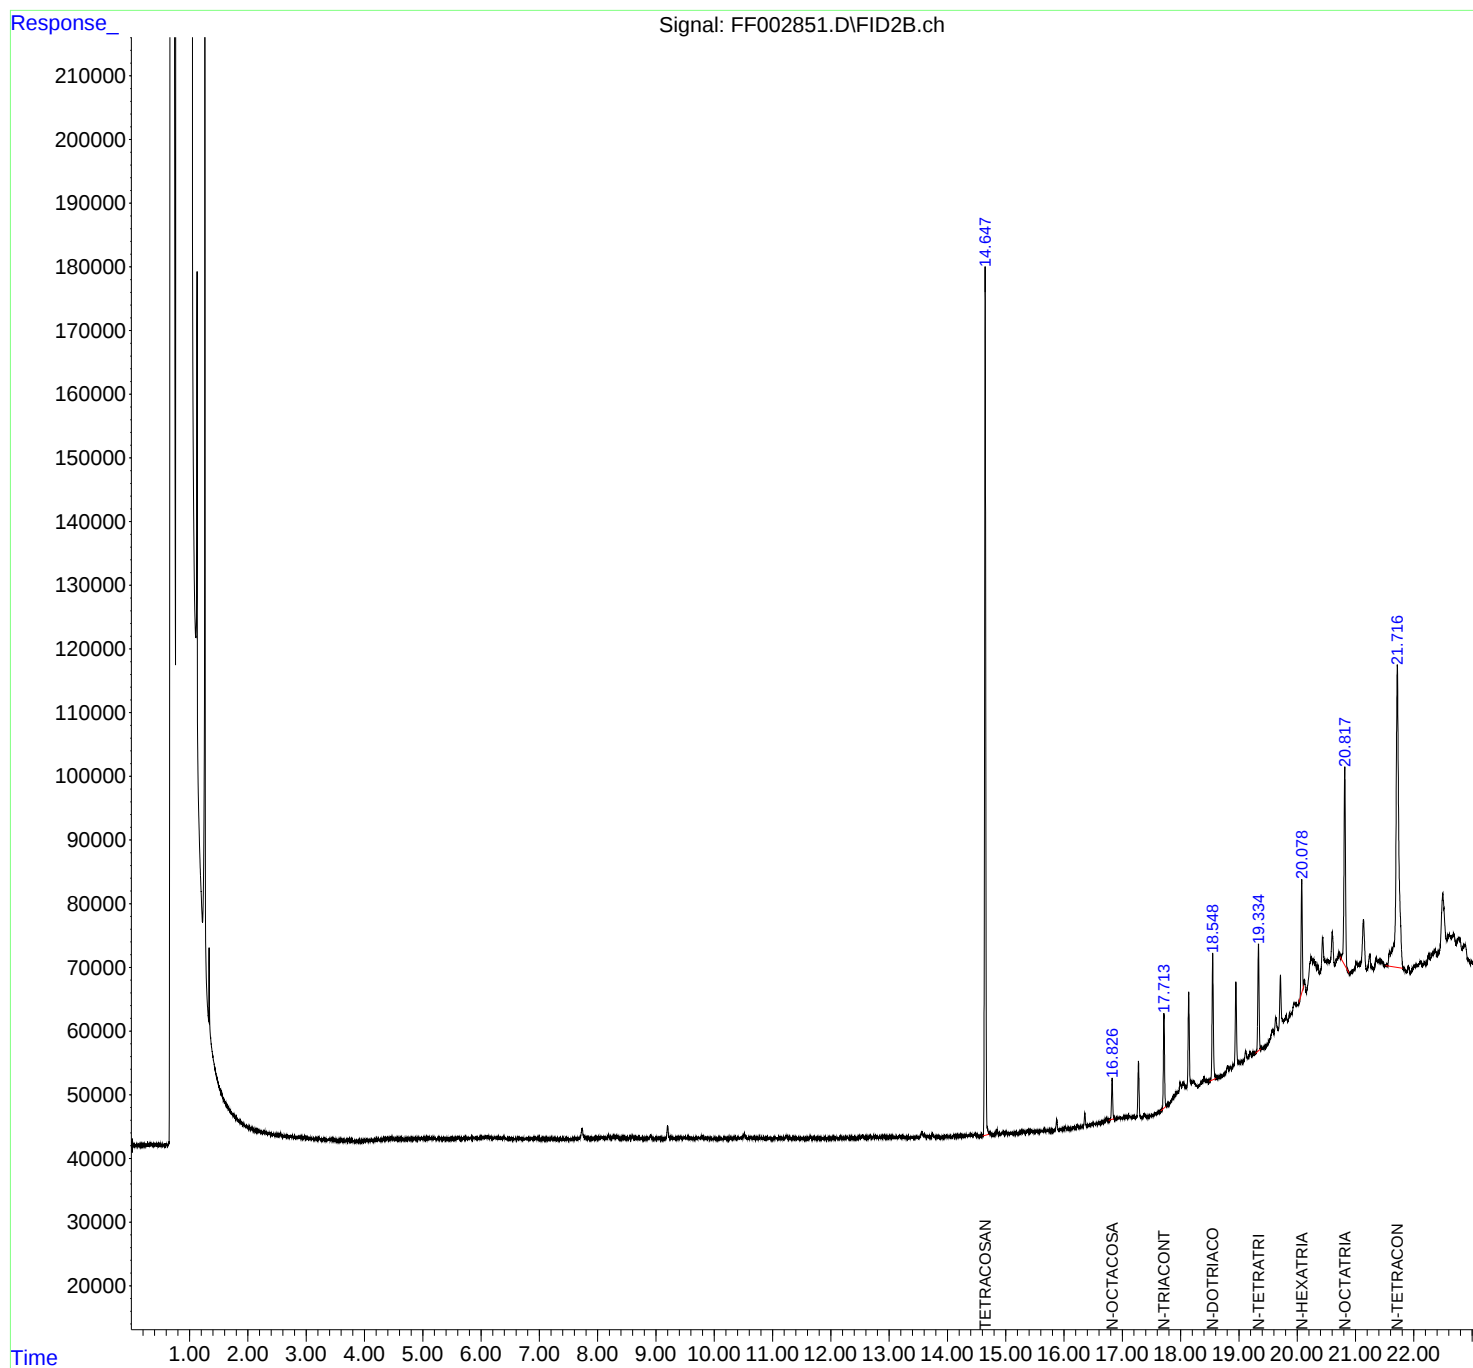


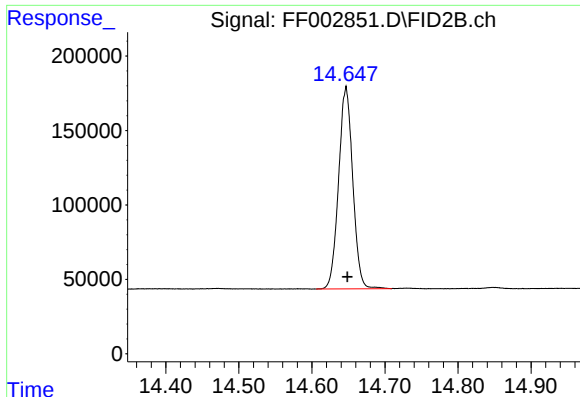

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.647 min
Delta R.T.: -0.002 min
Response: 1824591
Conc: 23.36 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

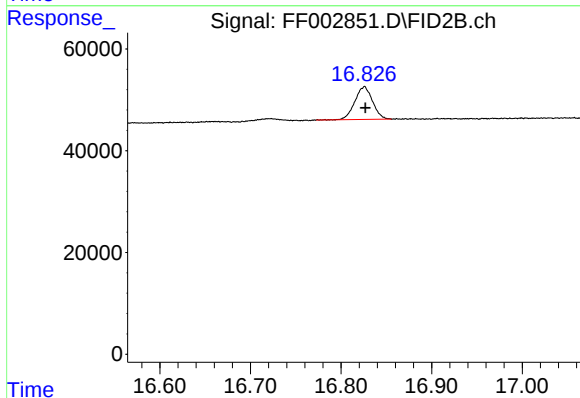


#12 N-OCTACOSANE

R.T.: 16.826 min
Delta R.T.: -0.001 min
Response: 87676
Conc: 0.92 ug/ml

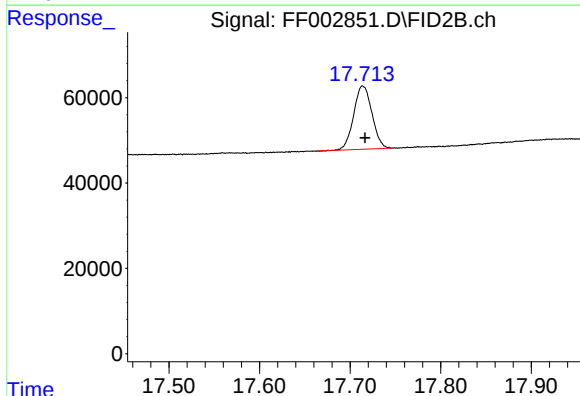


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.003 min
Response: 207904
Conc: 2.10 ug/ml

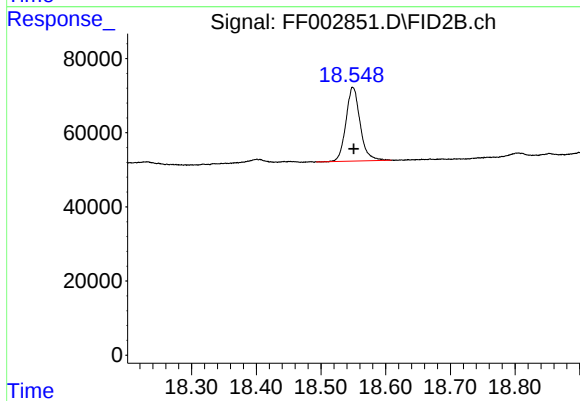

#14 N-DOTRIACONTANE


R.T.: 18.549 min
Delta R.T.: -0.001 min
Response: 302673
Conc: 3.06 ug/ml

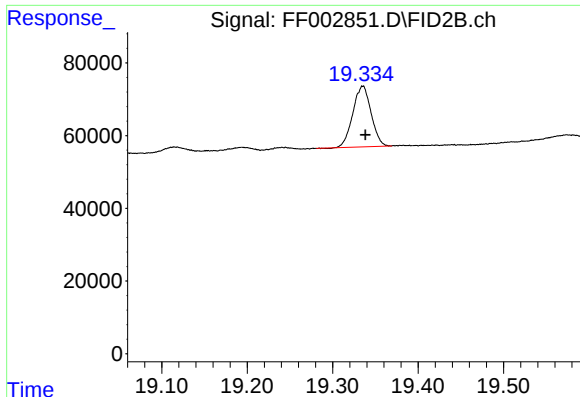

#15 N-TETRATRIACONTANE


R.T.: 19.335 min
Delta R.T.: -0.003 min
Response: 247649
Conc: 2.51 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

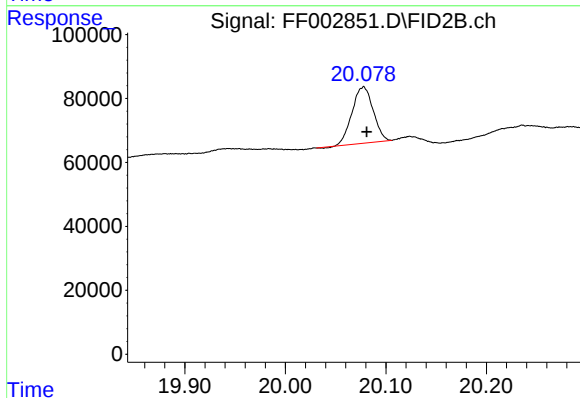


#16 N-HEXATRIACONTANE

R.T.: 20.078 min
Delta R.T.: -0.003 min
Response: 256789
Conc: 2.69 ug/ml

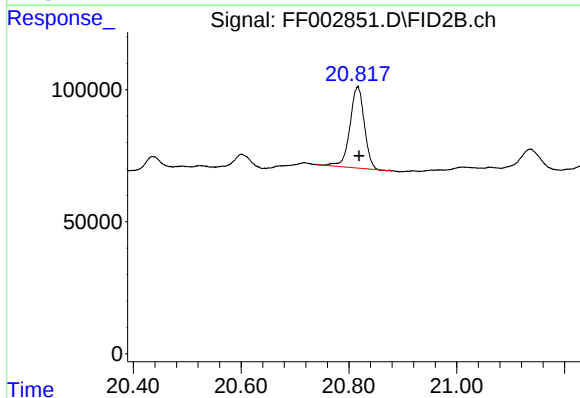

#17 N-OCTATRIACONTANE

R.T.: 20.816 min
Delta R.T.: -0.002 min
Response: 571363
Conc: 6.50 ug/ml

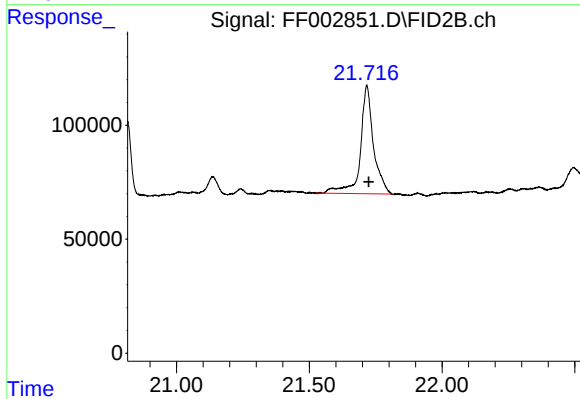

#18 N-TETRACONTANE

R.T.: 21.716 min
Delta R.T.: -0.007 min
Response: 1624633
Conc: 18.55 ug/ml