

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002857.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 14:56
 Operator : AJ\SJ
 Sample : J5770-13 2X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 OR-03-112918-A

Integration File: autoint1.e
 Quant Time: Dec 01 01:27:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	975159	12.483 ug/ml
Target Compounds			
4) N-TETRADECANE	8.185	120751	1.045 ug/ml
5) N-HEXADECANE	9.787	142027	1.299 ug/ml
6) N-OCTADECANE	11.230	95174	0.917 ug/ml
7) N-EICOSANE	12.542	125853	1.300 ug/ml
8) N-DOCOSANE	13.757	276916	3.025 ug/ml
10) N-TETRACOSANE	14.814	1021926	11.471 ug/ml
11) N-HEXACOSANE	15.875	157875	1.740 ug/ml
12) N-OCTACOSANE	16.818	470108	4.929 ug/ml
13) N-TRIACONTANE	17.714	389619	3.930 ug/ml
14) N-DOTRIACONTANE	18.545	342686	3.462 ug/ml
15) N-TETRATRIACONTANE	19.335	25109	0.254 ug/ml
18) N-TETRACONTANE	21.715	201056	2.295 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002857.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 14:56
Operator : AJ\SJ
Sample : J5770-13 2X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A

Integration File: autoint1.e
Quant Time: Dec 01 01:27:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

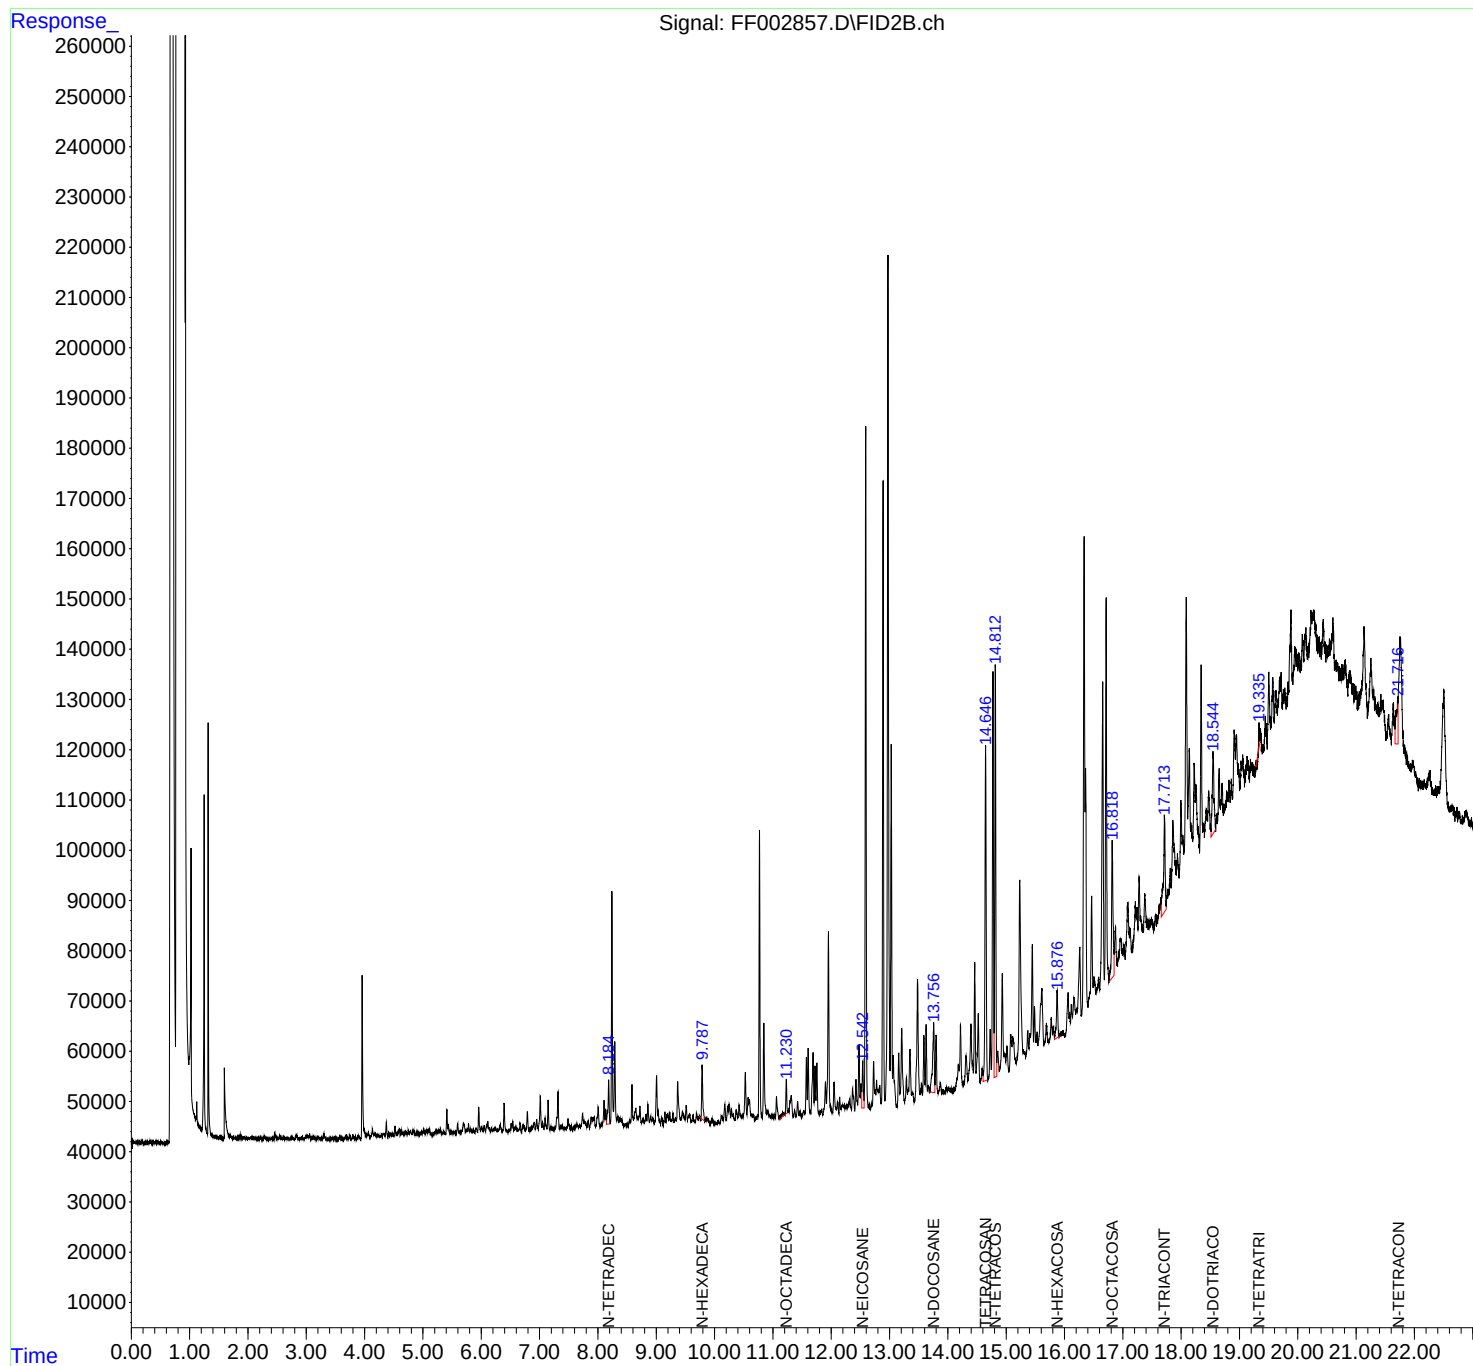


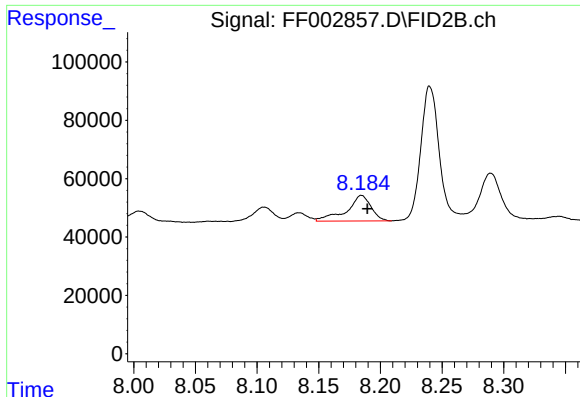

#4 N-TETRADECANE


R.T.: 8.185 min
Delta R.T.: -0.005 min
Response: 120751
Conc: 1.05 ug/ml

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A

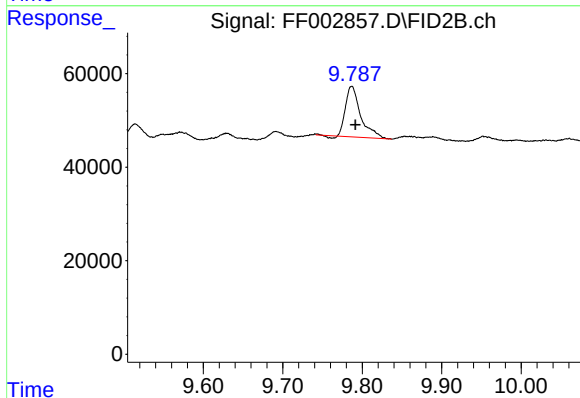


#5 N-HEXADECANE

R.T.: 9.787 min
Delta R.T.: -0.005 min
Response: 142027
Conc: 1.30 ug/ml

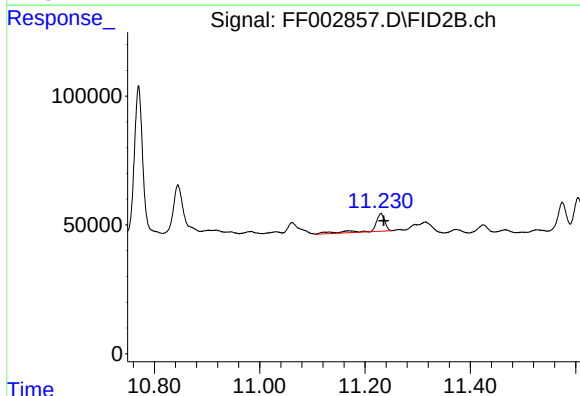


#6 N-OCTADECANE

R.T.: 11.230 min
Delta R.T.: -0.005 min
Response: 95174
Conc: 0.92 ug/ml

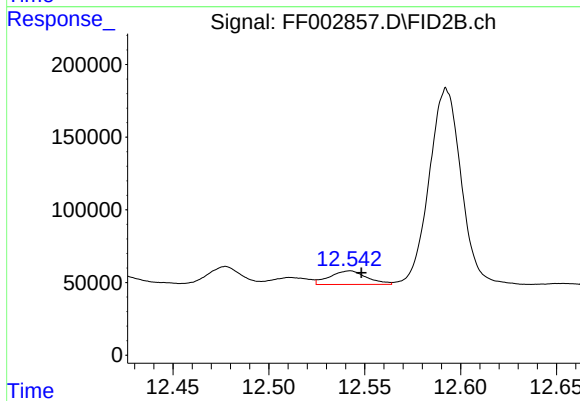

#7 N-EICOSANE


R.T.: 12.542 min
Delta R.T.: -0.006 min
Response: 125853
Conc: 1.30 ug/ml

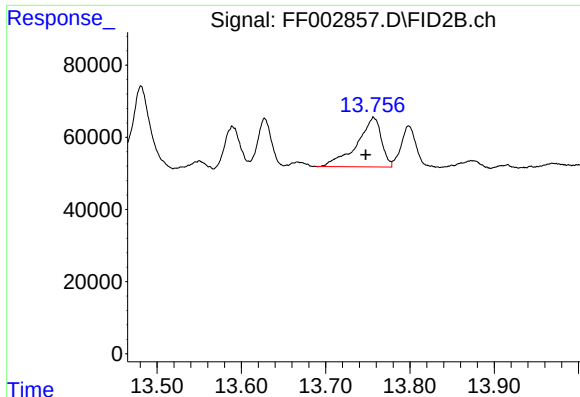

#8 N-DOCOSANE


R.T.: 13.757 min
Delta R.T.: 0.009 min
Response: 276916
Conc: 3.02 ug/ml

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A

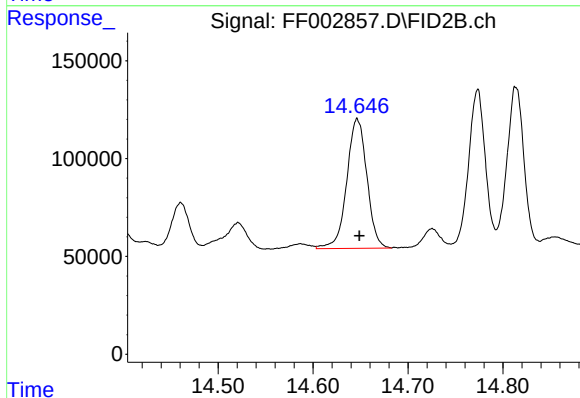


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.002 min
Response: 975159
Conc: 12.48 ug/ml

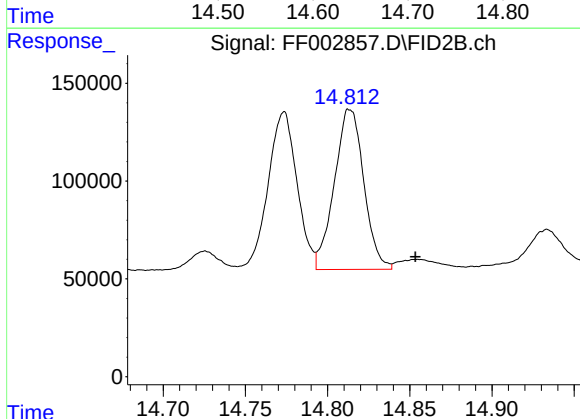


#10 N-TETRACOSANE

R.T.: 14.814 min
Delta R.T.: -0.040 min
Response: 1021926
Conc: 11.47 ug/ml

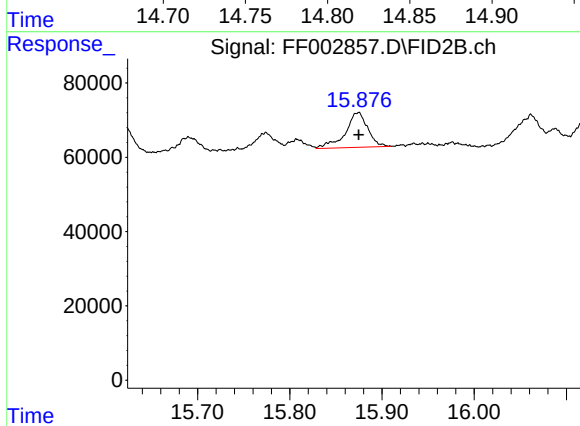

#11 N-HEXACOSANE


R.T.: 15.875 min
Delta R.T.: 0.000 min
Response: 157875
Conc: 1.74 ug/ml

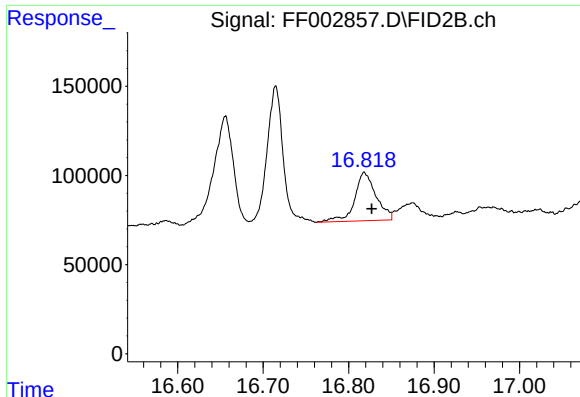

#12 N-OCTACOSANE


R.T.: 16.818 min
Delta R.T.: -0.009 min
Response: 470108
Conc: 4.93 ug/ml

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A

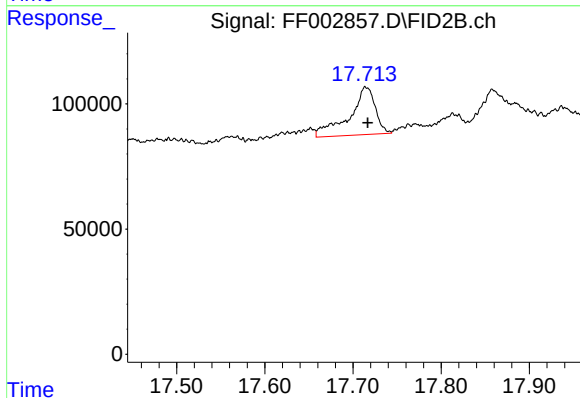


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.003 min
Response: 389619
Conc: 3.93 ug/ml

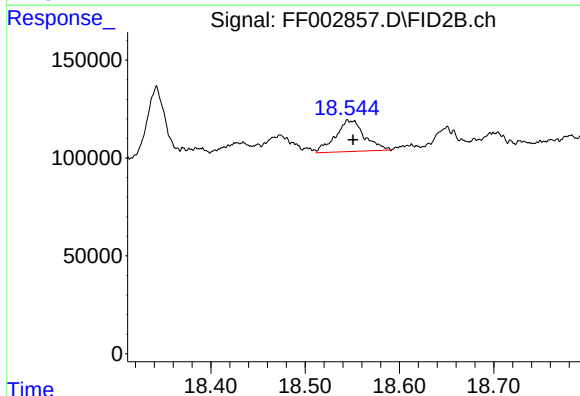


#14 N-DOTRIACONTANE

R.T.: 18.545 min
Delta R.T.: -0.005 min
Response: 342686
Conc: 3.46 ug/ml

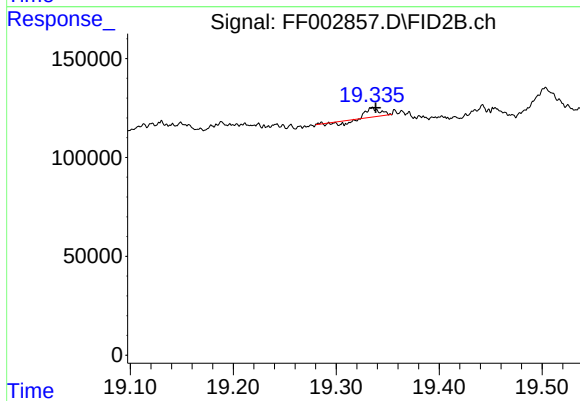

#15 N-TETRATRIACONTANE

R.T.: 19.335 min
Delta R.T.: -0.004 min
Response: 25109
Conc: 0.25 ug/ml

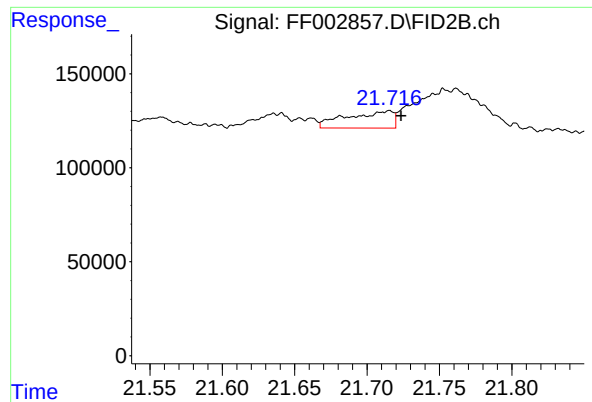

#18 N-TETRACONTANE

R.T.: 21.715 min
Delta R.T.: -0.008 min
Response: 201056
Conc: 2.30 ug/ml

Instrument :
FID_F
ClientSampleId :
OR-03-112918-A