

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002860.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 16:27
 Operator : AJ\SJ
 Sample : J5761-03 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 AU-05-112918

Integration File: autoint1.e
 Quant Time: Dec 01 01:28:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	1253115	16.042 ug/ml
Target Compounds			
4) N-TETRADECANE	8.241f	385814	3.340 ug/ml
5) N-HEXADECANE	9.791	110643	1.012 ug/ml
7) N-EICOSANE	12.600f	7283384	75.223 ug/ml
8) N-DOCOSANE	13.759	299927	3.276 ug/ml
10) N-TETRACOSANE	14.819	3267224	36.674 ug/ml
11) N-HEXACOSANE	15.874	275344	3.034 ug/ml
12) N-OCTACOSANE	16.820	1093093	11.460 ug/ml
13) N-TRIACONTANE	17.714	548295	5.531 ug/ml
14) N-DOTRIACONTANE	18.545	375886	3.797 ug/ml
16) N-HEXATRIACONTANE	20.023f	41122	0.432 ug/ml
18) N-TETRACONTANE	21.723	218609	2.496 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002860.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 16:27
Operator : AJ\SJ
Sample : J5761-03 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
AU-05-112918

Integration File: autoint1.e
Quant Time: Dec 01 01:28:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

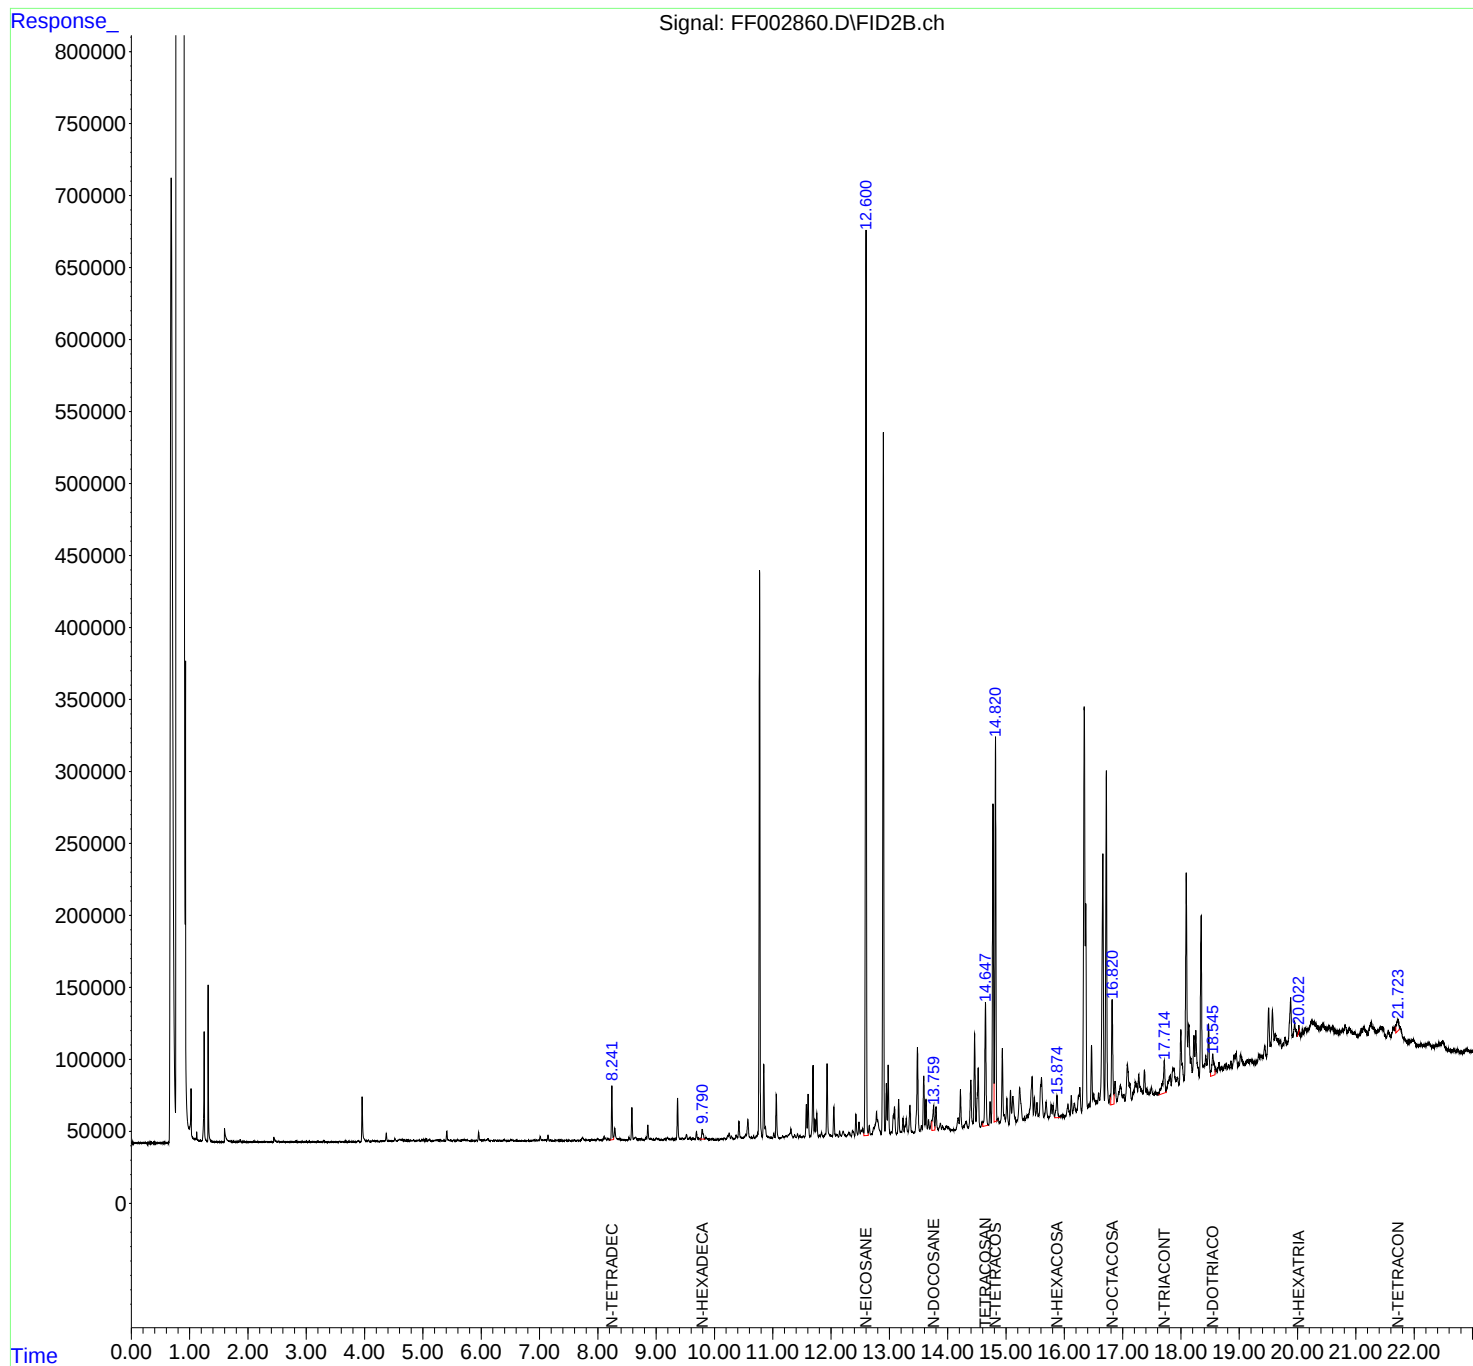


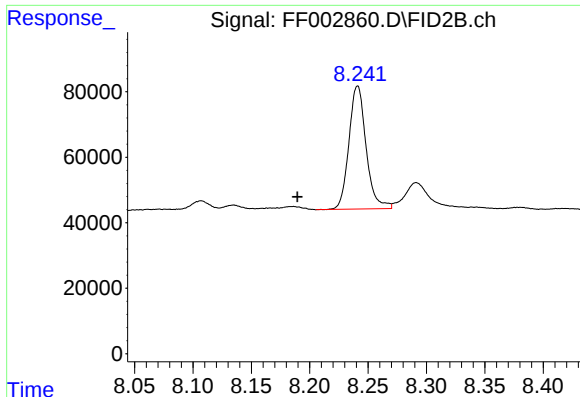

#4 N-TETRADECANE


R.T.: 8.241 min
Delta R.T.: 0.051 min
Response: 385814
Conc: 3.34 ug/ml

Instrument :
FID_F
ClientSampleId :
AU-05-112918

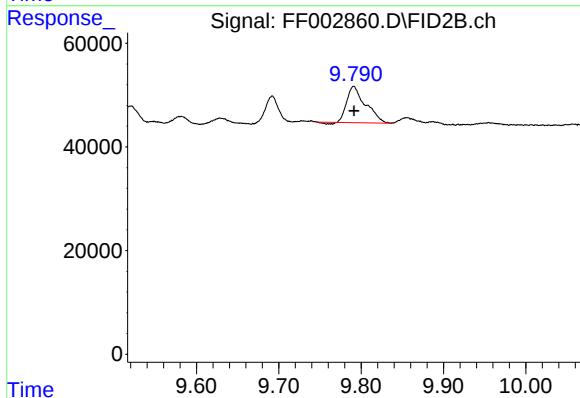


#5 N-HEXADECANE

R.T.: 9.791 min
Delta R.T.: 0.000 min
Response: 110643
Conc: 1.01 ug/ml

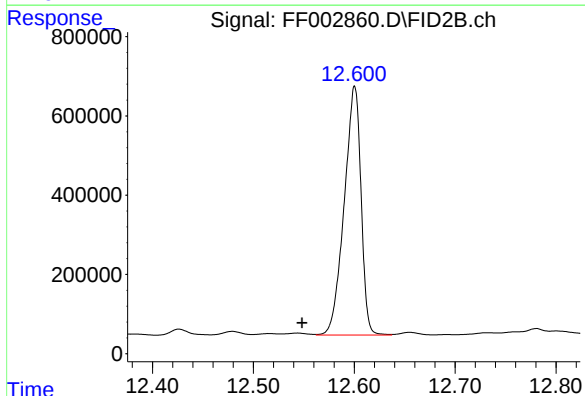


#7 N-EICOSANE

R.T.: 12.600 min
Delta R.T.: 0.052 min
Response: 7283384
Conc: 75.22 ug/ml

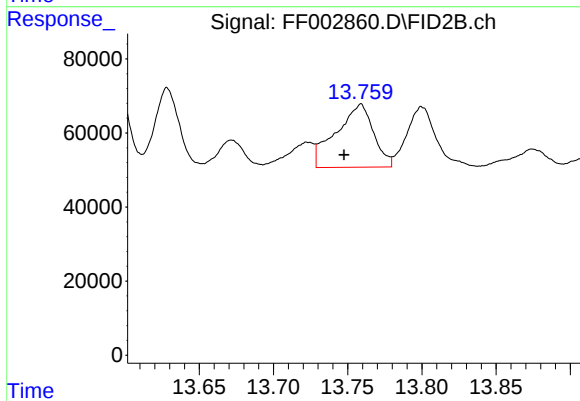

#8 N-DOCOSANE


R.T.: 13.759 min
Delta R.T.: 0.011 min
Response: 299927
Conc: 3.28 ug/ml

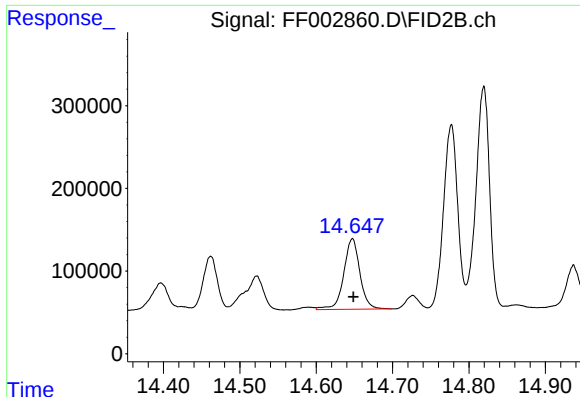

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.647 min
Delta R.T.: -0.001 min
Response: 1253115
Conc: 16.04 ug/ml

Instrument :
FID_F
ClientSampleId :
AU-05-112918

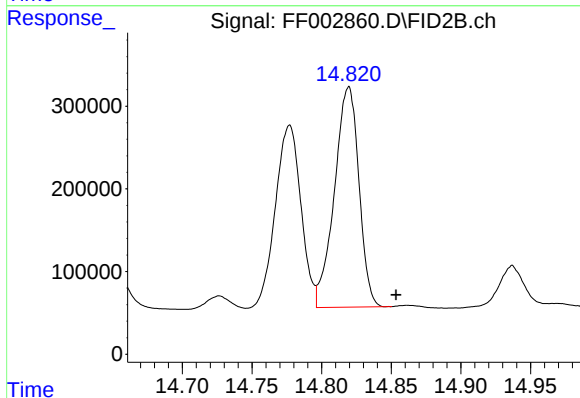


#10 N-TETRACOSANE

R.T.: 14.819 min
Delta R.T.: -0.034 min
Response: 3267224
Conc: 36.67 ug/ml

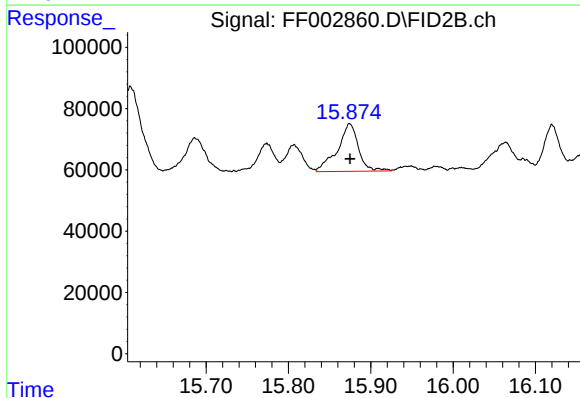


#11 N-HEXACOSANE

R.T.: 15.874 min
Delta R.T.: 0.000 min
Response: 275344
Conc: 3.03 ug/ml

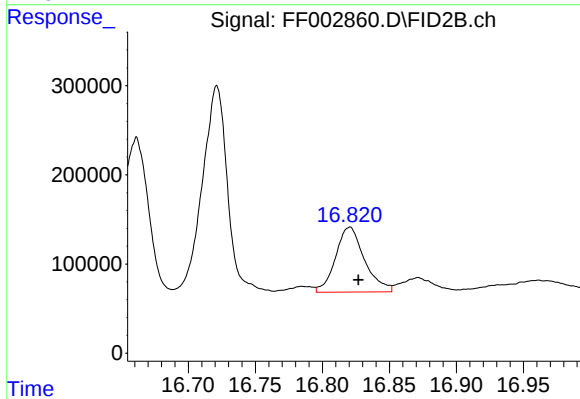

#12 N-OCTACOSANE


R.T.: 16.820 min
Delta R.T.: -0.007 min
Response: 1093093
Conc: 11.46 ug/ml

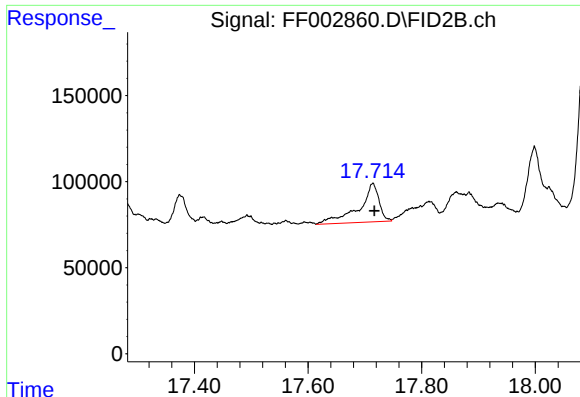

#13 N-TRIACONTANE


R.T.: 17.714 min
Delta R.T.: -0.003 min
Response: 548295
Conc: 5.53 ug/ml

Instrument :
FID_F
ClientSampleId :
AU-05-112918

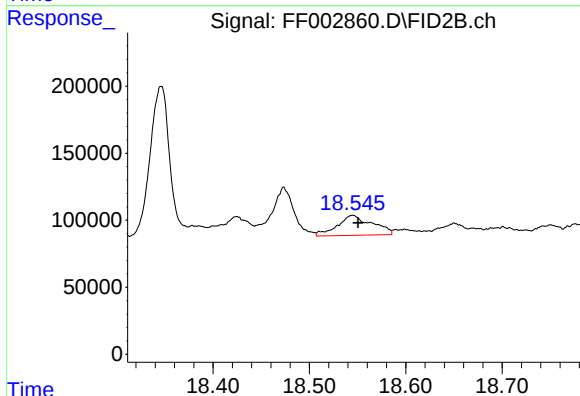


#14 N-DOTRIACONTANE

R.T.: 18.545 min
Delta R.T.: -0.006 min
Response: 375886
Conc: 3.80 ug/ml

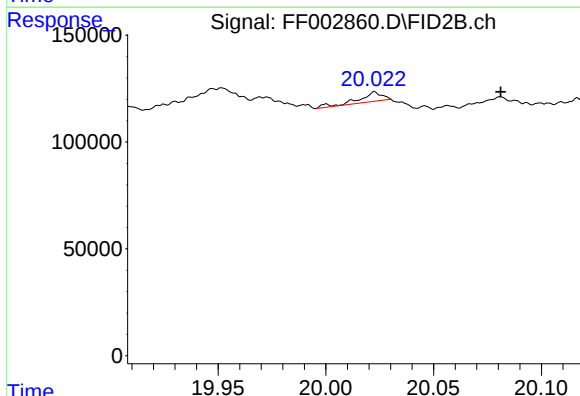

#16 N-HEXATRIACONTANE

R.T.: 20.023 min
Delta R.T.: -0.058 min
Response: 41122
Conc: 0.43 ug/ml

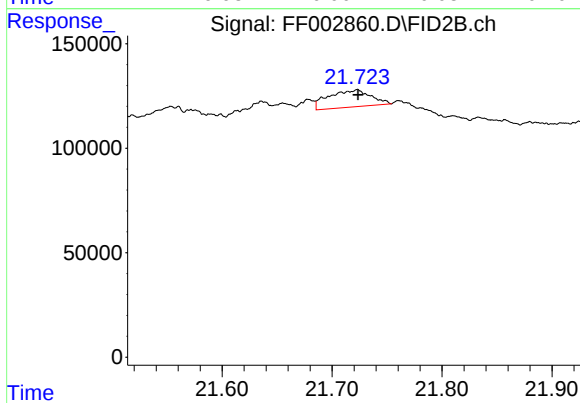

#18 N-TETRACONTANE

R.T.: 21.723 min
Delta R.T.: 0.000 min
Response: 218609
Conc: 2.50 ug/ml