

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002861.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 17:59
 Operator : AJ\SJ
 Sample : J5771-07 10X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 EO-02-112918-A

Integration File: autoint1.e
 Quant Time: Dec 01 01:28:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	133236	1.706 ug/ml
Target Compounds			
3) N-DODECANE	6.392	125921	1.039 ug/ml
4) N-TETRADECANE	8.185	186799	1.617 ug/ml
5) N-HEXADECANE	9.787	211428	1.934 ug/ml
6) N-OCTADECANE	11.230	145615	1.403 ug/ml
7) N-EICOSANE	12.543	138272	1.428 ug/ml
8) N-DOCOSANE	13.745	78057	0.853 ug/ml
10) N-TETRACOSANE	14.813	113261	1.271 ug/ml
11) N-HEXACOSANE	15.872	94817	1.045 ug/ml
12) N-OCTACOSANE	16.823	125458	1.315 ug/ml
13) N-TRIACONTANE	17.714	231154	2.332 ug/ml
14) N-DOTRIACONTANE	18.548	240978	2.434 ug/ml
15) N-TETRATRIACONTANE	19.336	108805	1.102 ug/ml
16) N-HEXATRIACONTANE	20.080	80757	0.847 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002861.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 17:59
Operator : AJ\SJ
Sample : J5771-07 10X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
EO-02-112918-A

Integration File: autoint1.e
Quant Time: Dec 01 01:28:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

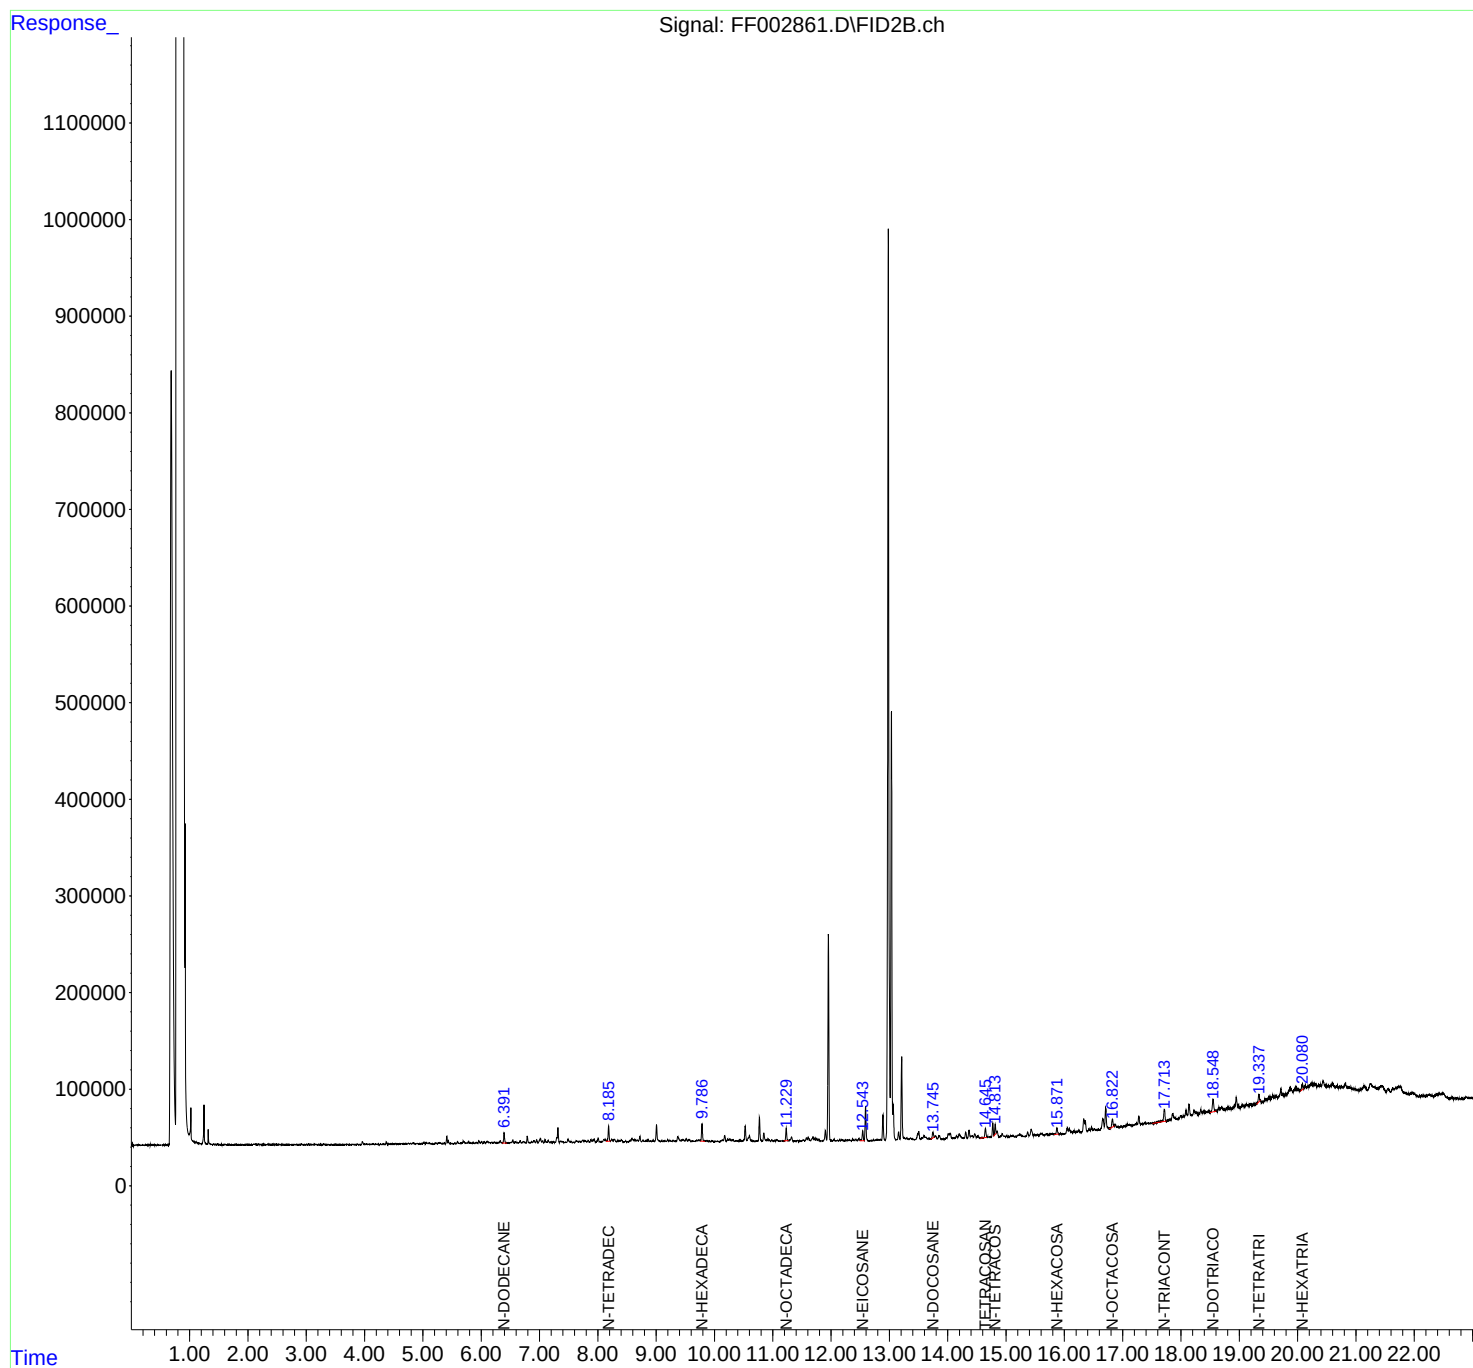


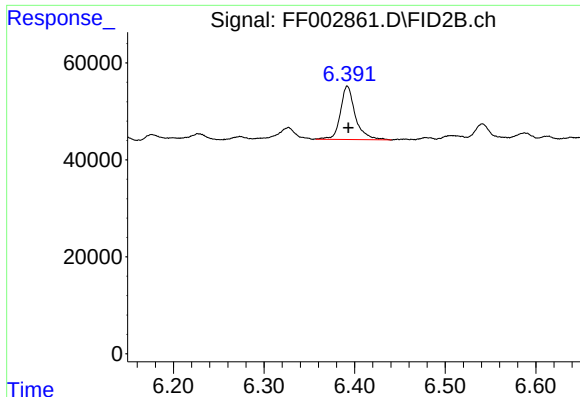

#3 N-DODECANE


R.T.: 6.392 min
Delta R.T.: -0.001 min
Response: 125921
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-02-112918-A

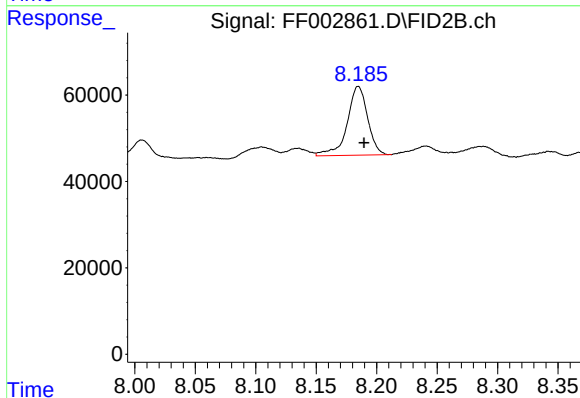


#4 N-TETRADECANE

R.T.: 8.185 min
Delta R.T.: -0.005 min
Response: 186799
Conc: 1.62 ug/ml

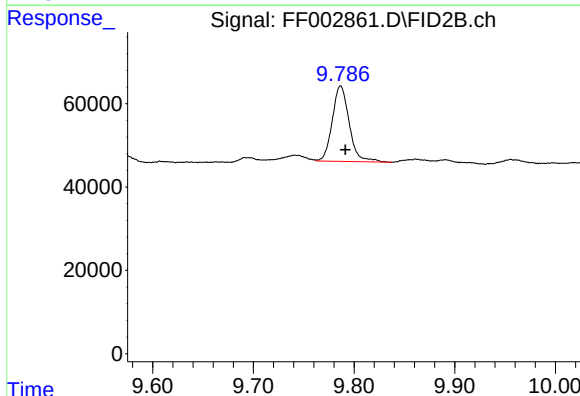


#5 N-HEXADECANE

R.T.: 9.787 min
Delta R.T.: -0.005 min
Response: 211428
Conc: 1.93 ug/ml

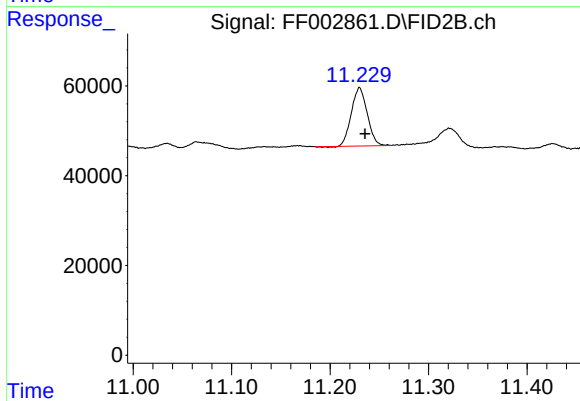

#6 N-OCTADECANE


R.T.: 11.230 min
Delta R.T.: -0.006 min
Response: 145615
Conc: 1.40 ug/ml

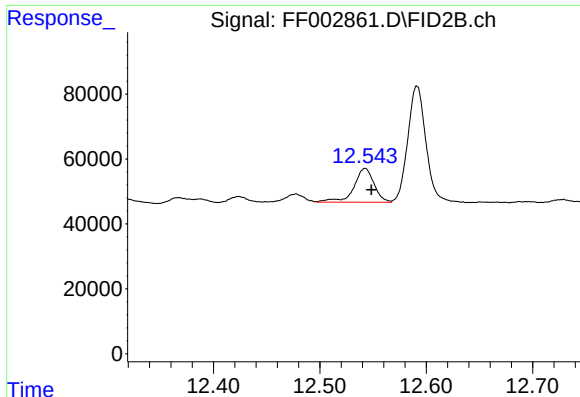

#7 N-EICOSANE


R.T.: 12.543 min
Delta R.T.: -0.006 min
Response: 138272
Conc: 1.43 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-02-112918-A

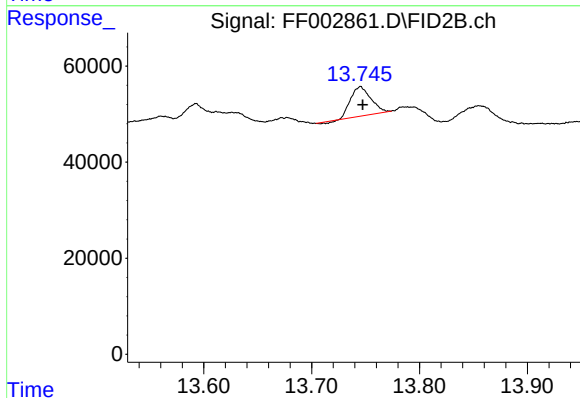


#8 N-DOCOSANE

R.T.: 13.745 min
Delta R.T.: -0.002 min
Response: 78057
Conc: 0.85 ug/ml

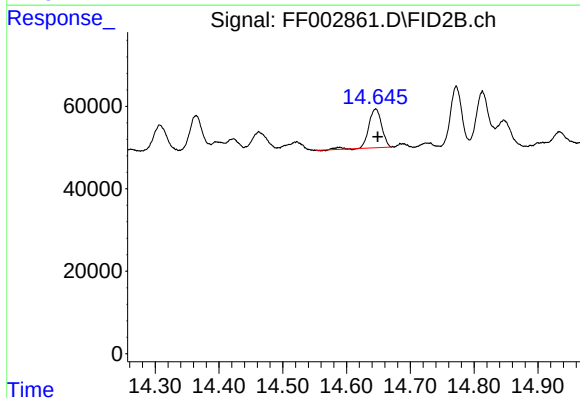


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.646 min
Delta R.T.: -0.003 min
Response: 133236
Conc: 1.71 ug/ml

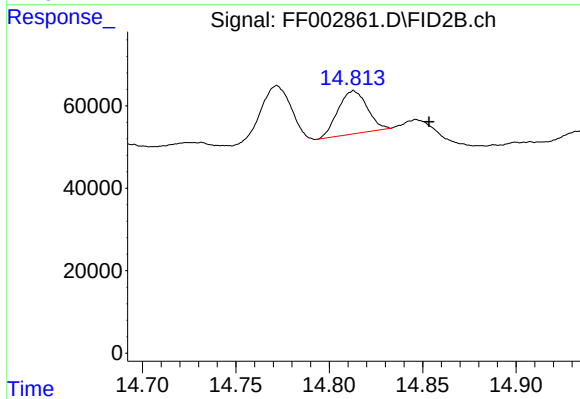

#10 N-TETRACOSANE


R.T.: 14.813 min
Delta R.T.: -0.040 min
Response: 113261
Conc: 1.27 ug/ml

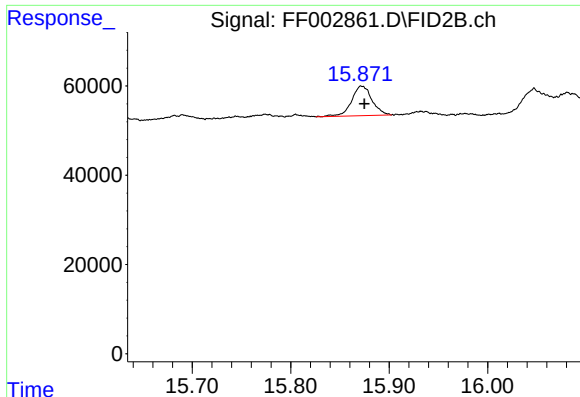

#11 N-HEXACOSANE


R.T.: 15.872 min
Delta R.T.: -0.003 min
Response: 94817
Conc: 1.04 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-02-112918-A

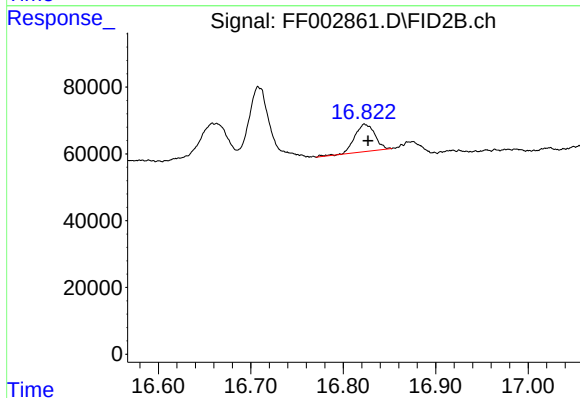


#12 N-OCTACOSANE

R.T.: 16.823 min
Delta R.T.: -0.004 min
Response: 125458
Conc: 1.32 ug/ml

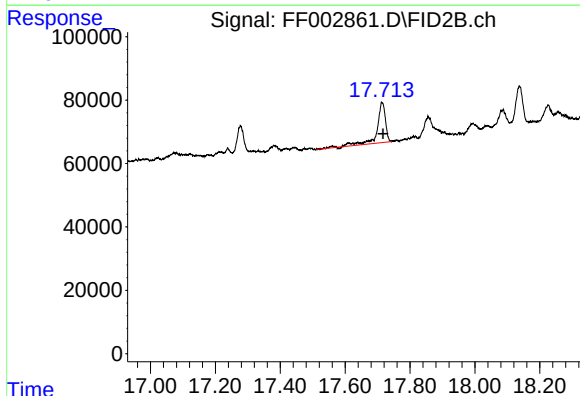


#13 N-TRIACONTANE

R.T.: 17.714 min
Delta R.T.: -0.003 min
Response: 231154
Conc: 2.33 ug/ml

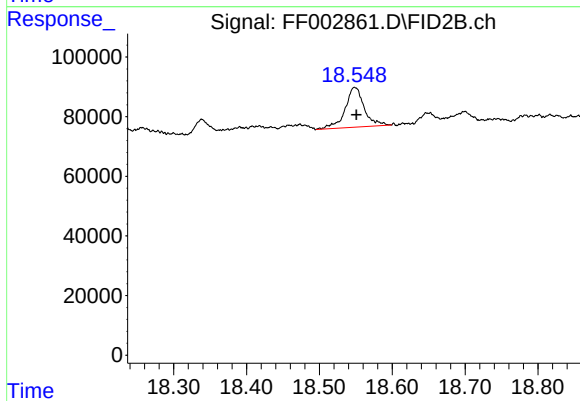

#14 N-DOTRIACONTANE


R.T.: 18.548 min
Delta R.T.: -0.002 min
Response: 240978
Conc: 2.43 ug/ml

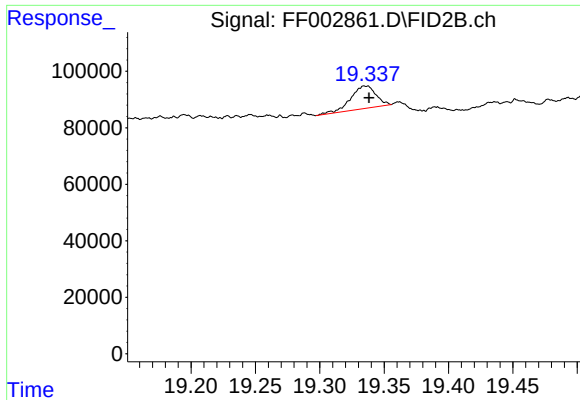

#15 N-TETRATRIACONTANE

R.T.: 19.336 min
Delta R.T.: -0.003 min
Response: 108805
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :
EO-02-112918-A

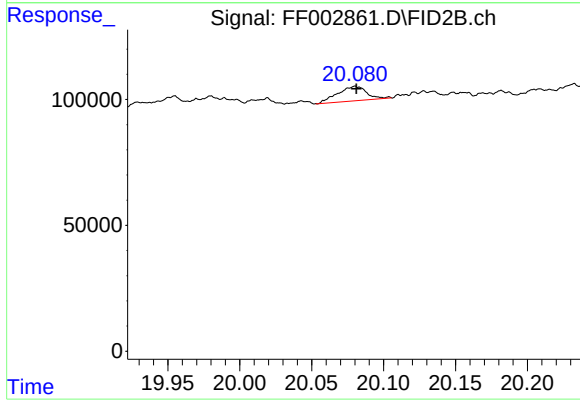

#16 N-HEXATRIACONTANE

R.T.: 20.080 min
Delta R.T.: 0.000 min
Response: 80757
Conc: 0.85 ug/ml