

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002862.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 18:30
 Operator : AJ\SJ
 Sample : J6134-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MW-11

Integration File: autoint1.e
 Quant Time: Dec 01 01:28:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.647	2038318	26.093 ug/ml
Target Compounds			
2) N-DECANE	4.371	1089097	8.720 ug/ml
3) N-DODECANE	6.391	2281776	18.826 ug/ml
4) N-TETRADECANE	8.186	2636540	22.824 ug/ml
5) N-HEXADECANE	9.794	1966318	17.984 ug/ml
6) N-OCTADECANE	11.232	1889520	18.203 ug/ml
7) N-EICOSANE	12.546	1555130	16.061 ug/ml
11) N-HEXACOSANE	15.874	95194	1.049 ug/ml
12) N-OCTACOSANE	16.824	360791	3.783 ug/ml
13) N-TRIACONTANE	17.715	511978	5.164 ug/ml
14) N-DOTRIACONTANE	18.548	367639	3.714 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002862.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 18:30
Operator : AJ\SJ
Sample : J6134-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MW-11

Integration File: autoint1.e
Quant Time: Dec 01 01:28:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

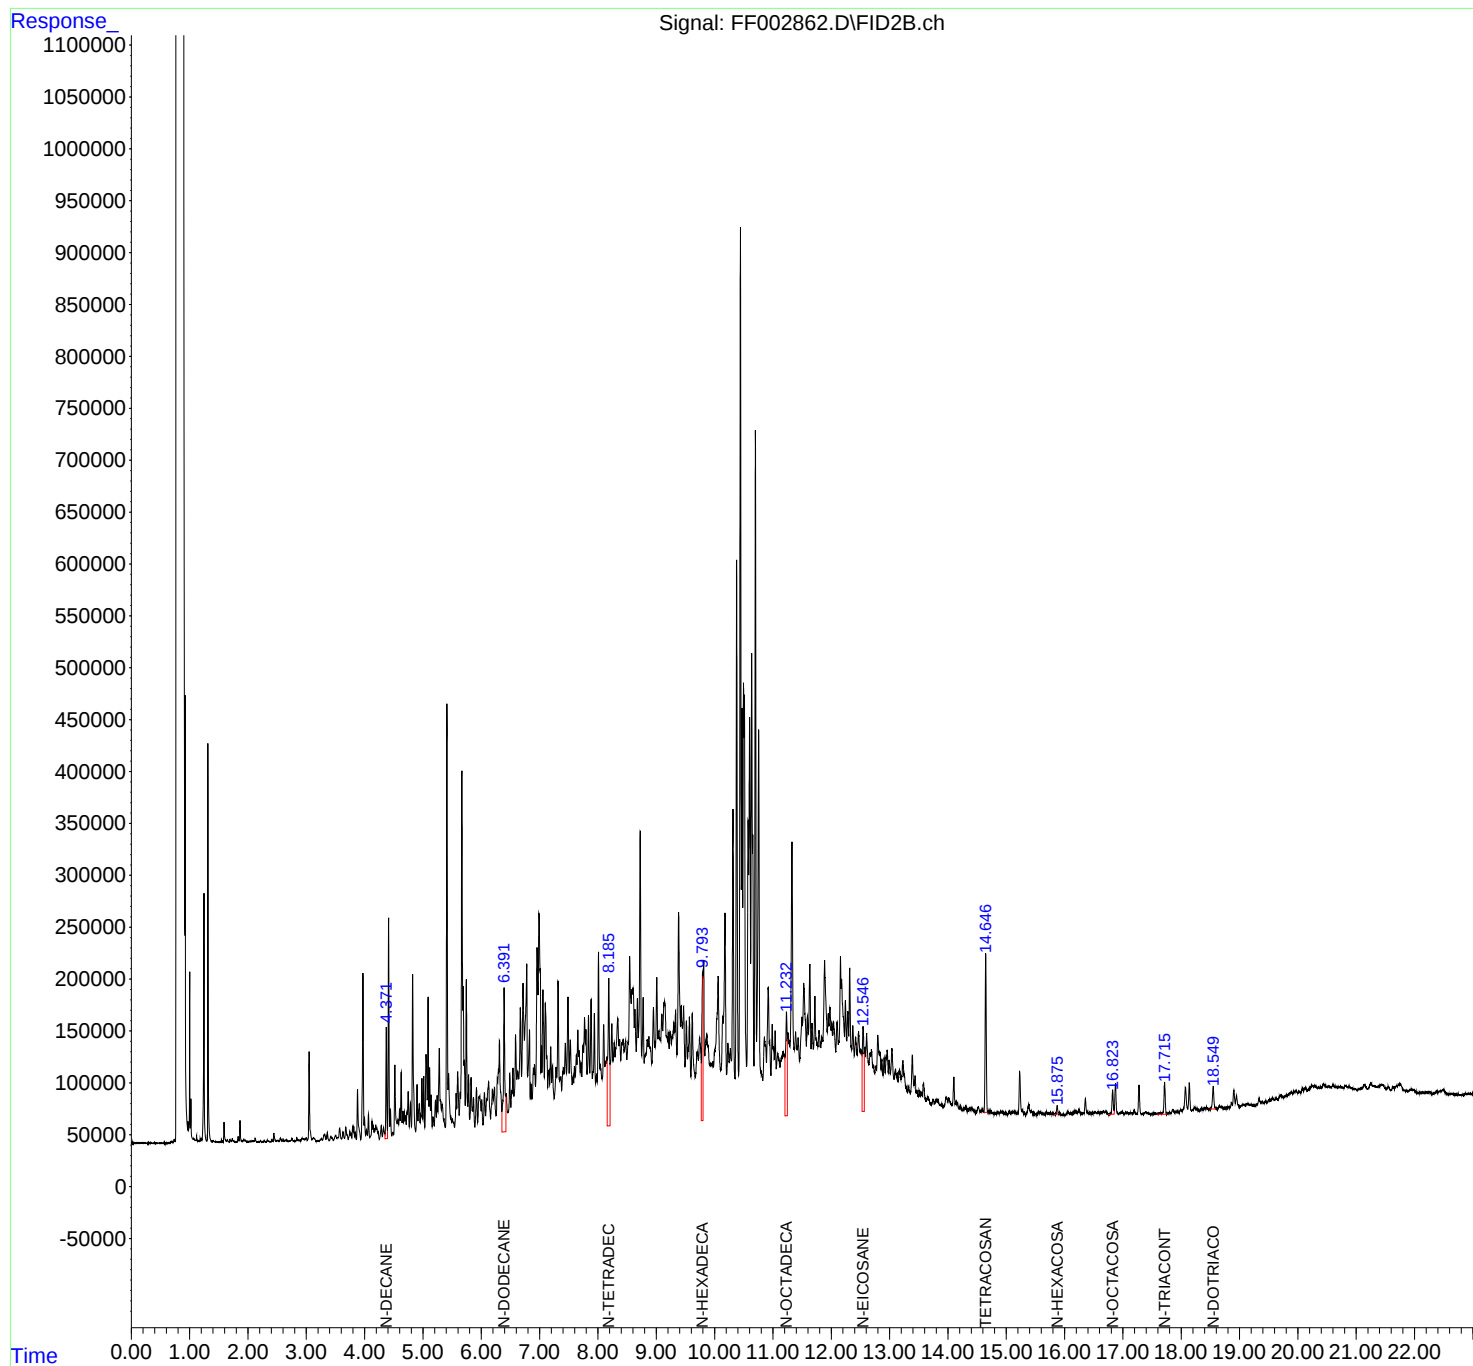


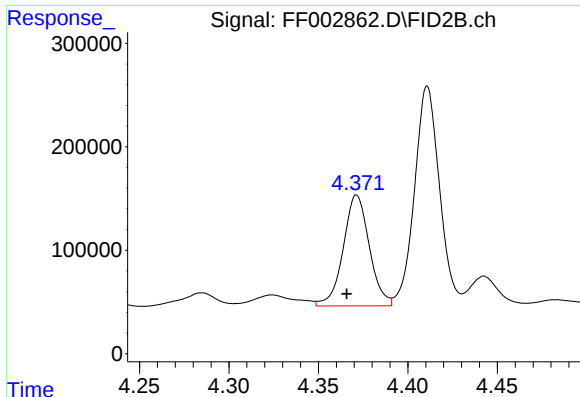

#2 N-DECANE


R.T.: 4.371 min
Delta R.T.: 0.006 min
Response: 1089097
Conc: 8.72 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-11

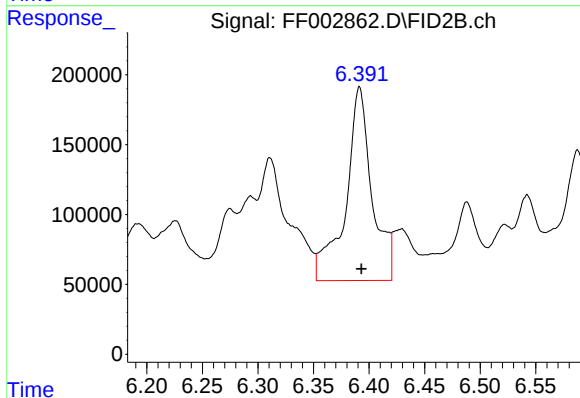


#3 N-DODECANE

R.T.: 6.391 min
Delta R.T.: -0.002 min
Response: 2281776
Conc: 18.83 ug/ml

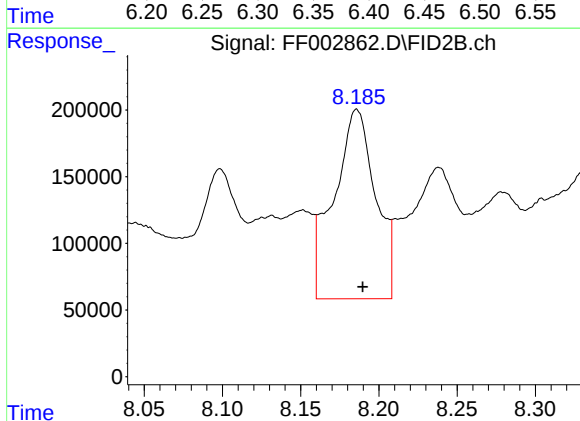


#4 N-TETRADECANE

R.T.: 8.186 min
Delta R.T.: -0.004 min
Response: 2636540
Conc: 22.82 ug/ml

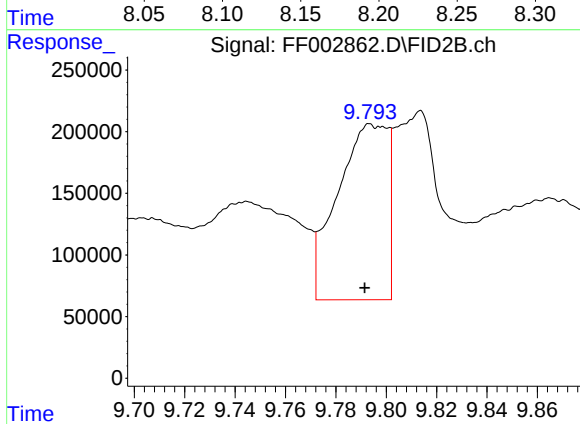

#5 N-HEXADECANE


R.T.: 9.794 min
Delta R.T.: 0.002 min
Response: 1966318
Conc: 17.98 ug/ml

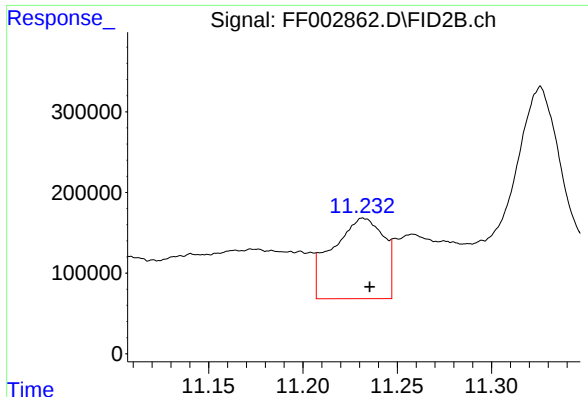

#6 N-OCTADECANE


R.T.: 11.232 min
Delta R.T.: -0.003 min
Response: 1889520
Conc: 18.20 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-11

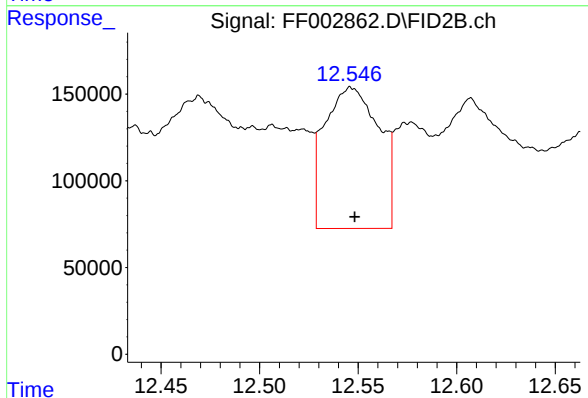


#7 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: -0.002 min
Response: 1555130
Conc: 16.06 ug/ml

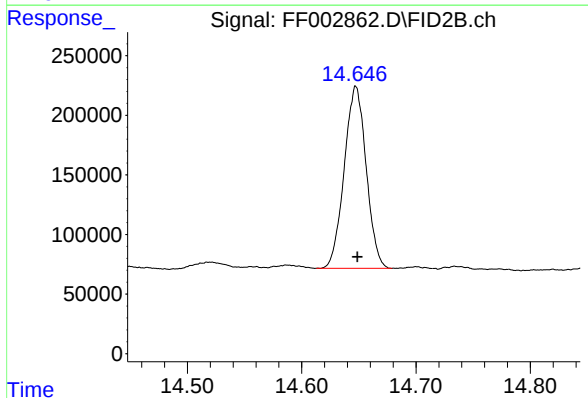


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.647 min
Delta R.T.: -0.001 min
Response: 2038318
Conc: 26.09 ug/ml

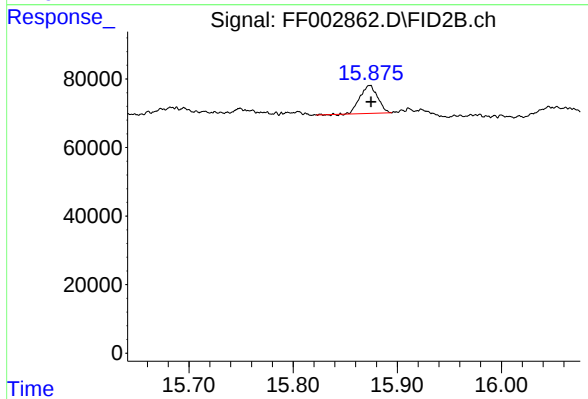

#11 N-HEXACOSANE


R.T.: 15.874 min
Delta R.T.: -0.001 min
Response: 95194
Conc: 1.05 ug/ml

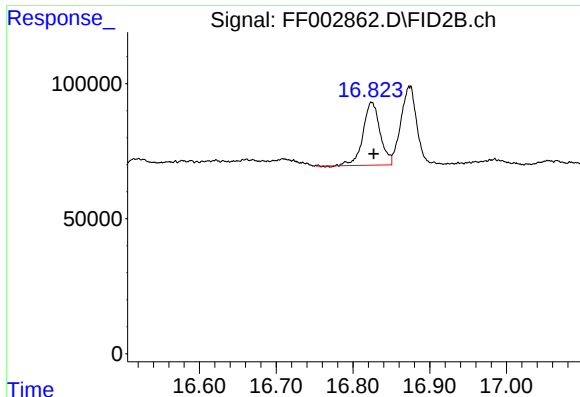

#12 N-OCTACOSANE


R.T.: 16.824 min
Delta R.T.: -0.003 min
Response: 360791
Conc: 3.78 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-11

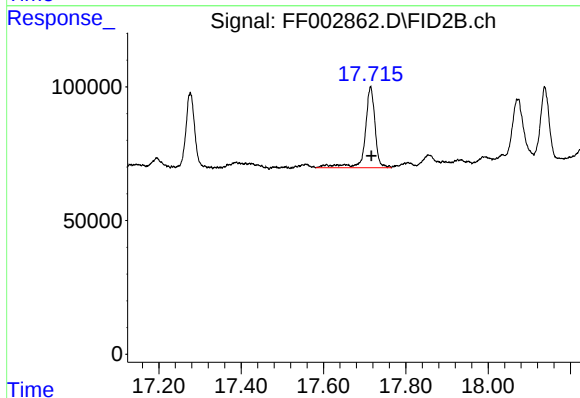

#13 N-TRIACONTANE

R.T.: 17.715 min
Delta R.T.: -0.002 min
Response: 511978
Conc: 5.16 ug/ml

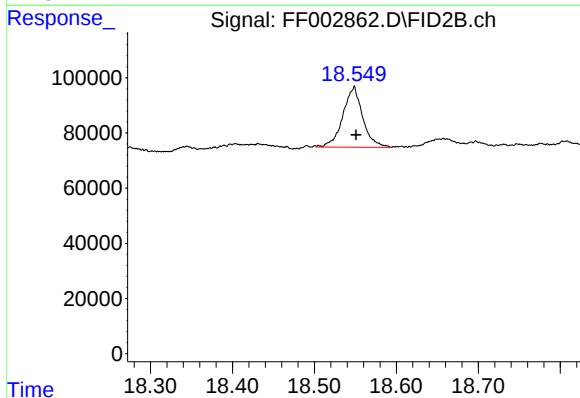

#14 N-DOTRIACONTANE

R.T.: 18.548 min
Delta R.T.: -0.002 min
Response: 367639
Conc: 3.71 ug/ml