

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002863.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 19:00
 Operator : AJ\SJ
 Sample : J6134-09
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TW-1

Integration File: autoint1.e
 Quant Time: Dec 01 01:28:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	1950851	24.974 ug/ml
Target Compounds			
2) N-DECANE	4.411	371797	2.977 ug/ml
3) N-DODECANE	6.391	185582	1.531 ug/ml
4) N-TETRADECANE	8.240f	156382	1.354 ug/ml
5) N-HEXADECANE	9.789	1196531	10.943 ug/ml
8) N-DOCOSANE	13.709	180972	1.977 ug/ml
12) N-OCTACOSANE	16.826	158686	1.664 ug/ml
13) N-TRIACONTANE	17.713	237566	2.396 ug/ml
14) N-DOTRIACONTANE	18.550	322305	3.256 ug/ml
16) N-HEXATRIACONTANE	20.123	68677	0.721 ug/ml
18) N-TETRACONTANE	21.753	390753	4.461 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002863.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 19:00
Operator : AJ\SJ
Sample : J6134-09
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TW-1

Integration File: autoint1.e
Quant Time: Dec 01 01:28:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

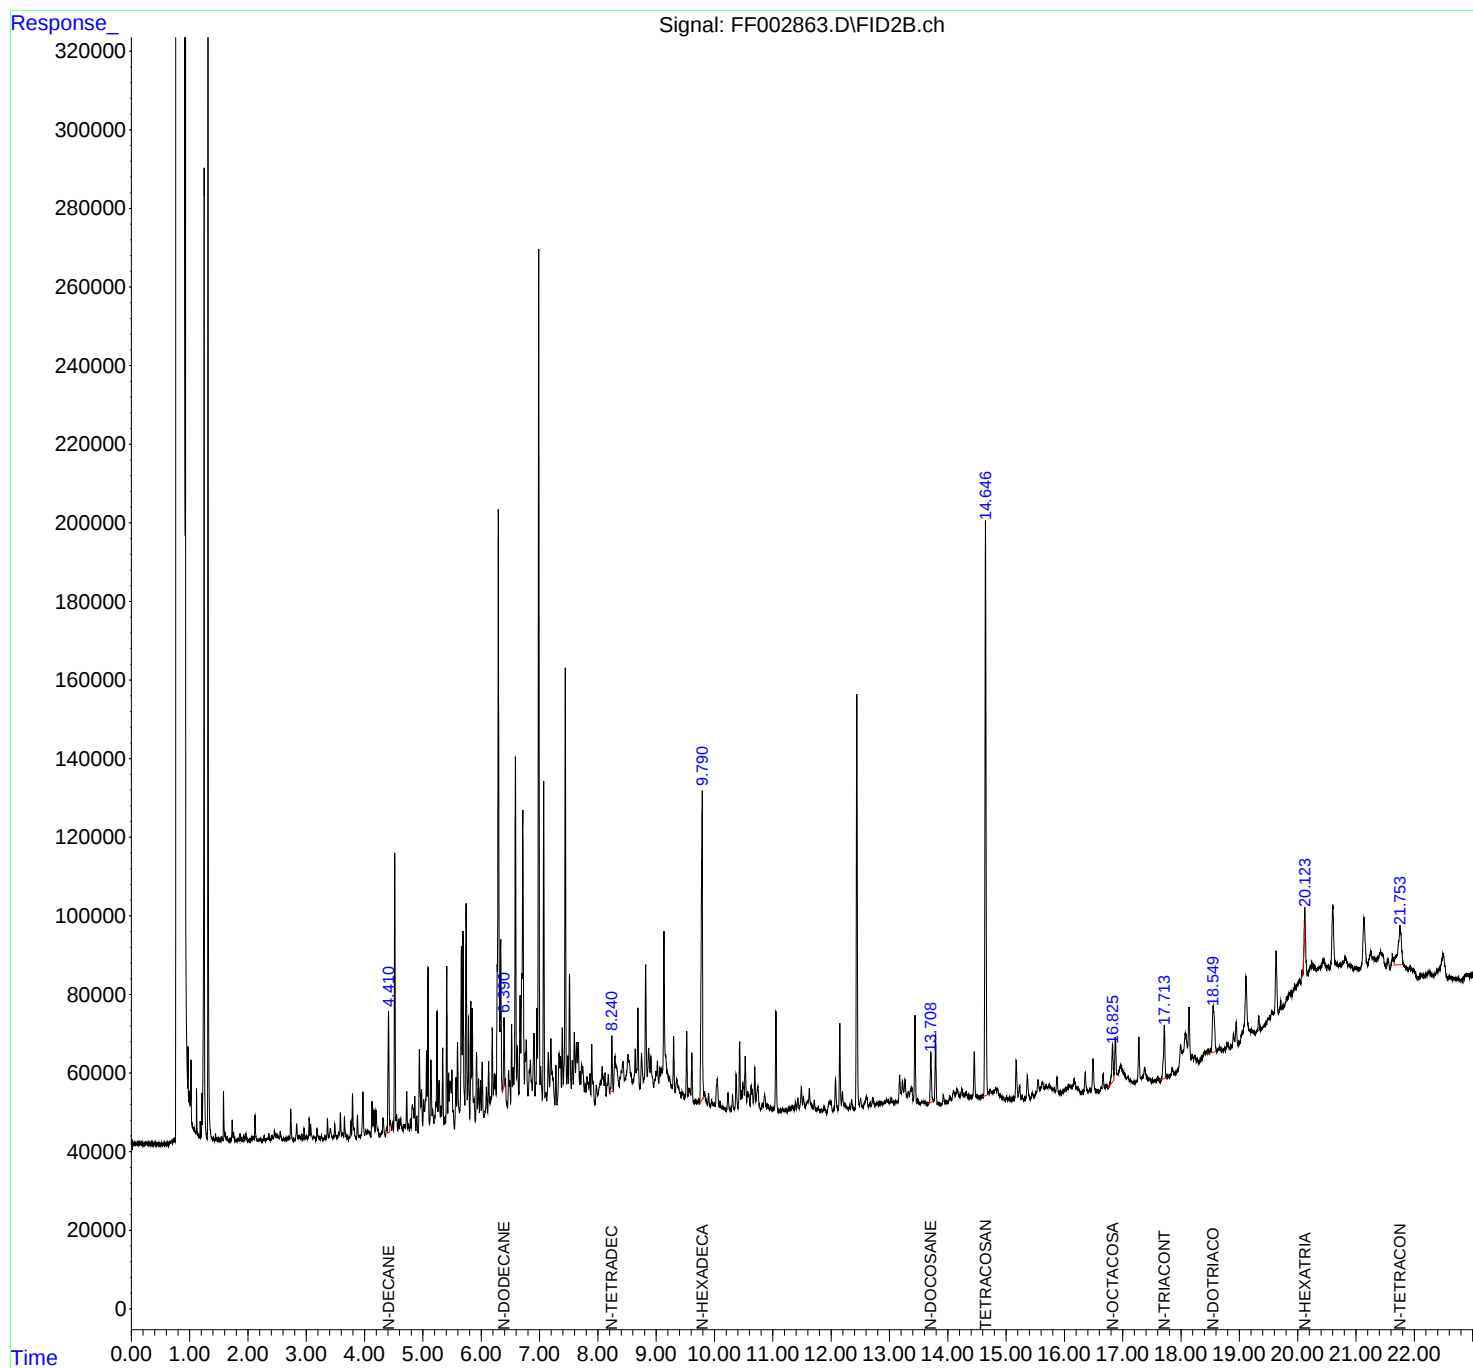


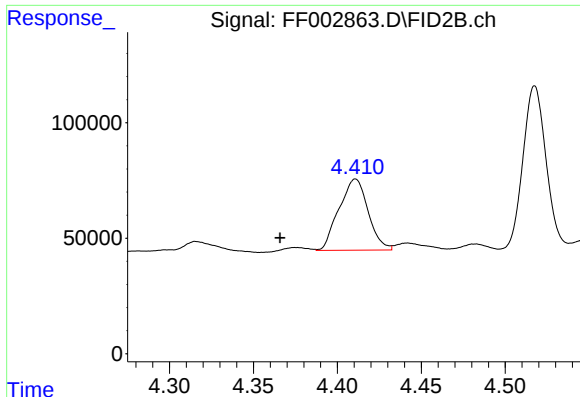

#2 N-DECANE


R.T.: 4.411 min
Delta R.T.: 0.045 min
Response: 371797
Conc: 2.98 ug/ml

Instrument :
FID_F
ClientSampleId :
TW-1

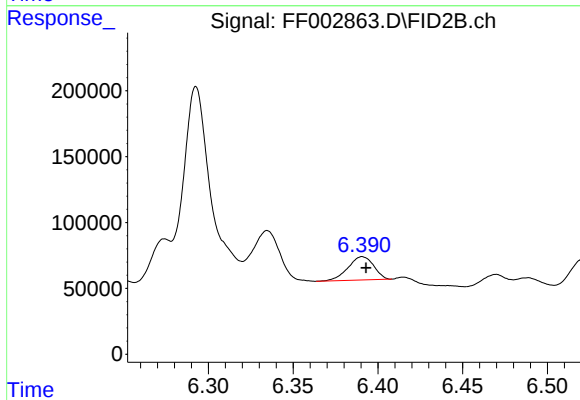


#3 N-DODECANE

R.T.: 6.391 min
Delta R.T.: -0.002 min
Response: 185582
Conc: 1.53 ug/ml

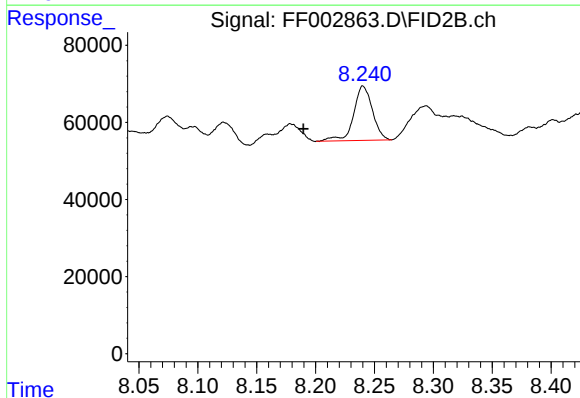


#4 N-TETRADECANE

R.T.: 8.240 min
Delta R.T.: 0.051 min
Response: 156382
Conc: 1.35 ug/ml

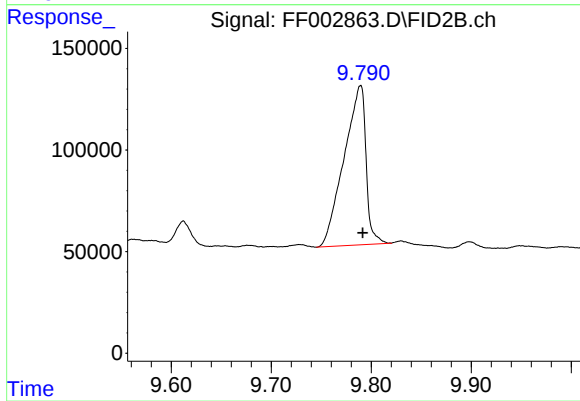

#5 N-HEXADECANE


R.T.: 9.789 min
Delta R.T.: -0.002 min
Response: 1196531
Conc: 10.94 ug/ml

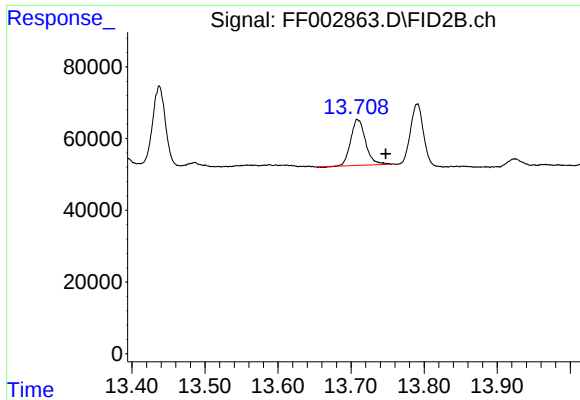

#8 N-DOCOSANE


R.T.: 13.709 min
Delta R.T.: -0.038 min
Response: 180972
Conc: 1.98 ug/ml

Instrument :
FID_F
ClientSampleId :
TW-1

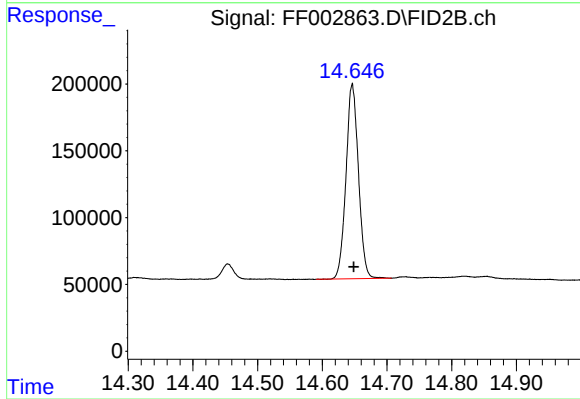


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.646 min
Delta R.T.: -0.003 min
Response: 1950851
Conc: 24.97 ug/ml

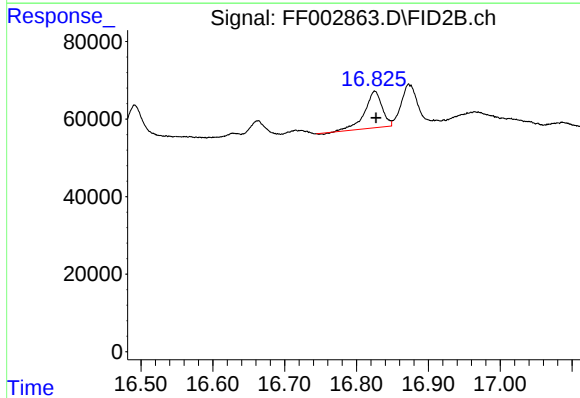


#12 N-OCTACOSANE

R.T.: 16.826 min
Delta R.T.: -0.001 min
Response: 158686
Conc: 1.66 ug/ml

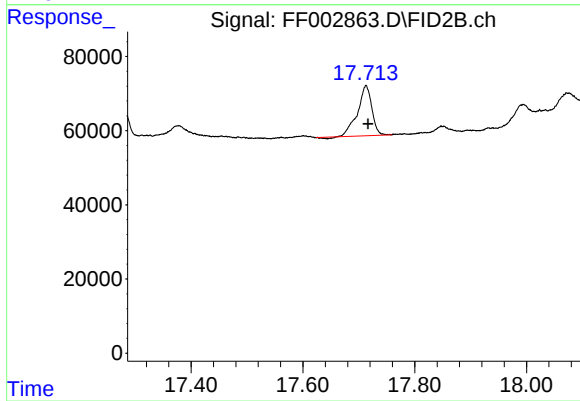

#13 N-TRIACONTANE


R.T.: 17.713 min
Delta R.T.: -0.004 min
Response: 237566
Conc: 2.40 ug/ml

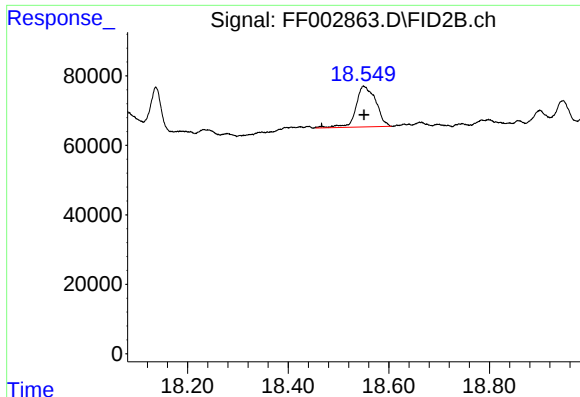

#14 N-DOTRIACONTANE


R.T.: 18.550 min
Delta R.T.: 0.000 min
Response: 322305
Conc: 3.26 ug/ml

Instrument :
FID_F
ClientSampleId :
TW-1

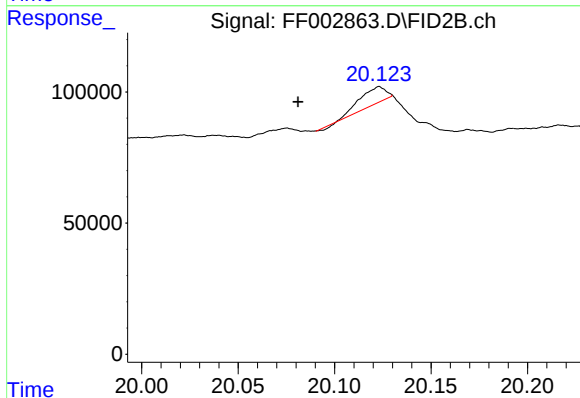

#16 N-HEXATRIACONTANE

R.T.: 20.123 min
Delta R.T.: 0.042 min
Response: 68677
Conc: 0.72 ug/ml

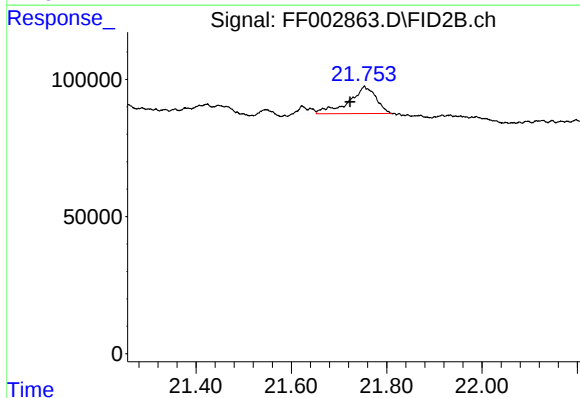

#18 N-TETRACONTANE

R.T.: 21.753 min
Delta R.T.: 0.029 min
Response: 390753
Conc: 4.46 ug/ml