

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
 Data File : FF002864.D
 Signal(s) : FID2B.ch
 Acq On : 30 Nov 2018 19:30
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Dec 01 01:29:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
 Quant Title :
 QLast Update : Wed Nov 14 13:46:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.646	1347085	17.245 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.713	169679	1.712 ug/ml
14) N-DOTRIACONTANE	18.548	223881	2.262 ug/ml
15) N-TETRATRIACONTANE	19.334	148085	1.500 ug/ml
16) N-HEXATRIACONTANE	20.125	51468	0.540 ug/ml
18) N-TETRACONTANE	21.757	465760	5.317 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF113018\
Data File : FF002864.D
Signal(s) : FID2B.ch
Acq On : 30 Nov 2018 19:30
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Dec 01 01:29:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF111418.M
Quant Title :
QLast Update : Wed Nov 14 13:46:00 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

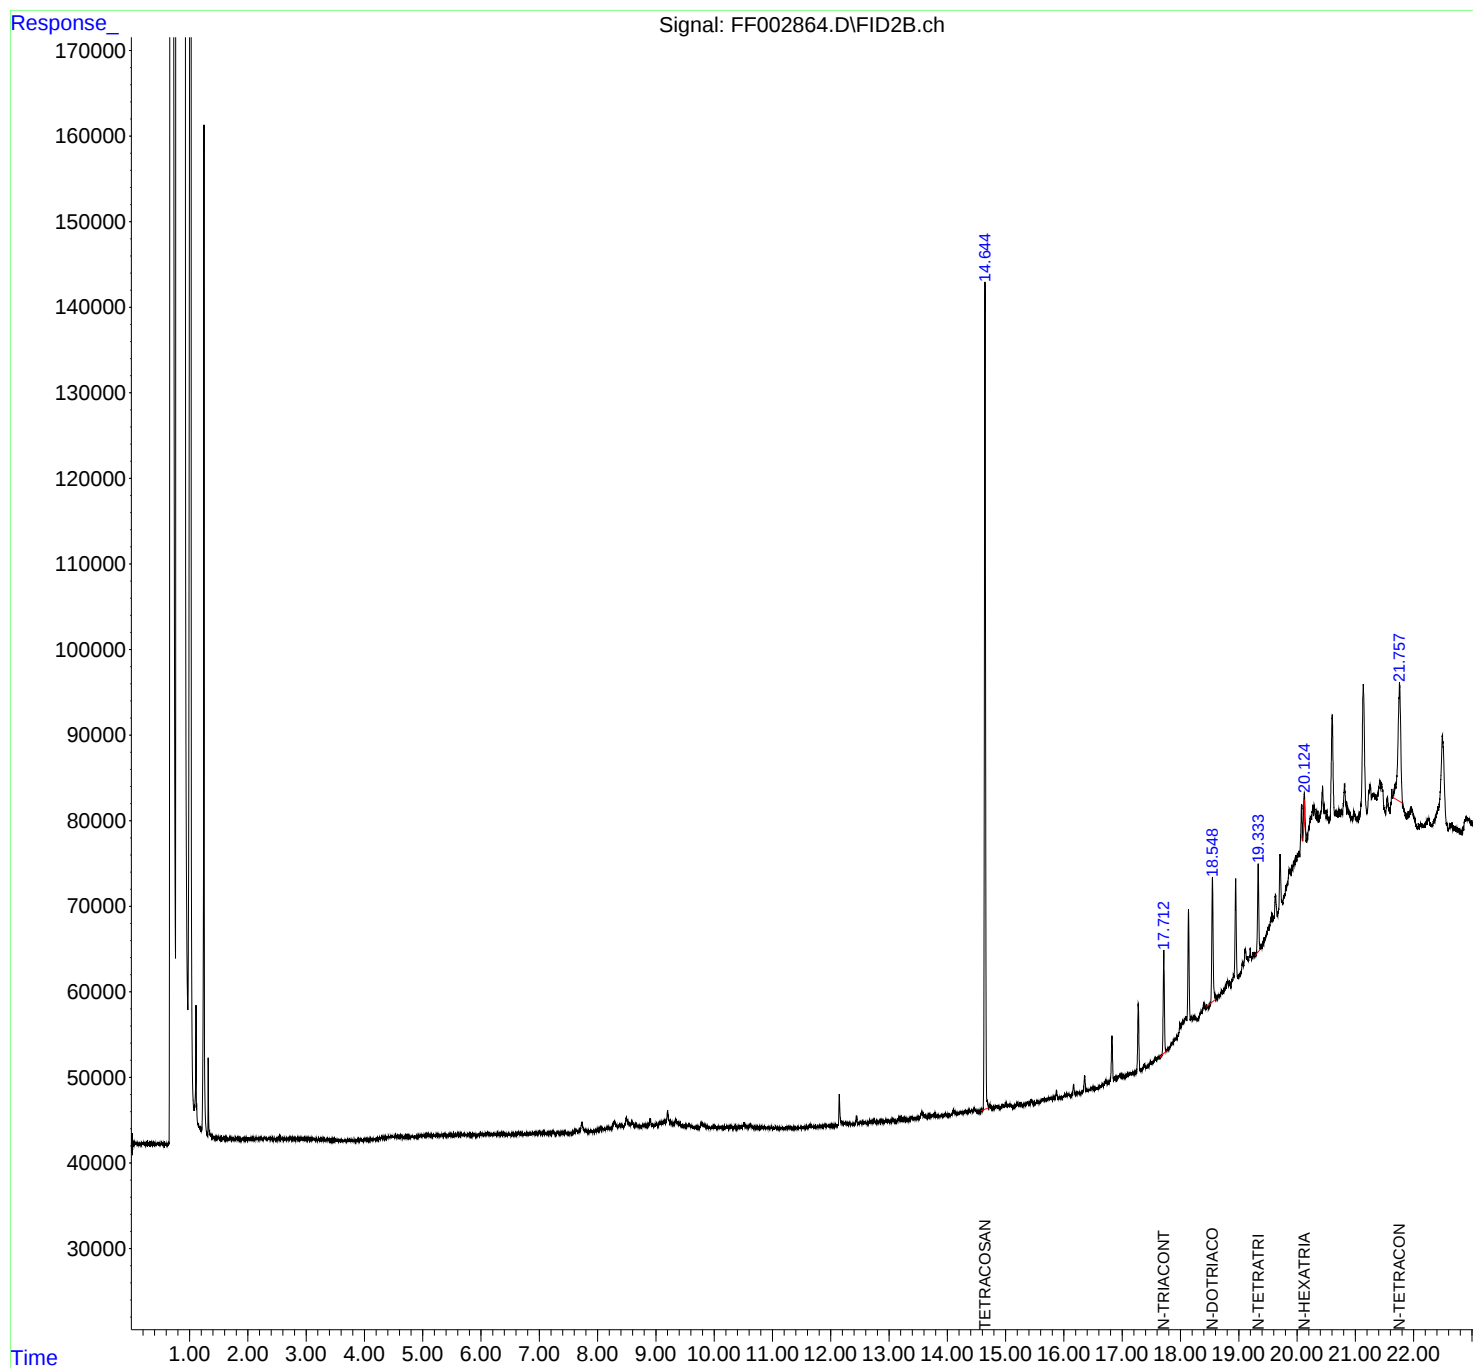


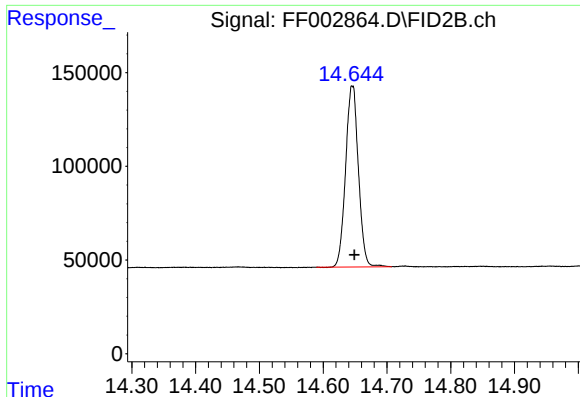

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.646 min
Delta R.T.: -0.003 min
Response: 1347085
Conc: 17.24 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

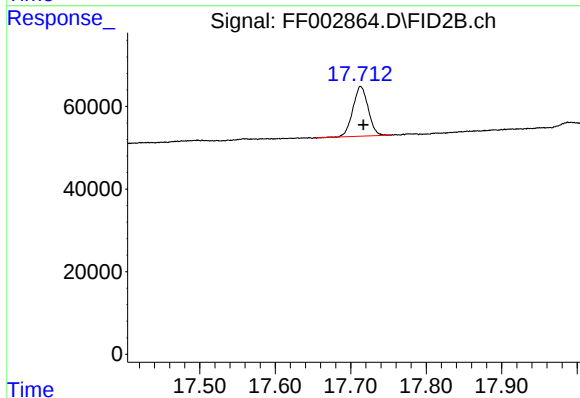


#13 N-TRIACONTANE

R.T.: 17.713 min
Delta R.T.: -0.004 min
Response: 169679
Conc: 1.71 ug/ml

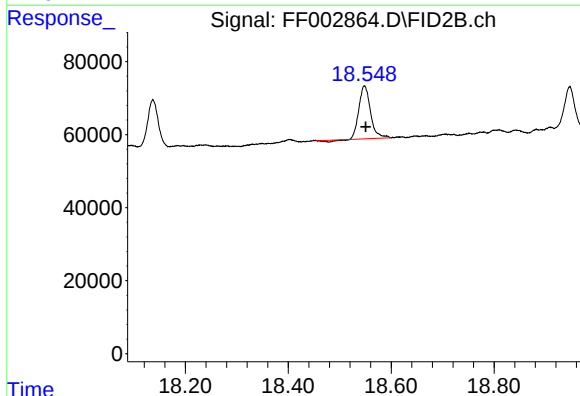


#14 N-DOTRIACONTANE

R.T.: 18.548 min
Delta R.T.: -0.003 min
Response: 223881
Conc: 2.26 ug/ml

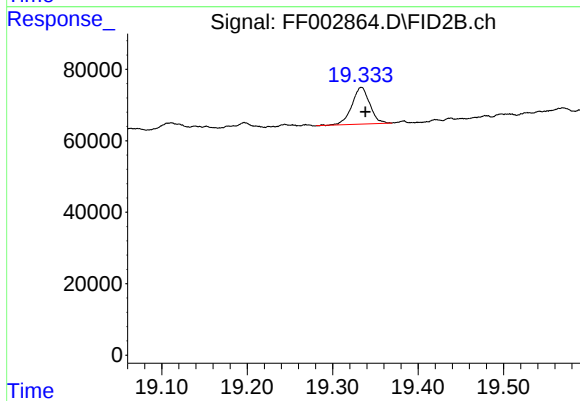

#15 N-TETRATRIACONTANE


R.T.: 19.334 min
Delta R.T.: -0.005 min
Response: 148085
Conc: 1.50 ug/ml

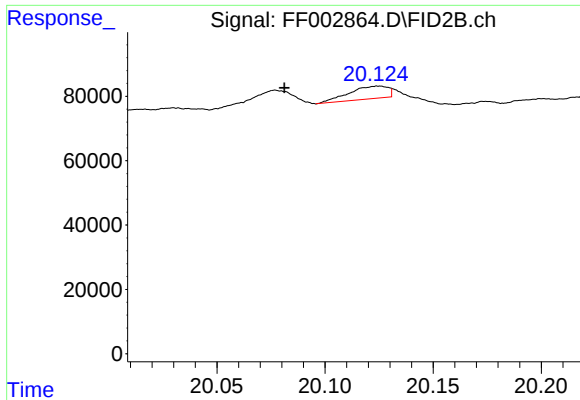

#16 N-HEXATRIACONTANE

R.T.: 20.125 min
Delta R.T.: 0.044 min
Response: 51468
Conc: 0.54 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

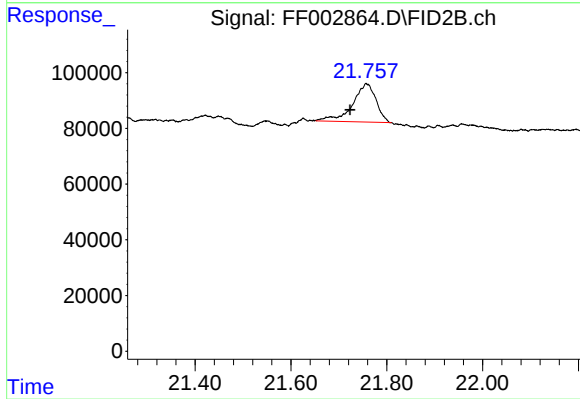

#18 N-TETRACONTANE

R.T.: 21.757 min
Delta R.T.: 0.034 min
Response: 465760
Conc: 5.32 ug/ml